

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090923\
 Data File : PD077782.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2023 12:52
 Operator : AR\AJ
 Sample : PIBLK263
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 22:51:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.760	58827682	35394603	23.181	23.950
27)	SA Decachlor...	9.081	7.898	133.9E6	76214115	42.870	47.060
Target Compounds							
2)	A alpha-BHC	3.949f	0.000	550686	0	0.129	N.D. #
3)	MA gamma-BHC...	0.000	3.602	0	103018	N.D.	<MDL
6)	B beta-BHC	0.000	3.844f	0	904669	N.D.	0.916
8)	B Heptachlo...	5.687	0.000	3219674	0	0.833	N.D. #
9)	A Endosulfan I	0.000	5.132f	0	815515	N.D.	0.454
14)	MA Endrin	0.000	5.640	0	575659	N.D.	0.315
23)	Toxaphene-2	0.000	5.640	0	575659	N.D.	47.737

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090923\
Data File : PD077782.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2023 12:52
Operator : AR\AJ
Sample : PIBLK263
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 22:51:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

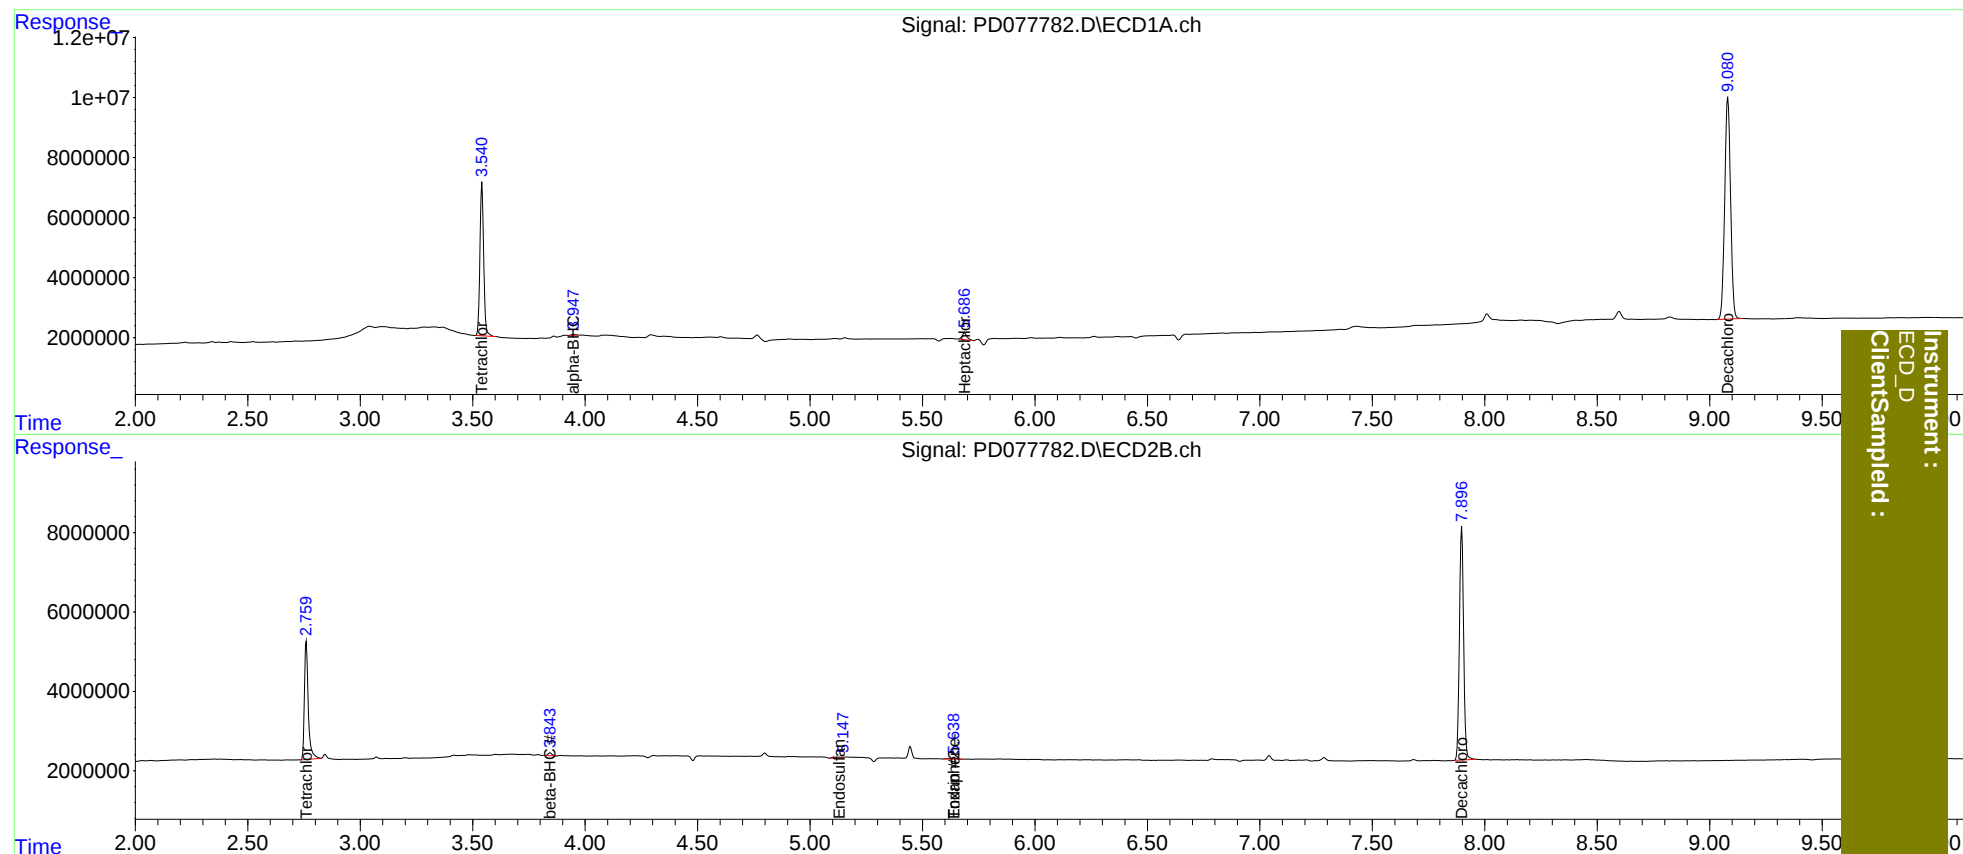


Instrument :
ECD_D
ClientSampled :
0

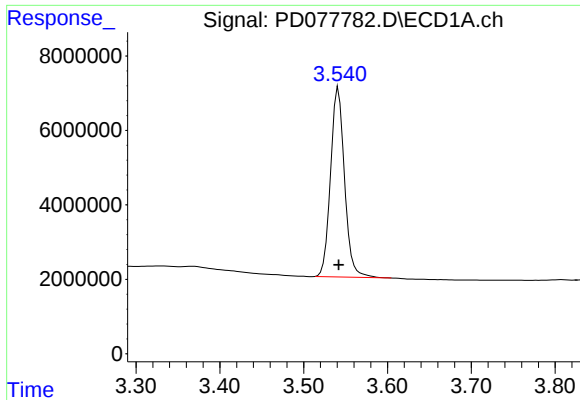

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.000 min
Response: 58827682
Conc: 23.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

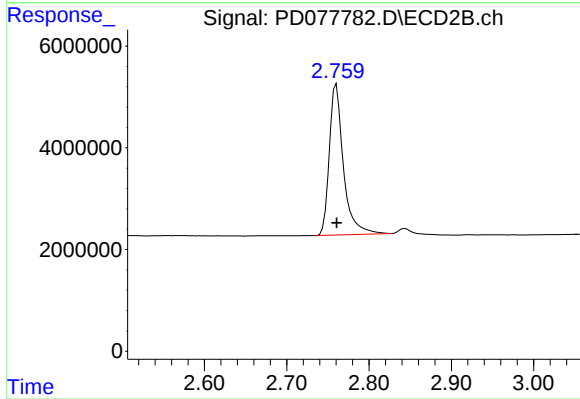


#1 Tetrachloro-m-xylene

R.T.: 2.760 min
Delta R.T.: 0.000 min
Response: 35394603
Conc: 23.95 ng/ml

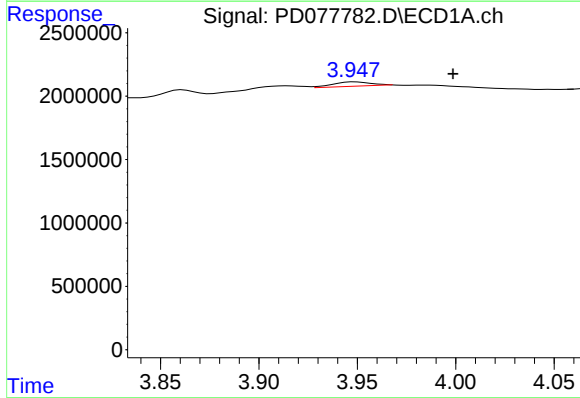


#2 alpha-BHC

R.T.: 3.949 min
Delta R.T.: -0.049 min
Response: 550686
Conc: 0.13 ng/ml

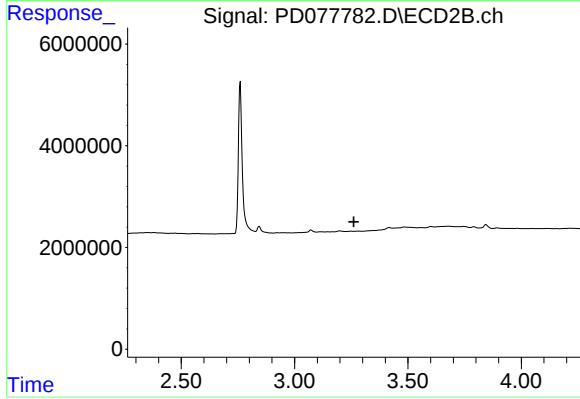

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 3.262 min
Response: 0
Conc: N.D.

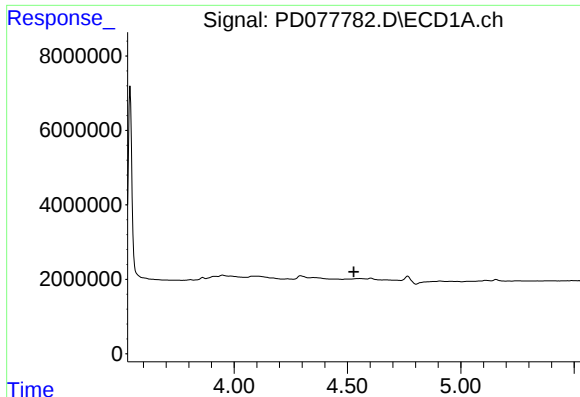

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.528 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

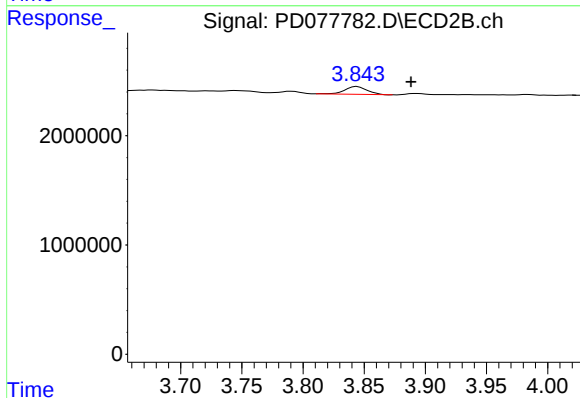


#6 beta-BHC

R.T.: 3.844 min
Delta R.T.: -0.044 min
Response: 904669
Conc: 0.92 ng/ml

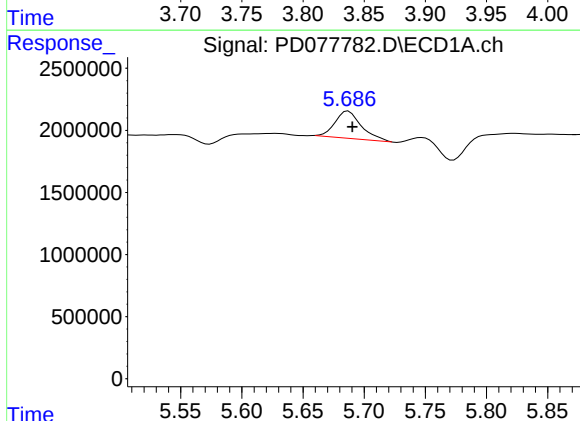


#8 Heptachlor epoxide

R.T.: 5.687 min
Delta R.T.: -0.003 min
Response: 3219674
Conc: 0.83 ng/ml

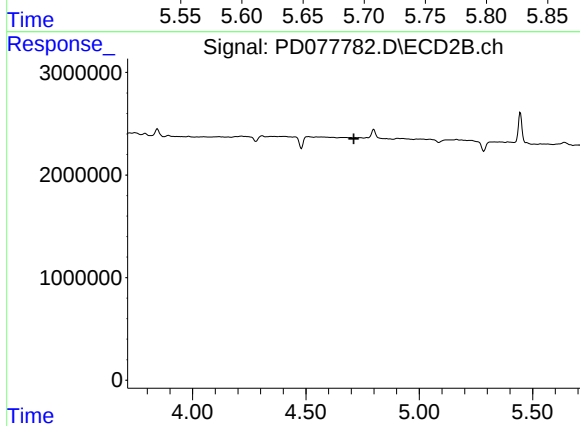

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.712 min
Response: 0
Conc: N.D.

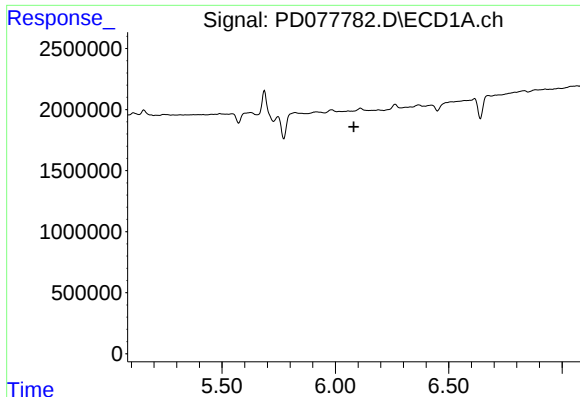

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.081 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

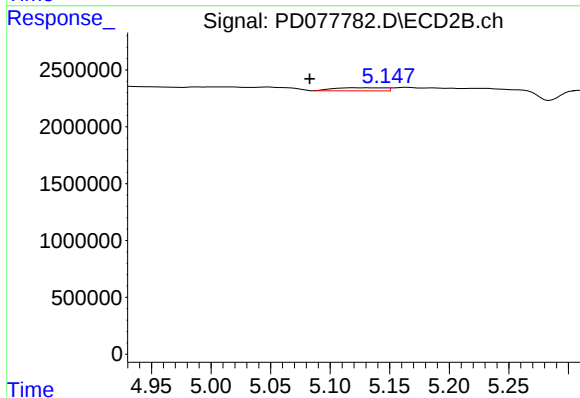


#9 Endosulfan I

R.T.: 5.132 min
Delta R.T.: 0.049 min
Response: 815515
Conc: 0.45 ng/ml

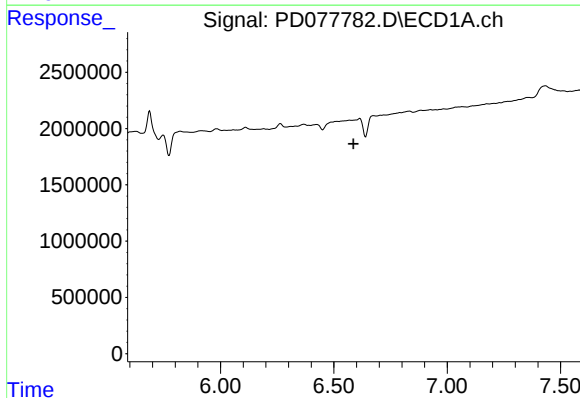


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.587 min
Response: 0
Conc: N.D.

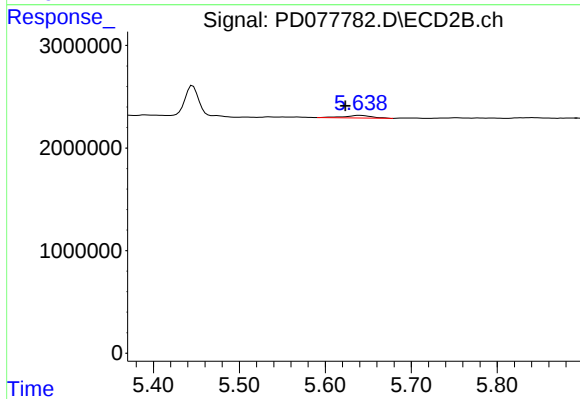

#14 Endrin


R.T.: 5.640 min
Delta R.T.: 0.016 min
Response: 575659
Conc: 0.31 ng/ml

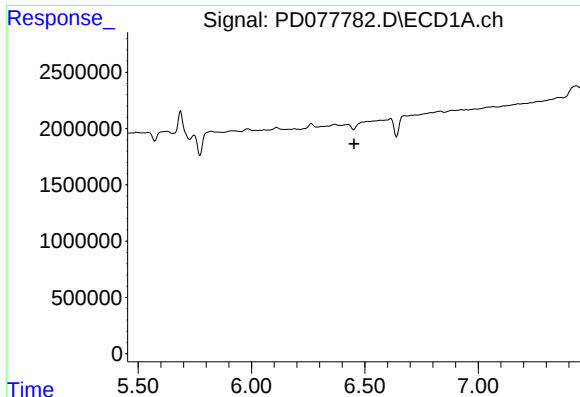

#23 Toxaphene-2


R.T.: 0.000 min
Exp R.T.: 6.452 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

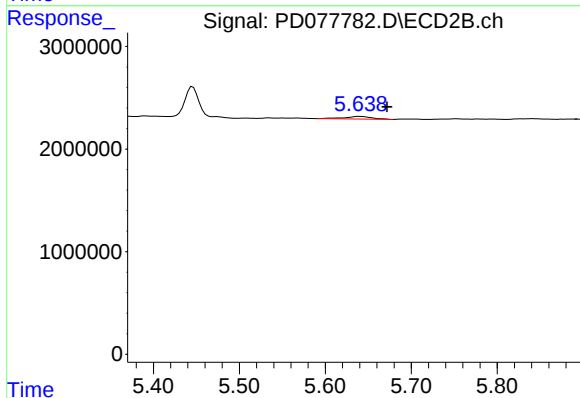


#23 Toxaphene-2

R.T.: 5.640 min
Delta R.T.: -0.032 min
Response: 575659
Conc: 47.74 ng/ml

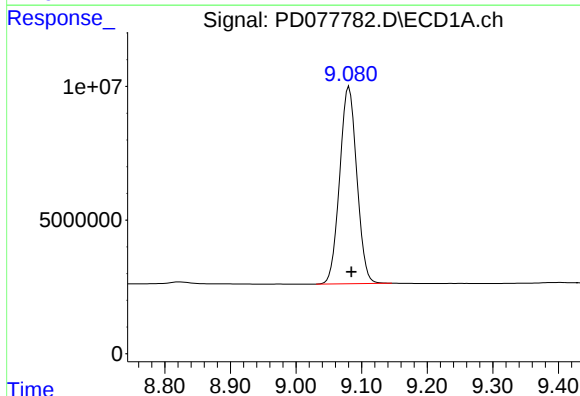

#27 Decachlorobiphenyl

R.T.: 9.081 min
Delta R.T.: -0.004 min
Response: 133922040
Conc: 42.87 ng/ml

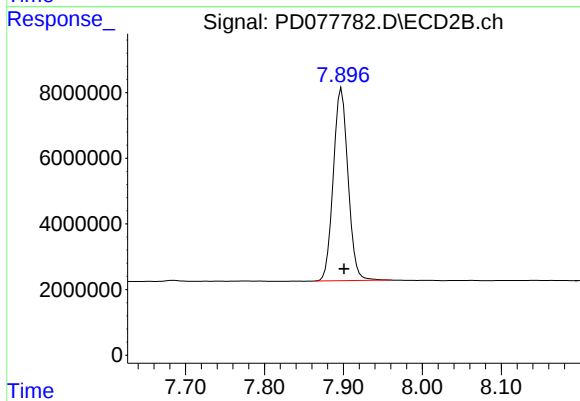

#27 Decachlorobiphenyl

R.T.: 7.898 min
Delta R.T.: -0.003 min
Response: 76214115
Conc: 47.06 ng/ml