

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090923\
 Data File : PD077814.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2023 21:45
 Operator : AR\AJ
 Sample : 04280-03
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 23:03:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.761	53022214	32099564	20.894	21.720
27)	SA Decachlor...	9.079	7.897	68924307	36733153	22.064	22.682
Target Compounds							
3)	MA gamma-BHC...	4.305f	3.602	2017012	115764	0.499	<MDL #
6)	B beta-BHC	0.000	3.846f	0	4280841	N.D.	4.332
7)	B delta-BHC	4.768	0.000	6478975	0	1.614	N.D. #
9)	A Endosulfan I	0.000	5.125f	0	125567	N.D.	<MDL
10)	B trans-Chl...	0.000	5.001f	0	990390	N.D.	0.496
11)	B cis-Chlor...	0.000	5.001	0	990390	N.D.	0.484
15)	B Endosulfa...	0.000	5.943	0	761958	N.D.	0.421
21)	B Endrin ke...	0.000	6.872f	0	186178	N.D.	<MDL
22)	Toxaphene-1	0.000	5.001	0	990390	N.D.	94.885
24)	Toxaphene-3	0.000	5.943	0	761958	N.D.	55.869


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090923\
Data File : PD077814.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2023 21:45
Operator : AR\AJ
Sample : 04280-03
Misc :
ALS Vial : 48 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 23:03:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

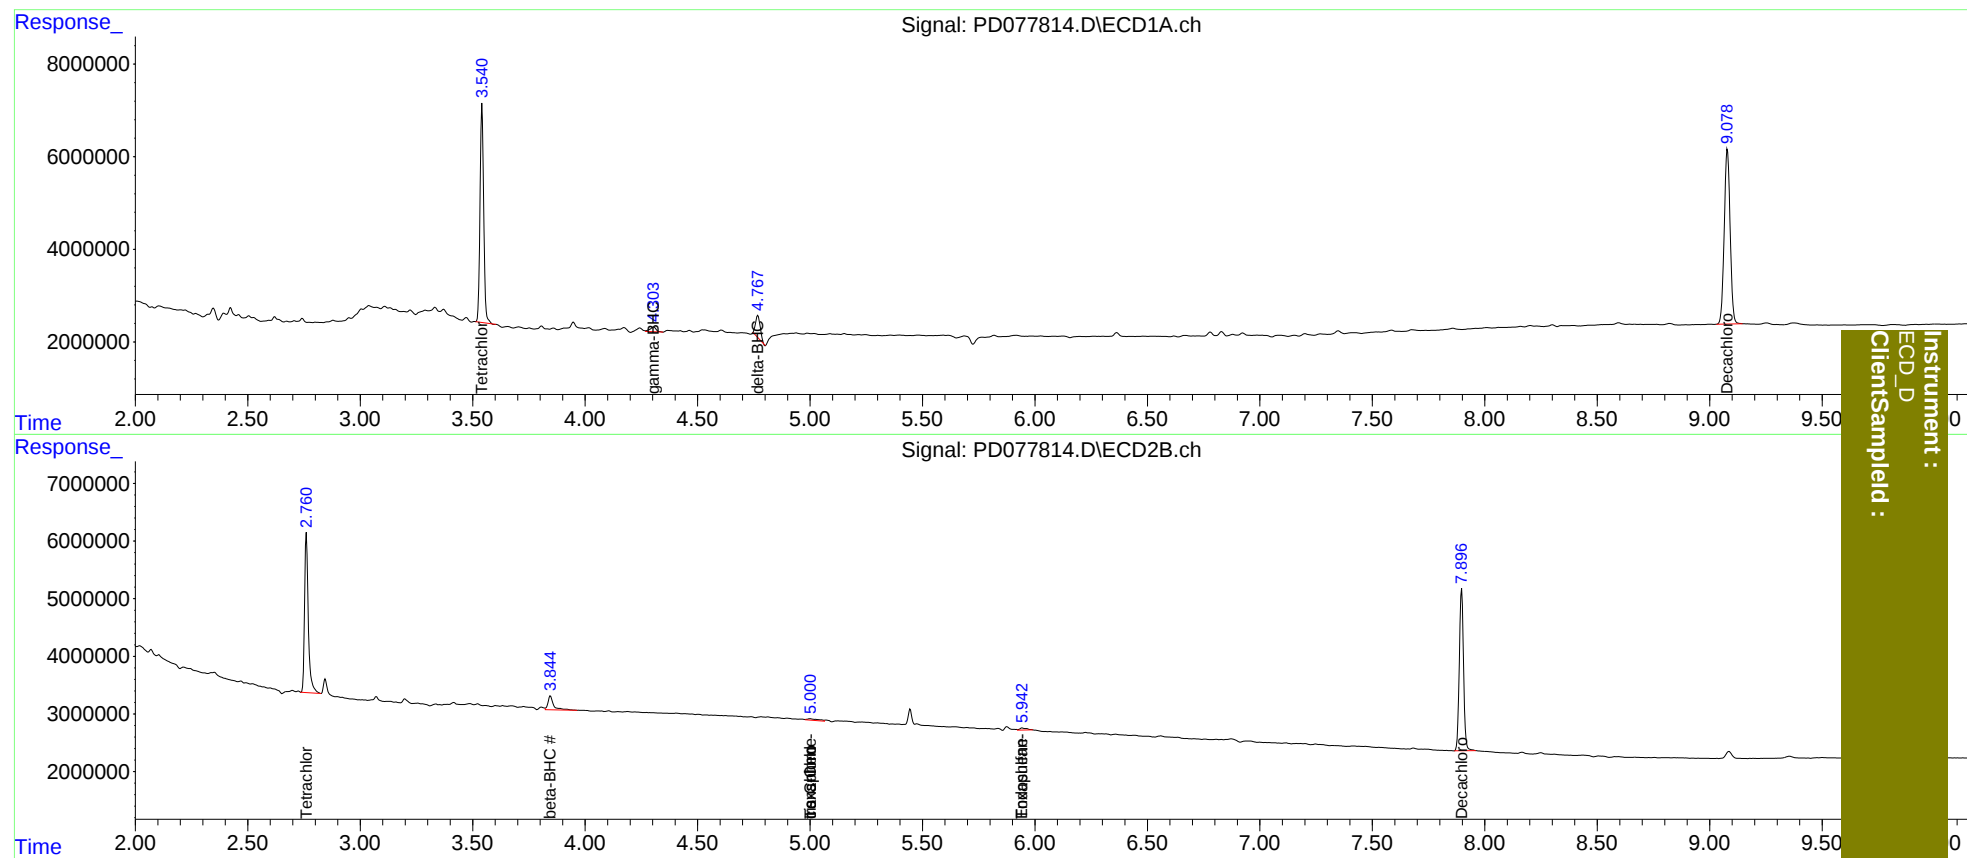


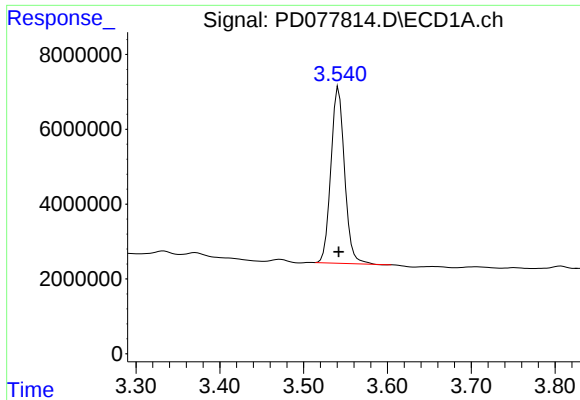

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.000 min
Response: 53022214
Conc: 20.89 ng/ml

Instrument :
ECD_D
ClientSampleId :

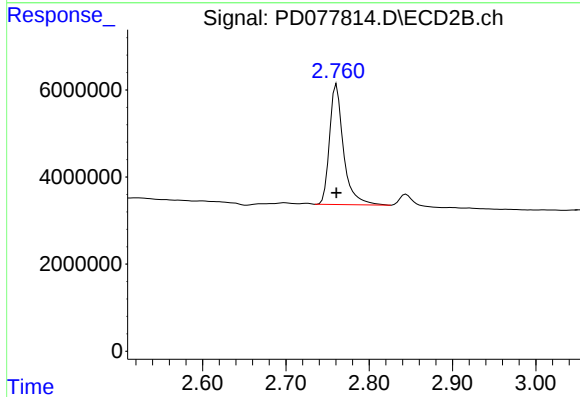


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: 0.000 min
Response: 32099564
Conc: 21.72 ng/ml

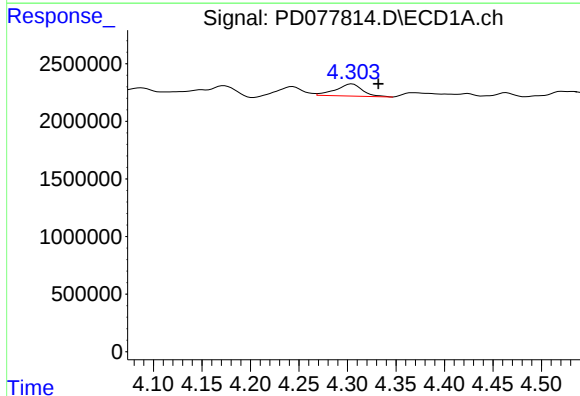


#3 gamma-BHC (Lindane)

R.T.: 4.305 min
Delta R.T.: -0.027 min
Response: 2017012
Conc: 0.50 ng/ml

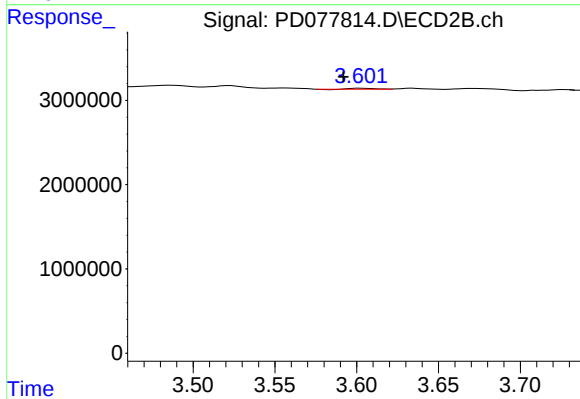

#3 gamma-BHC (Lindane)


R.T.: 3.602 min
Delta R.T.: 0.011 min
Response: 115764
Conc: N.D.

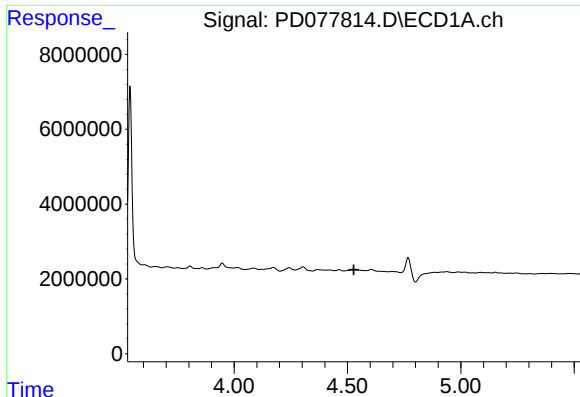

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.528 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

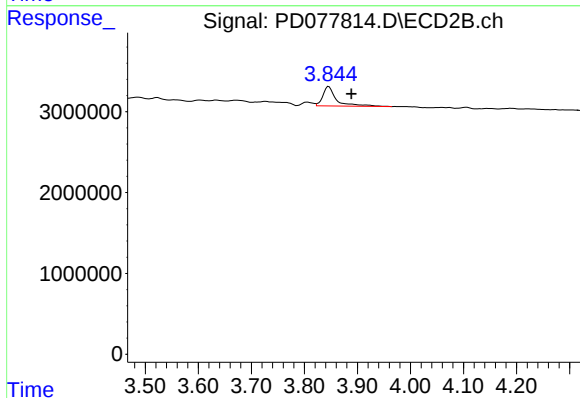


#6 beta-BHC

R.T.: 3.846 min
Delta R.T.: -0.043 min
Response: 4280841
Conc: 4.33 ng/ml

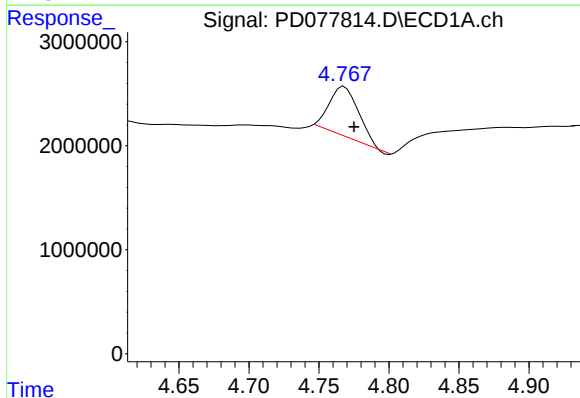


#7 delta-BHC

R.T.: 4.768 min
Delta R.T.: -0.007 min
Response: 6478975
Conc: 1.61 ng/ml

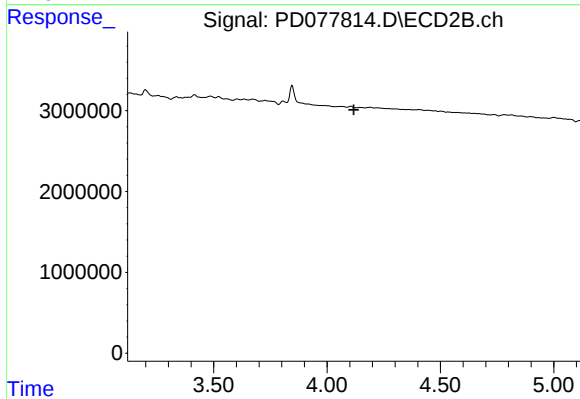

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.118 min
Response: 0
Conc: N.D.

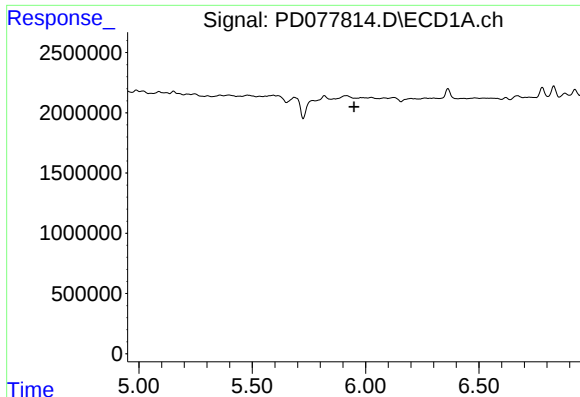

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.949 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

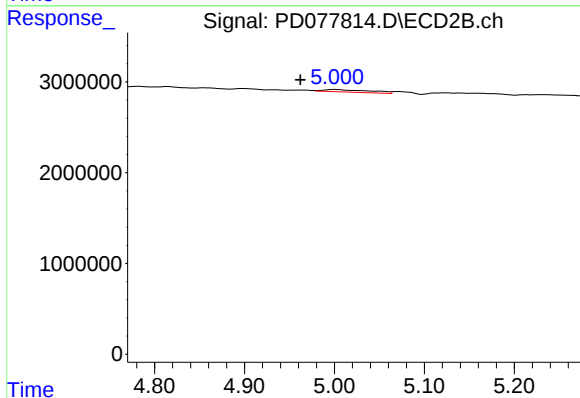


#10 trans-Chlordane

R.T.: 5.001 min
Delta R.T.: 0.039 min
Response: 990390
Conc: 0.50 ng/ml

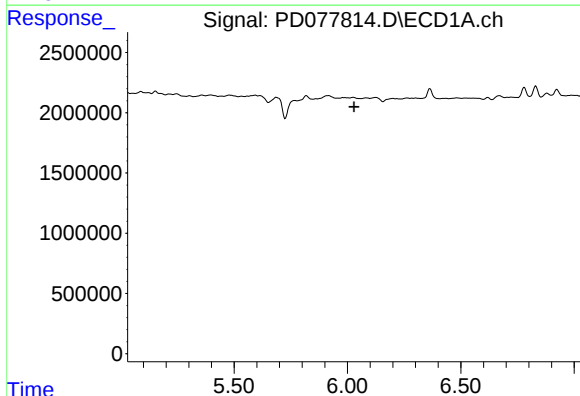


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 6.029 min
Response: 0
Conc: N.D.

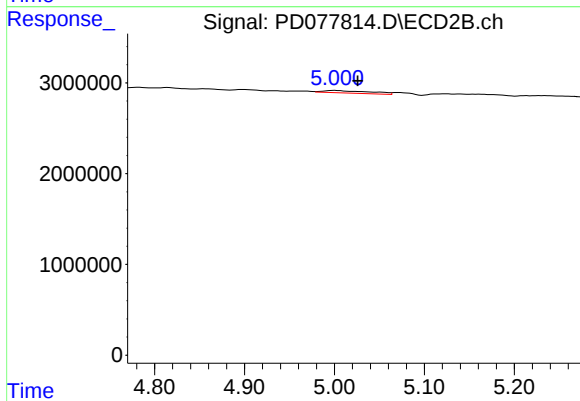

#11 cis-Chlordane


R.T.: 5.001 min
Delta R.T.: -0.025 min
Response: 990390
Conc: 0.48 ng/ml

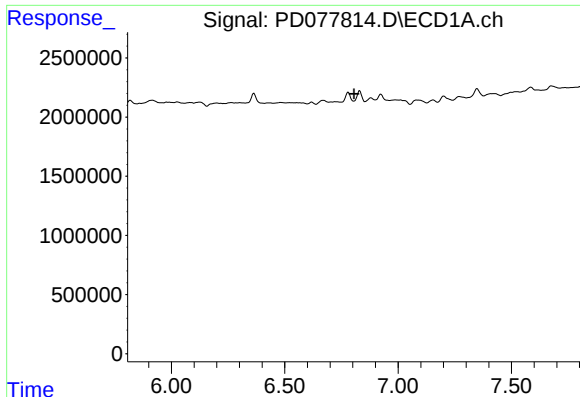

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.806 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

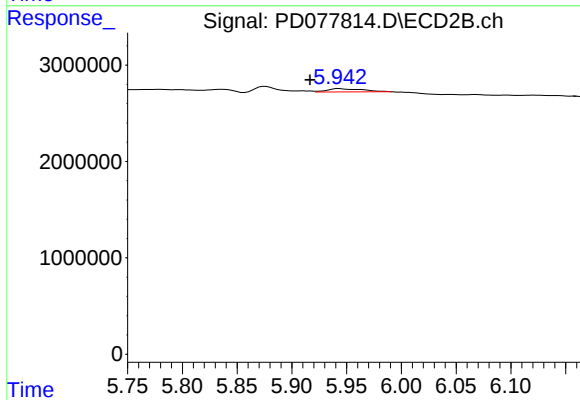


#15 Endosulfan II

R.T.: 5.943 min
Delta R.T.: 0.026 min
Response: 761958
Conc: 0.42 ng/ml

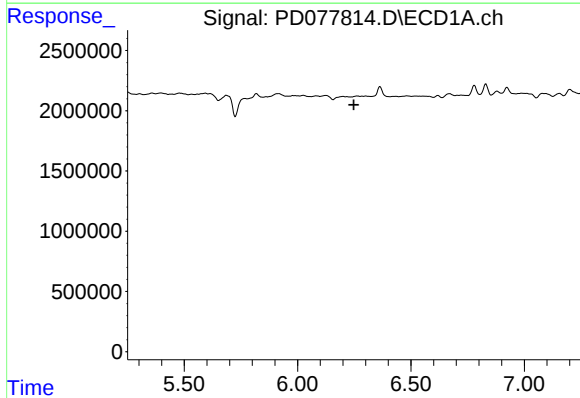


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T.: 6.247 min
Response: 0
Conc: N.D.

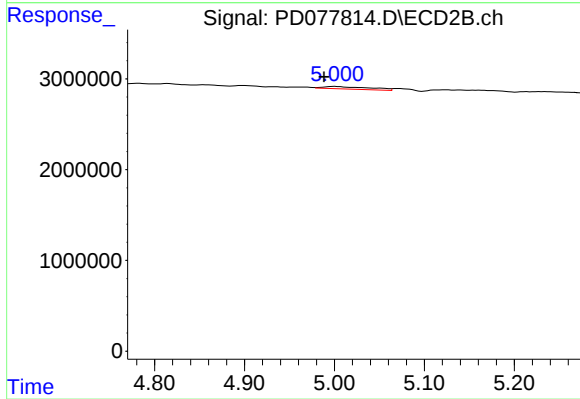

#22 Toxaphene-1


R.T.: 5.001 min
Delta R.T.: 0.012 min
Response: 990390
Conc: 94.89 ng/ml

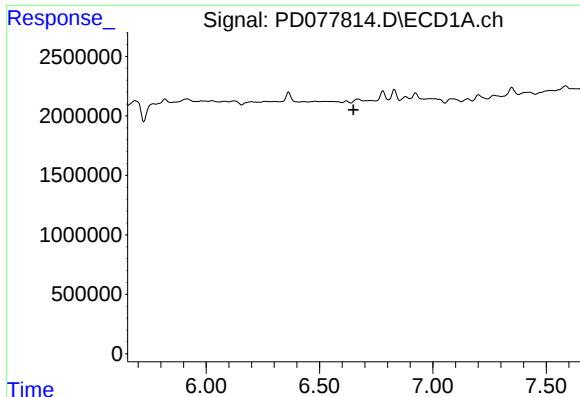

#24 Toxaphene-3


R.T.: 0.000 min
Exp R.T.: 6.650 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

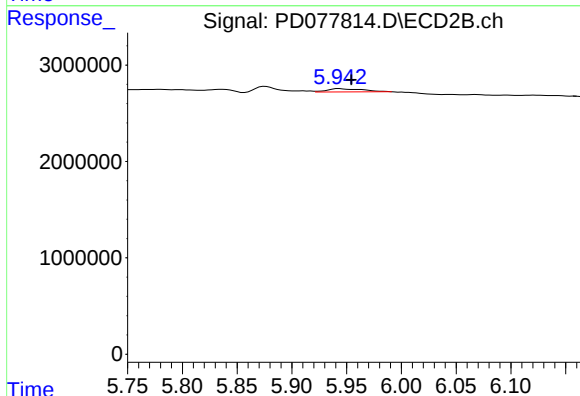


#24 Toxaphene-3

R.T.: 5.943 min
Delta R.T.: -0.011 min
Response: 761958
Conc: 55.87 ng/ml

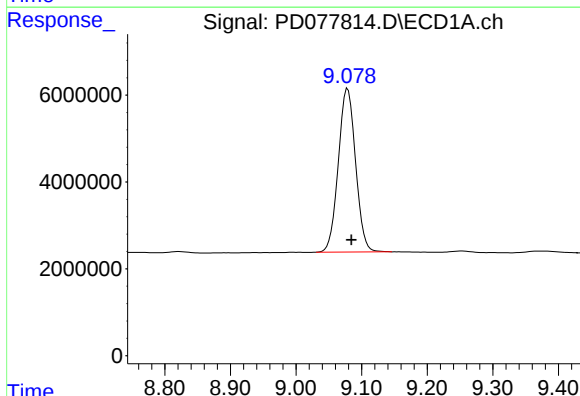

#27 Decachlorobiphenyl

R.T.: 9.079 min
Delta R.T.: -0.006 min
Response: 68924307
Conc: 22.06 ng/ml

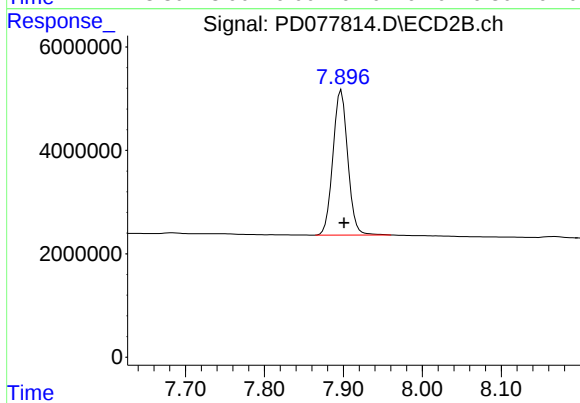

#27 Decachlorobiphenyl

R.T.: 7.897 min
Delta R.T.: -0.004 min
Response: 36733153
Conc: 22.68 ng/ml