

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090923\
 Data File : PD077793.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2023 16:56
 Operator : AR\AJ
 Sample : 04306-10MS
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH4K6MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/11/2023
 Supervised By : Ankita Jodhani 09/11/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 22:56:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.761	55363560	32128878	21.816	21.740
27)	SA Decachlor...	9.081	7.899	64459824	35731721	20.634	22.063
Target Compounds							
2)	A alpha-BHC	3.999	3.262	258.2E6	141.5E6	60.295	62.441
3)	MA gamma-BHC...	4.332	3.591	242.1E6	128.3E6	59.875	59.435
4)	MA Heptachlor	4.923	3.930	238.7E6	133.6E6	57.130	60.074
5)	MB Aldrin	5.265	4.210	241.4E6	131.1E6	57.824	58.493
6)	B beta-BHC	4.529	3.888	88351033	52093004	48.091	52.721
7)	B delta-BHC	4.778	4.118	231.3E6	130.9E6	57.611	58.747
8)	B Heptachlo...	5.693	4.712	188.7E6	119.0E6	48.834m	56.669
9)	A Endosulfan I	6.080	5.082	196.5E6	118.7E6	58.530	66.156
10)	B trans-Chl...	5.949	4.962	209.6E6	118.9E6	56.307	59.558
11)	B cis-Chlor...	6.029	5.026	208.9E6	118.1E6	54.198	57.769
12)	B 4,4'-DDE	6.201	5.215	410.7E6	233.4E6	115.856	122.873
13)	MA Dieldrin	6.355	5.346	441.6E6	254.3E6	117.988	123.081
14)	MA Endrin	6.586	5.622	372.2E6	225.7E6	120.640	123.421
15)	B Endosulfa...	6.806	5.917	362.3E6	213.1E6	109.419	117.736
16)	A 4,4'-DDD	6.720	5.769	323.8E6	183.4E6	121.718	136.239
17)	MA 4,4'-DDT	7.035	6.021	354.8E6	197.9E6	129.516	140.054
18)	B Endrin al...	6.936	6.096	257.4E6	151.3E6	99.060	107.582
19)	B Endosulfa...	7.171	6.319	329.5E6	195.3E6	108.749	118.218
20)	A Methoxychlor	7.511	6.596	904.4E6	488.8E6	579.865	626.442
21)	B Endrin ke...	7.657	6.825	380.9E6	231.5E6	110.642	120.834

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090923\
Data File : PD077793.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2023 16:56
Operator : AR\AJ
Sample : 04306-10MS
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 22:56:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

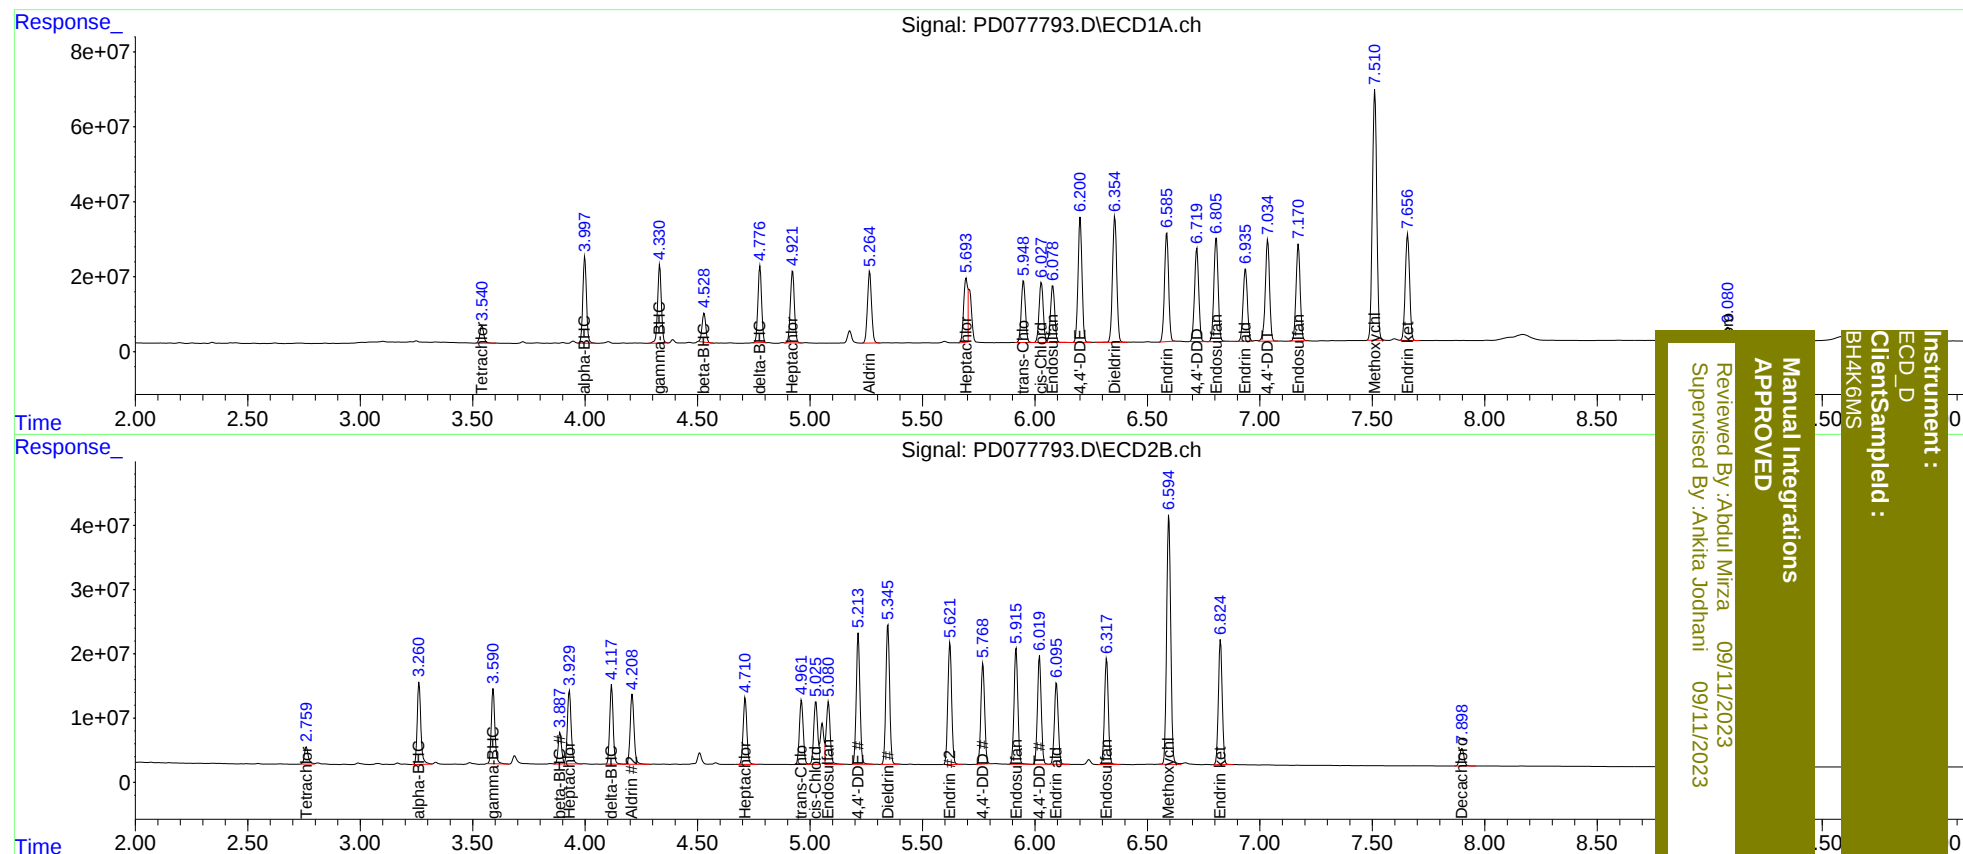

Instrument :
ECD_D
ClientSampled :
BH4K6MS

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 09/11/2023
Supervised By: Ankita Jodhani 09/11/2023