

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090923\
 Data File : PD077794.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2023 17:17
 Operator : AR\AJ
 Sample : 04306-11MSD
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH4K6MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/11/2023
 Supervised By : Ankita Jodhani 09/11/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 22:57:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.759	55231408	31159933	21.764	21.084
27)	SA Decachlor...	9.087	7.899	65231725	35348487	20.881	21.827
Target Compounds							
2)	A alpha-BHC	4.004	3.261	252.4E6	138.6E6	58.938	61.128
3)	MA gamma-BHC...	4.337	3.590	238.4E6	125.4E6	58.974	58.098
4)	MA Heptachlor	4.928	3.929	233.9E6	131.1E6	55.961	58.952
5)	MB Aldrin	5.271	4.209	238.8E6	128.5E6	57.197	57.321
6)	B beta-BHC	4.535	3.887	91242001	49914953	49.664	50.517
7)	B delta-BHC	4.782	4.117	227.4E6	126.7E6	56.640m	56.858
8)	B Heptachlo...	5.698	4.711	215.2E6	116.6E6	55.694m	55.523
9)	A Endosulfan I	6.085	5.081	194.3E6	118.1E6	57.879	65.800
10)	B trans-Chl...	5.955	4.961	206.9E6	116.6E6	55.560	58.403
11)	B cis-Chlor...	6.034	5.026	206.8E6	115.7E6	53.646	56.560
12)	B 4,4'-DDE	6.207	5.215	402.7E6	224.1E6	113.592	117.985
13)	MA Dieldrin	6.360	5.346	437.8E6	249.4E6	116.968	120.681
14)	MA Endrin	6.591	5.622	367.4E6	222.2E6	119.089	121.554
15)	B Endosulfa...	6.811	5.917	360.0E6	209.0E6	108.737	115.486
16)	A 4,4'-DDD	6.725	5.770	318.4E6	172.8E6	119.717	128.377
17)	MA 4,4'-DDT	7.039	6.021	355.9E6	191.4E6	129.912	135.454
18)	B Endrin al...	6.941	6.096	257.4E6	148.9E6	99.063	105.839
19)	B Endosulfa...	7.176	6.319	328.2E6	192.9E6	108.290	116.731
20)	A Methoxychlor	7.515	6.596	897.8E6	475.8E6	575.658	609.696
21)	B Endrin ke...	7.662	6.826	379.4E6	228.6E6	110.203	119.329

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090923\
Data File : PD077794.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2023 17:17
Operator : AR\AJ
Sample : 04306-11MSD
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 22:57:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

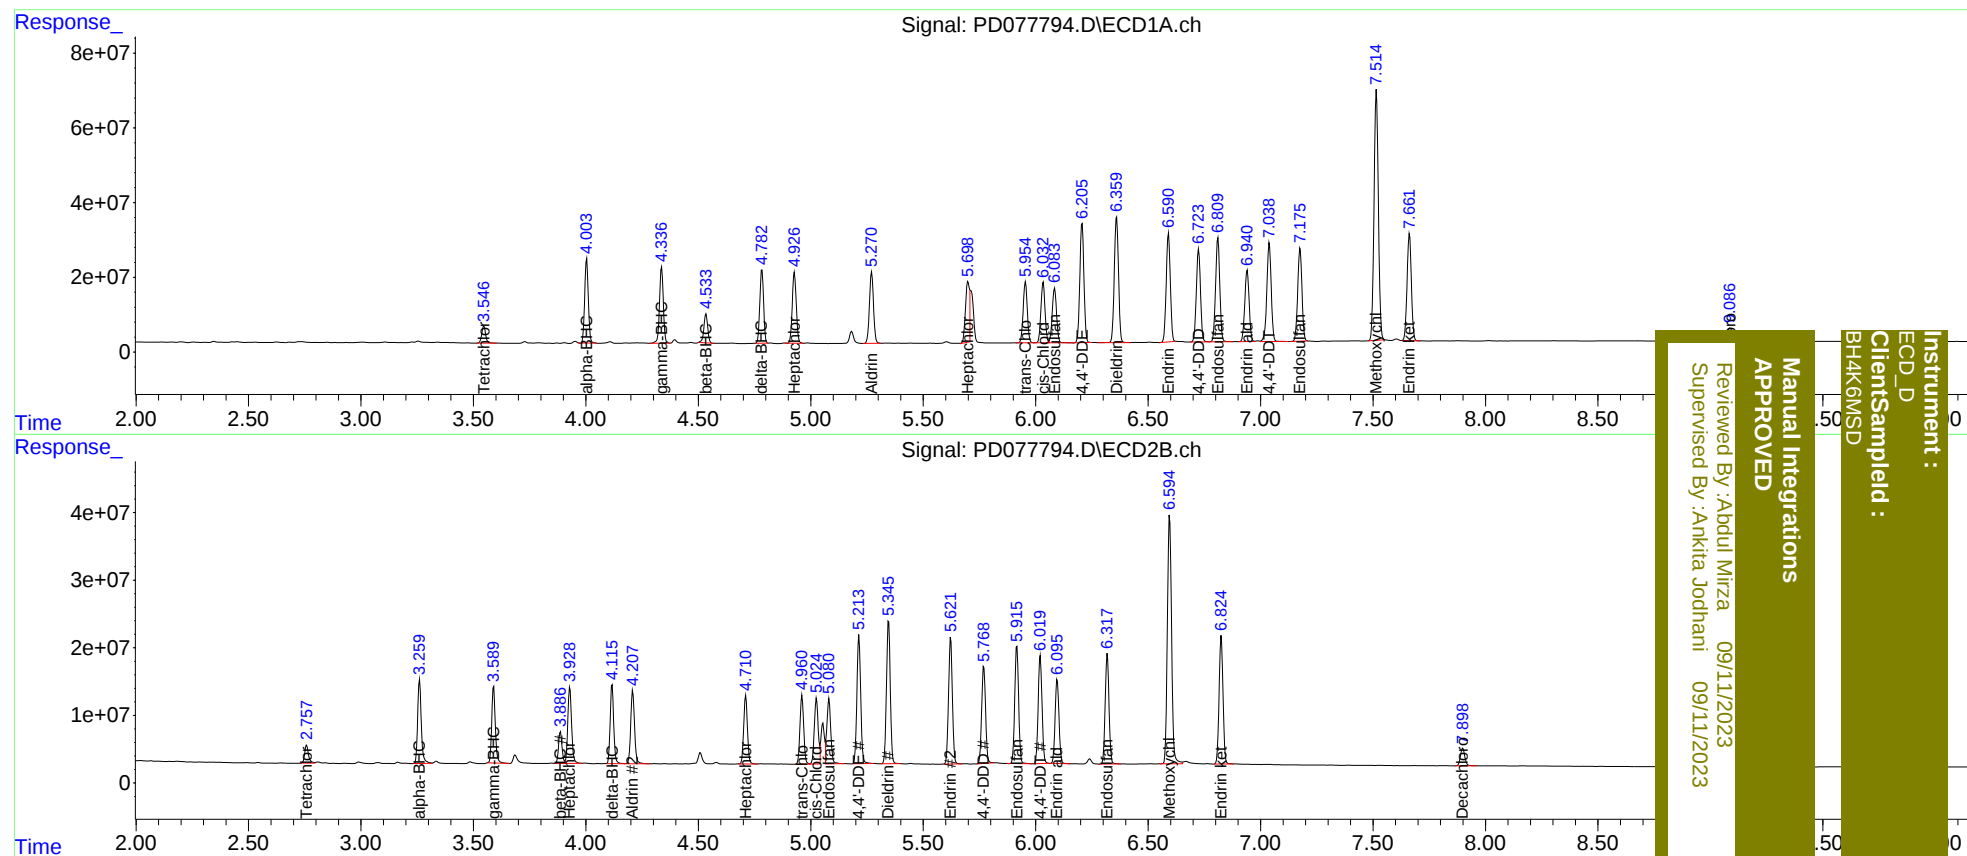

Reviewed By: Abdul Mirza 09/11/2023
Supervised By: Ankita Jodhani 09/11/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
BH4K6MSD