

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090924\
 Data File : PD084962.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2024 14:53
 Operator : AR\AJ
 Sample : P3877-12
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCVY5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 01:48:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
27)	SA Decachlor...	9.035	8.108	13586688	27541020	10.403	7.920
Target Compounds							
4)	MA Heptachlor	0.000	4.092	0	85590440	N.D.	20.106
6)	B beta-BHC	0.000	4.092f	0	85590440	N.D.	39.480
7)	B delta-BHC	4.764	0.000	33079322	0	20.170	N.D. #
9)	A Endosulfan I	6.069	0.000	7173321	0	5.214	N.D. #
11)	B cis-Chlor...	6.069f	0.000	7173321	0	4.852	N.D. #
12)	B 4,4'-DDE	6.200	0.000	17734669	0	14.217	N.D. #
19)	B Endosulfa...	7.138	0.000	19503387	0	16.930	N.D. #
20)	A Methoxychlor	7.497	0.000	235.0E6	0	451.177	N.D. #
21)	B Endrin ke...	7.585	0.000	38052406	0	31.123	N.D. #
25)	Toxaphene-4	7.138	0.000	19503387	0	757.964	N.D. #
26)	Toxaphene-5	0.000	7.365	0	33767857	N.D.	820.918


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090924\
Data File : PD084962.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2024 14:53
Operator : AR\AJ
Sample : P3877-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:48:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

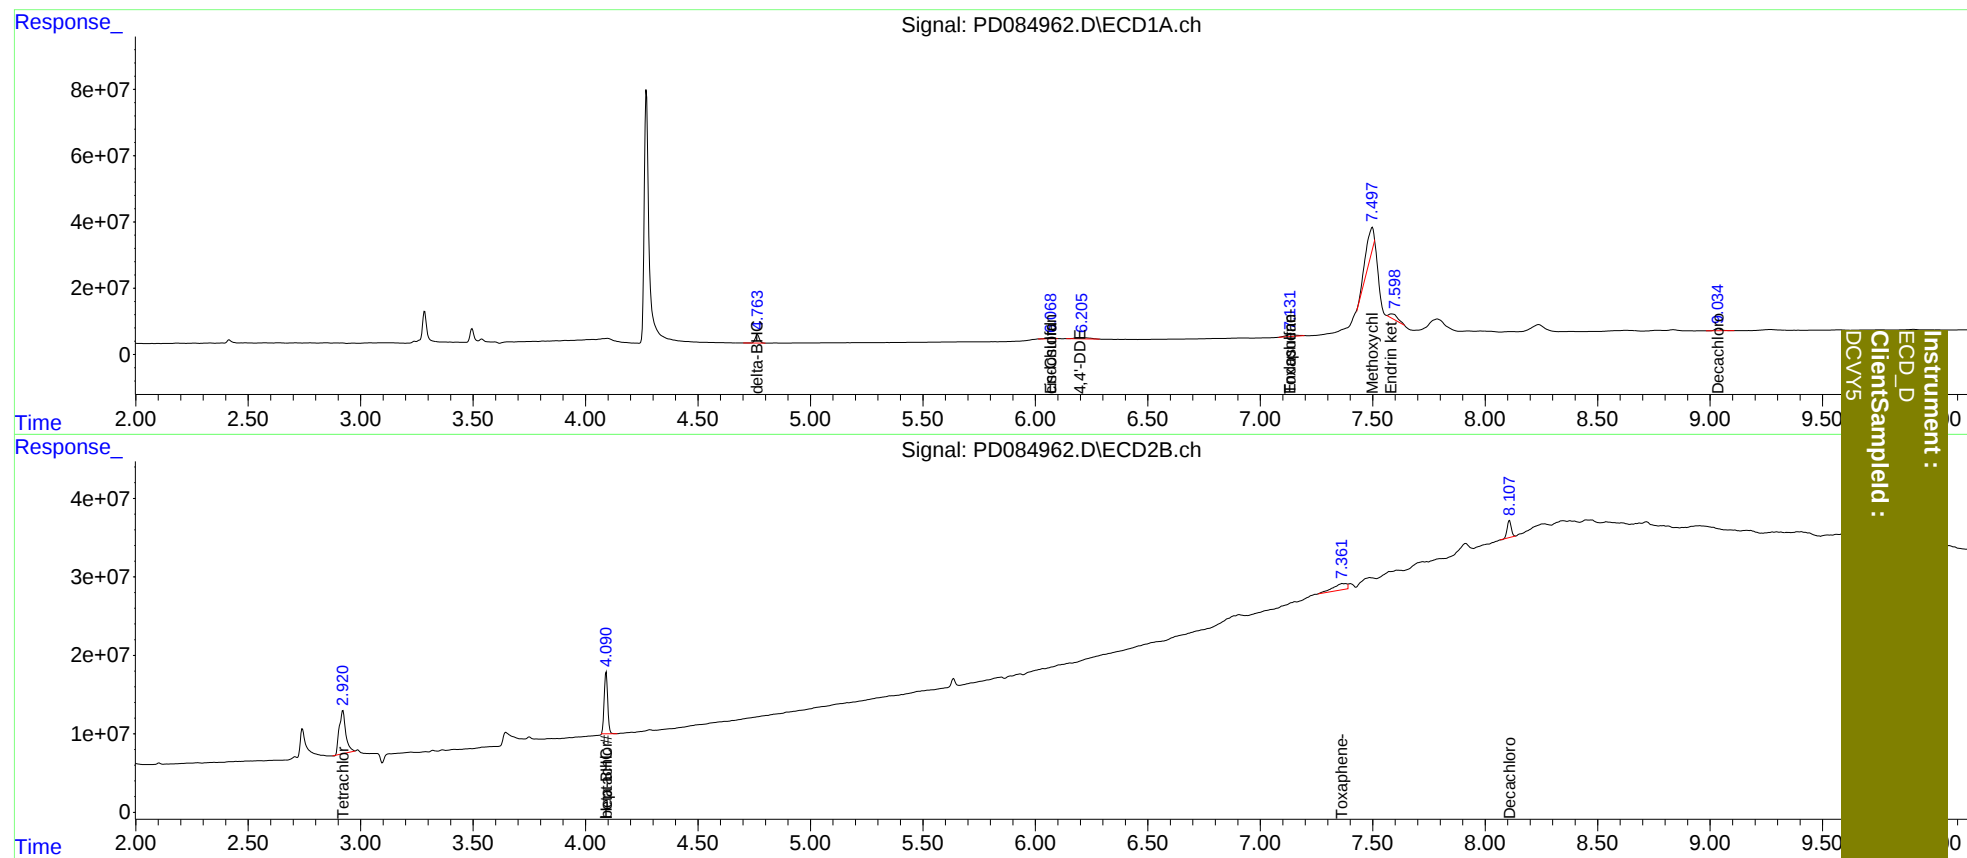


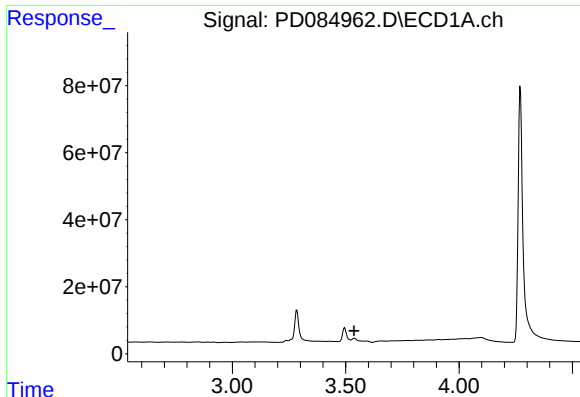

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: 0.002 min
Response: -49886167
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DCVY5

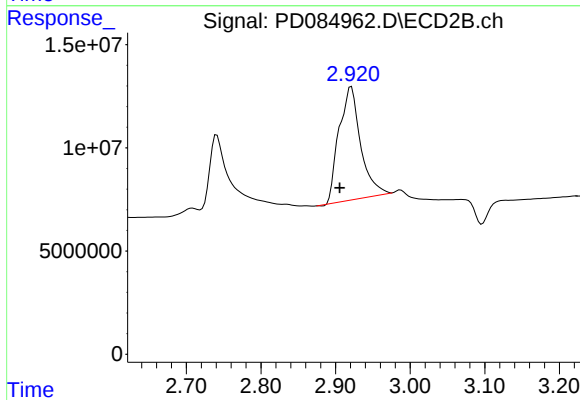


#1 Tetrachloro-m-xylene

R.T.: 2.921 min
Delta R.T.: 0.015 min
Response: 110360542
Conc: 31.19 ng/ml

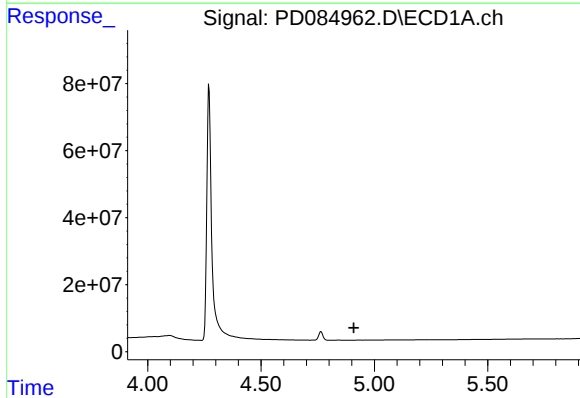


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

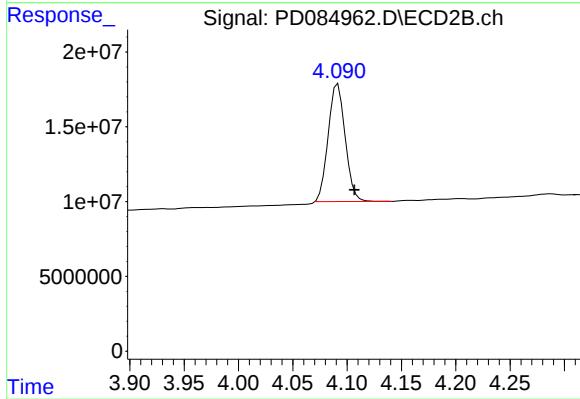

#4 Heptachlor


R.T.: 4.092 min
Delta R.T.: -0.015 min
Response: 85590440
Conc: 20.11 ng/ml

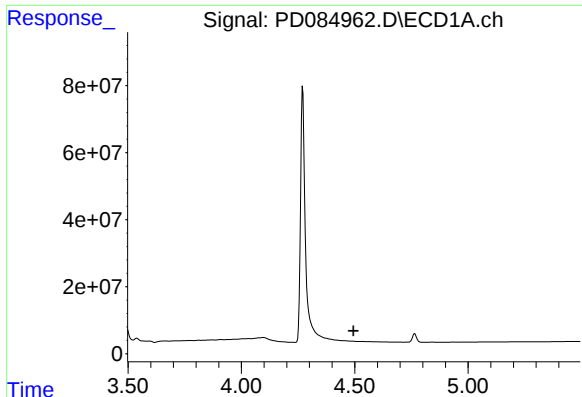

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DCVY5

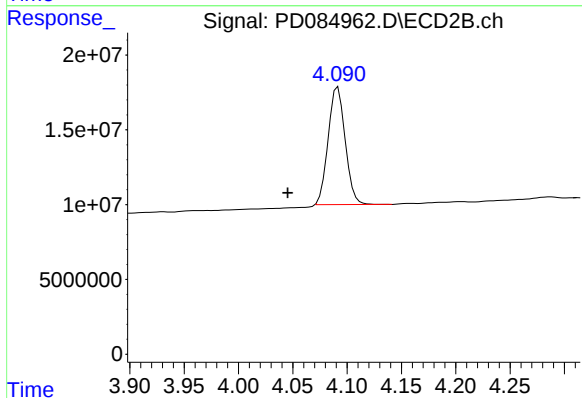


#6 beta-BHC

R.T.: 4.092 min
Delta R.T.: 0.046 min
Response: 85590440
Conc: 39.48 ng/ml

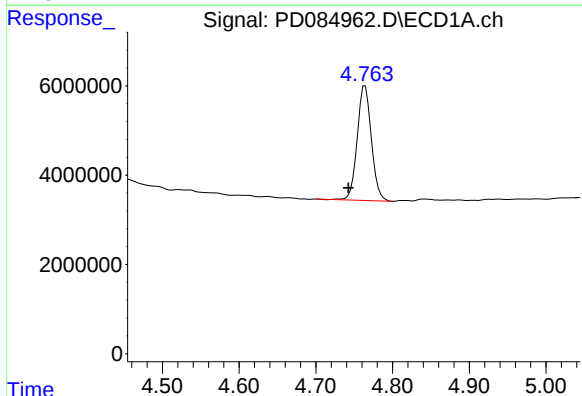


#7 delta-BHC

R.T.: 4.764 min
Delta R.T.: 0.022 min
Response: 33079322
Conc: 20.17 ng/ml

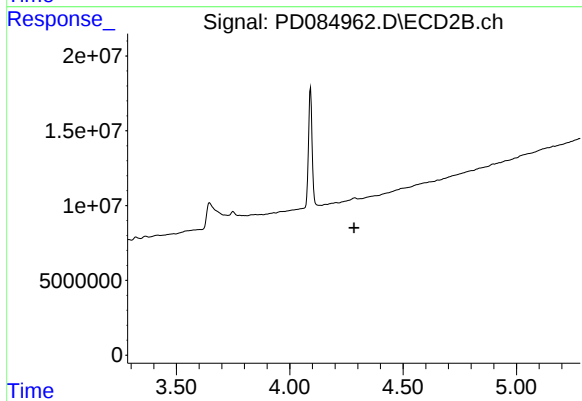

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.283 min
Response: 0
Conc: N.D.

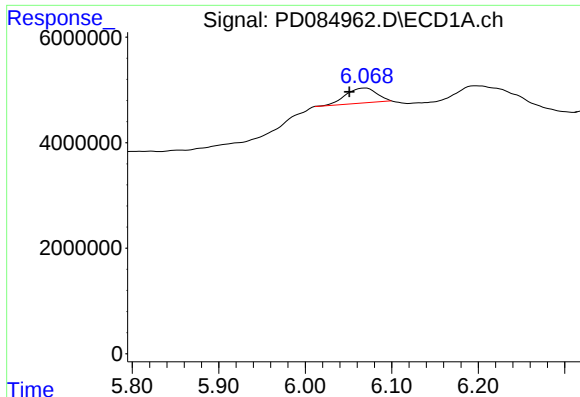

#9 Endosulfan I


R.T.: 6.069 min
Delta R.T.: 0.017 min
Response: 7173321
Conc: 5.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
DCVY5

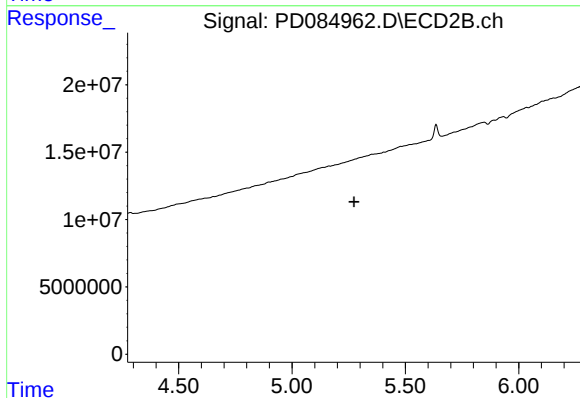


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.273 min
Response: 0
Conc: N.D.

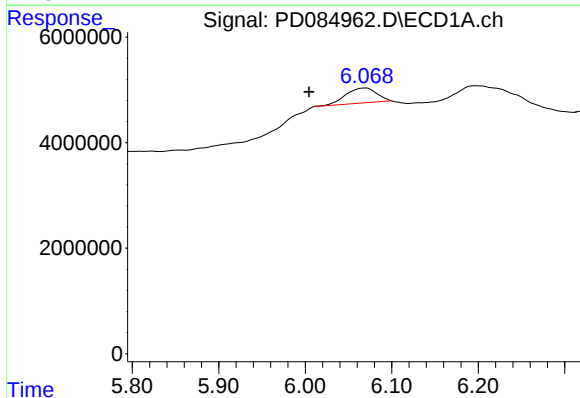


#11 cis-Chlordane

R.T.: 6.069 min
Delta R.T.: 0.064 min
Response: 7173321
Conc: 4.85 ng/ml

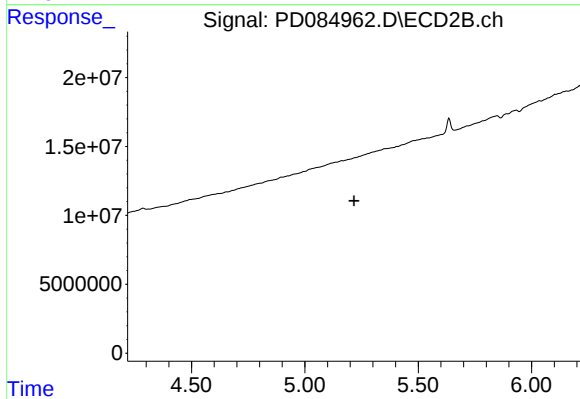

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.217 min
Response: 0
Conc: N.D.

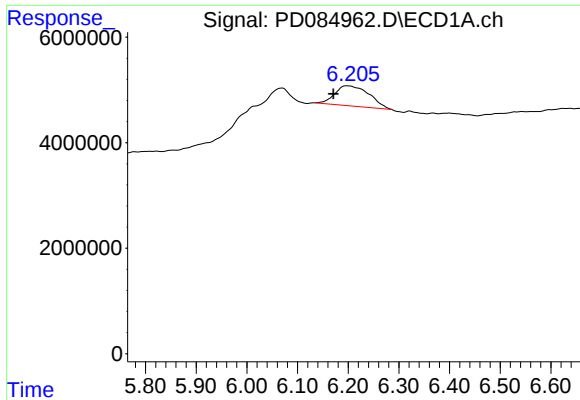

#12 4,4'-DDE


R.T.: 6.200 min
Delta R.T.: 0.029 min
Response: 17734669
Conc: 14.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
DCVY5

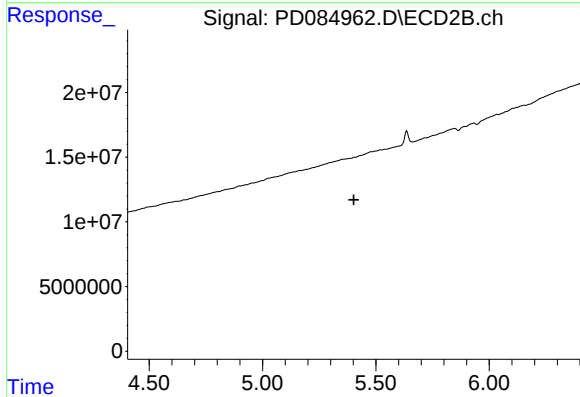


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.402 min
Response: 0
Conc: N.D.

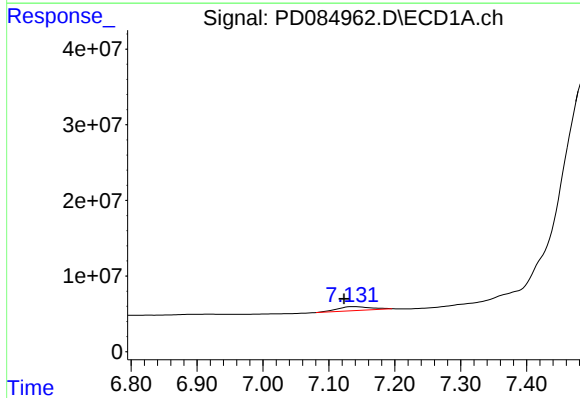


#19 Endosulfan Sulfate

R.T.: 7.138 min
Delta R.T.: 0.015 min
Response: 19503387
Conc: 16.93 ng/ml

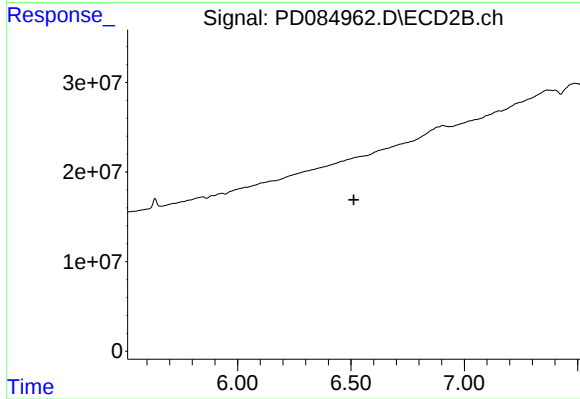

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.513 min
Response: 0
Conc: N.D.

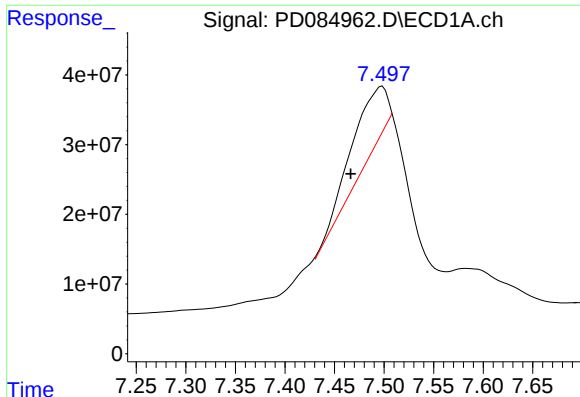

#20 Methoxychlor


R.T.: 7.497 min
Delta R.T.: 0.031 min
Response: 235024812
Conc: 451.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
DCVY5

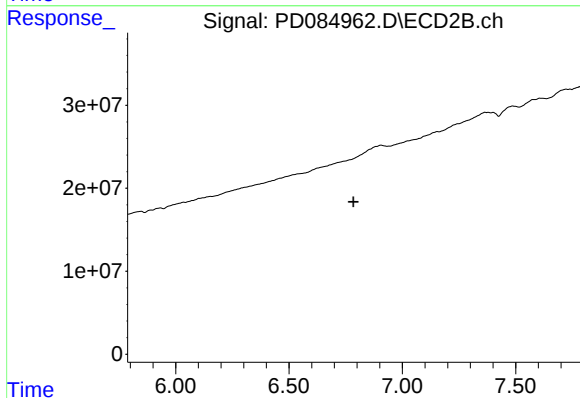


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.785 min
Response: 0
Conc: N.D.

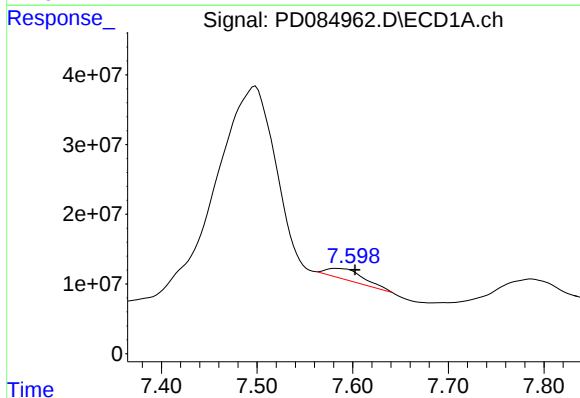


#21 Endrin ketone

R.T.: 7.585 min
Delta R.T.: -0.018 min
Response: 38052406
Conc: 31.12 ng/ml

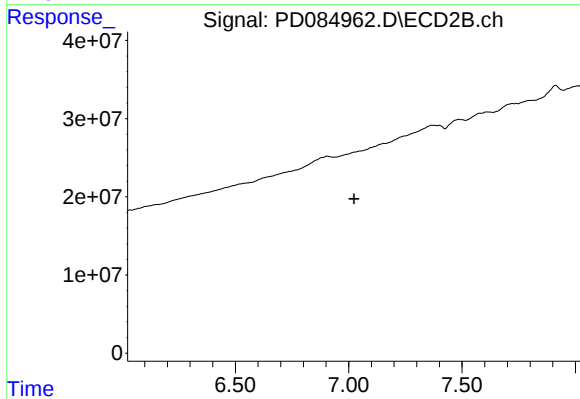

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.023 min
Response: 0
Conc: N.D.

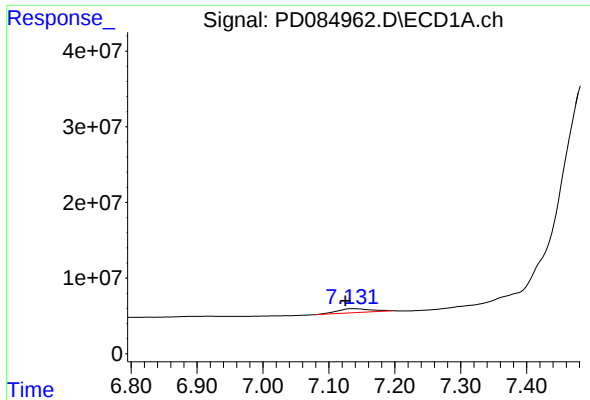

#25 Toxaphene-4


R.T.: 7.138 min
Delta R.T.: 0.013 min
Response: 19503387
Conc: 757.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
DCVY5

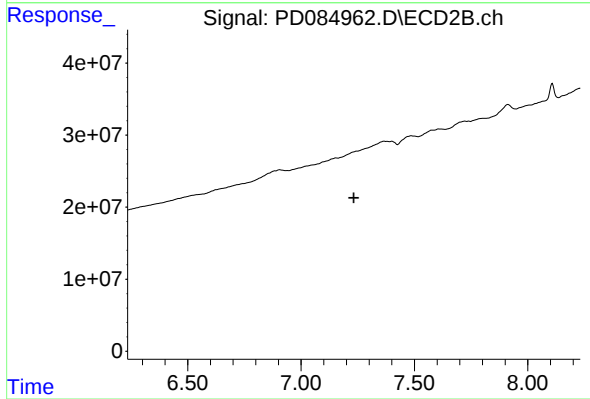


#25 Toxaphene-4

R.T.: 0.000 min
Exp R.T. : 7.232 min
Response: 0
Conc: N.D.

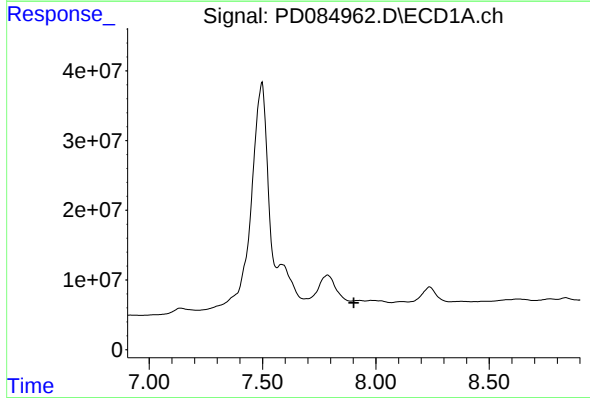


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T. : 7.902 min
Response: 0
Conc: N.D.

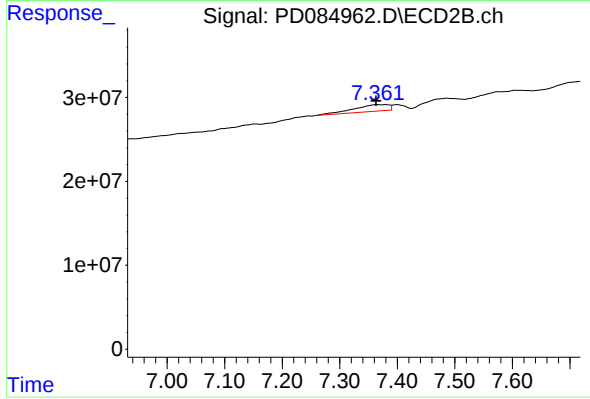

#26 Toxaphene-5


R.T.: 7.365 min
Delta R.T.: 0.002 min
Response: 33767857
Conc: 820.92 ng/ml

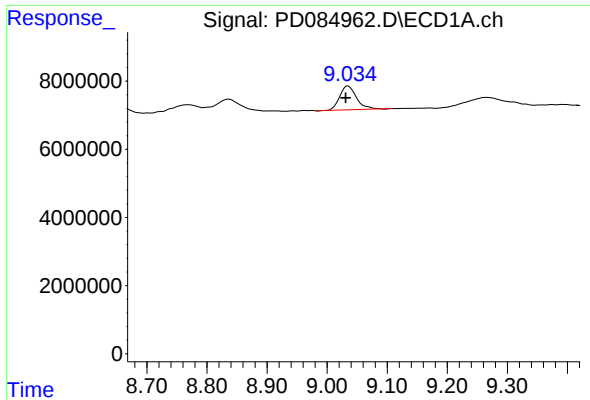

#27 Decachlorobiphenyl

R.T.: 9.035 min
Delta R.T.: 0.004 min
Response: 13586688
Conc: 10.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
DCVY5

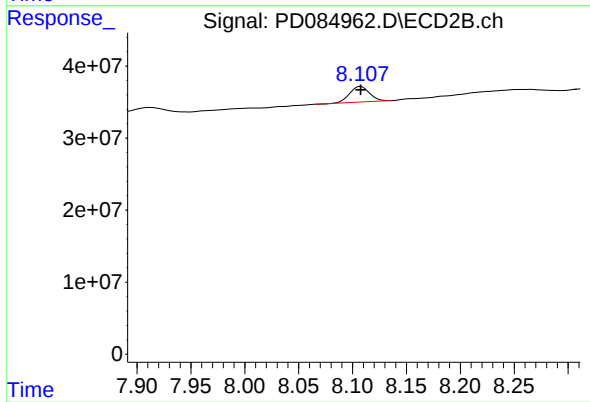

#27 Decachlorobiphenyl

R.T.: 8.108 min
Delta R.T.: 0.000 min
Response: 27541020
Conc: 7.92 ng/ml