

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090924\
 Data File : PD084970.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2024 16:53
 Operator : AR\AJ
 Sample : P3877-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 01:51:14 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.906	11462570	53027161	11.333	14.984 #
2)	SA Decachlor...	9.036	8.106	13239314	34410607	10.137	9.896
Target Compounds							
4)	MA Heptachlor	0.000	4.091	0	175.3E6	N.D.	41.189
6)	B beta-BHC	0.000	4.091f	0	175.3E6	N.D.	80.881
7)	B delta-BHC	4.764	0.000	70427049	0	42.943	N.D. #
19)	B Endosulfa...	0.000	6.455f	0	3830302	N.D.	1.072
20)	A Methoxychlor	7.498	0.000	14139801	0	27.144	N.D. #
21)	B Endrin ke...	7.606	0.000	3437048	0	2.811	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090924\
Data File : PD084970.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2024 16:53
Operator : AR\AJ
Sample : P3877-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:51:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

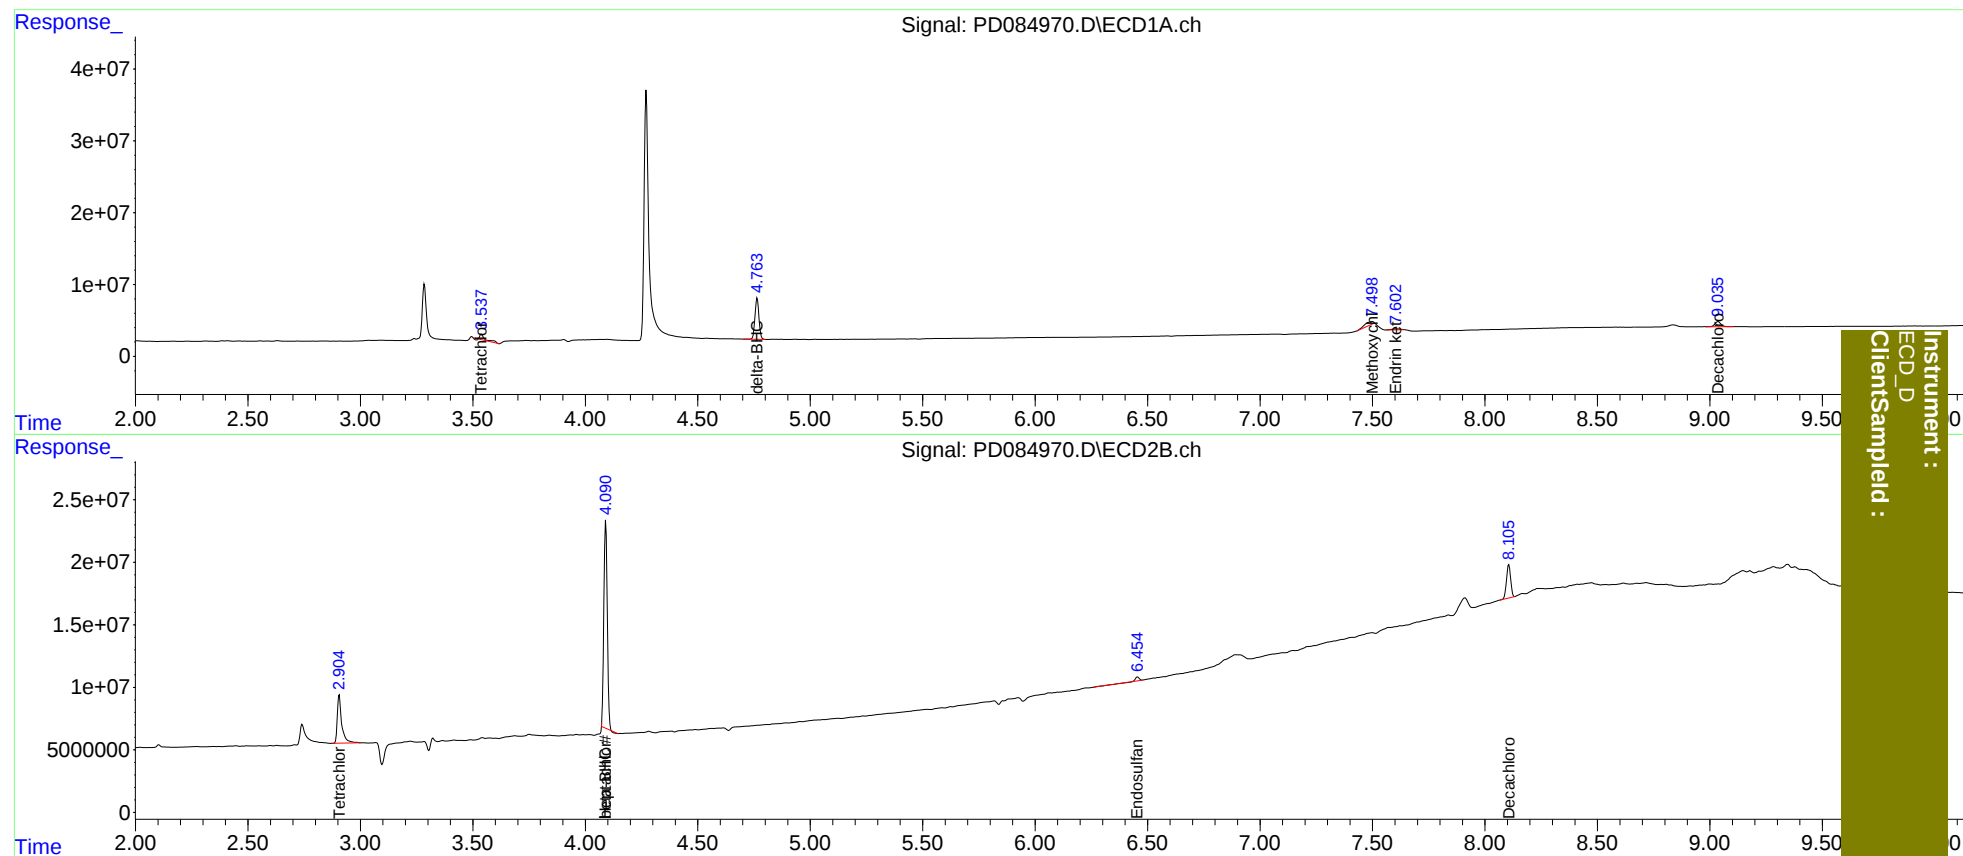


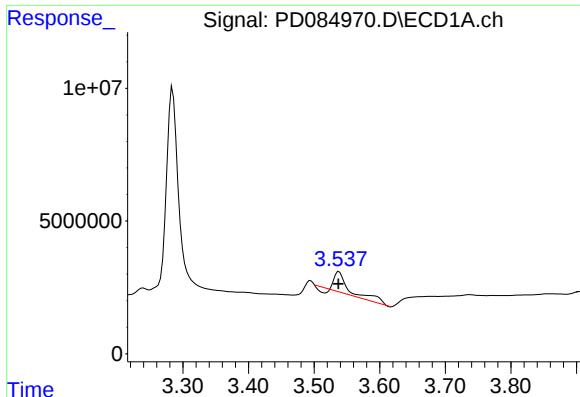

#1 Tetrachloro-m-xylene


R.T.: 3.538 min
Delta R.T.: 0.001 min
Response: 11462570
Conc: 11.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

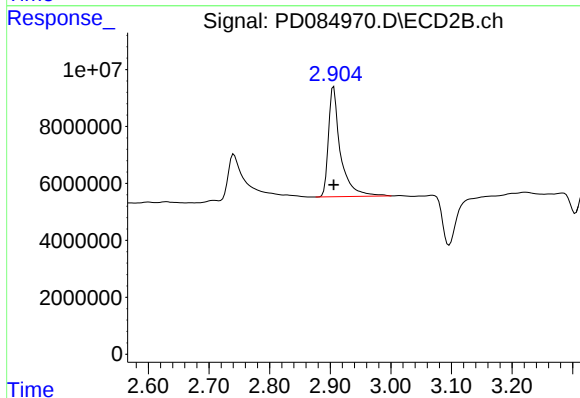


#1 Tetrachloro-m-xylene

R.T.: 2.906 min
Delta R.T.: 0.000 min
Response: 53027161
Conc: 14.98 ng/ml

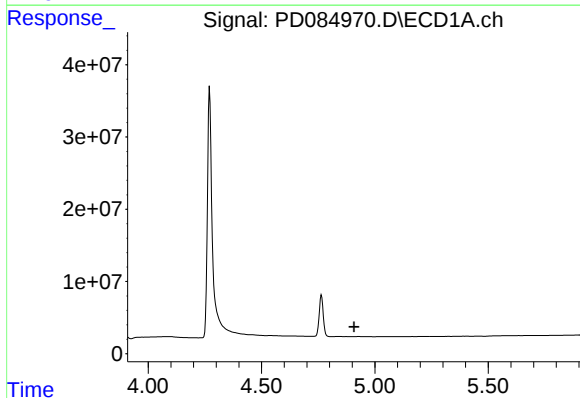


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

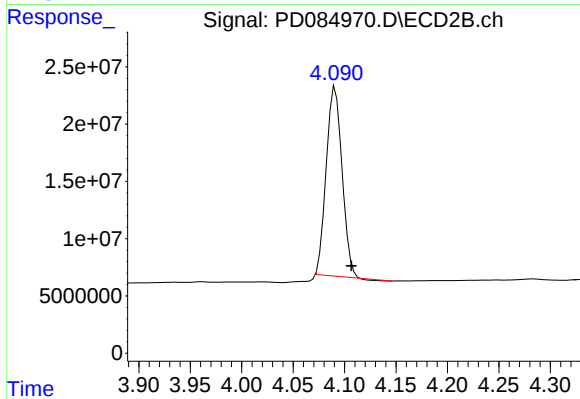

#4 Heptachlor


R.T.: 4.091 min
Delta R.T.: -0.016 min
Response: 175344798
Conc: 41.19 ng/ml

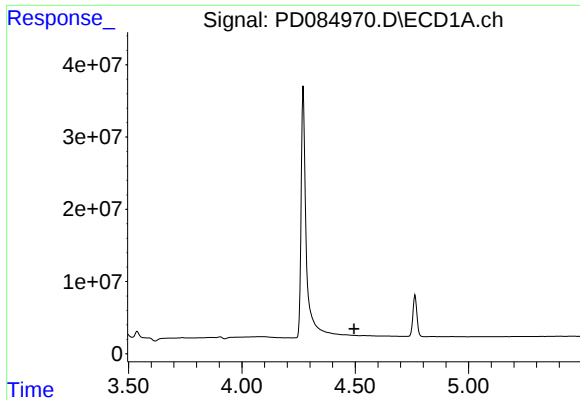

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

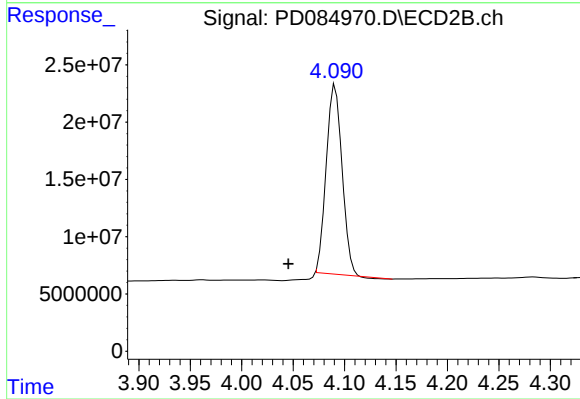


#6 beta-BHC

R.T.: 4.091 min
Delta R.T.: 0.046 min
Response: 175344798
Conc: 80.88 ng/ml

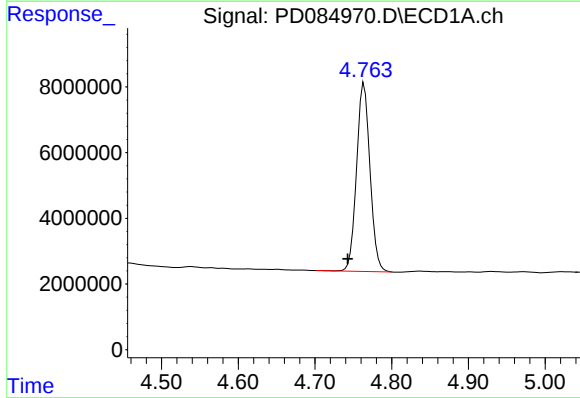


#7 delta-BHC

R.T.: 4.764 min
Delta R.T.: 0.022 min
Response: 70427049
Conc: 42.94 ng/ml

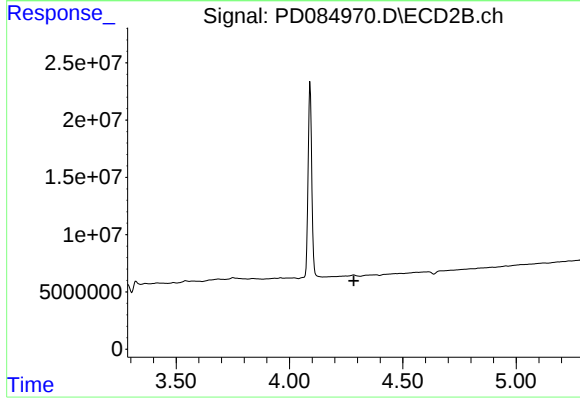

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.283 min
Response: 0
Conc: N.D.

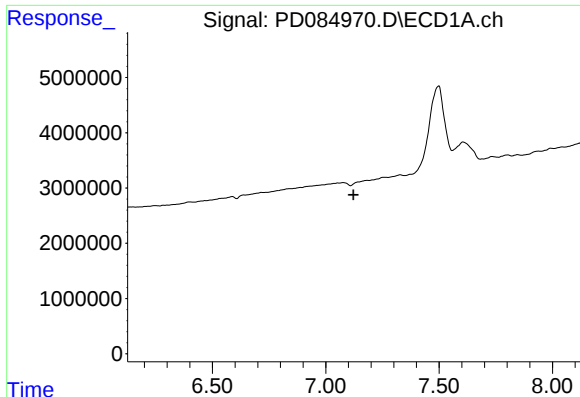

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.123 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

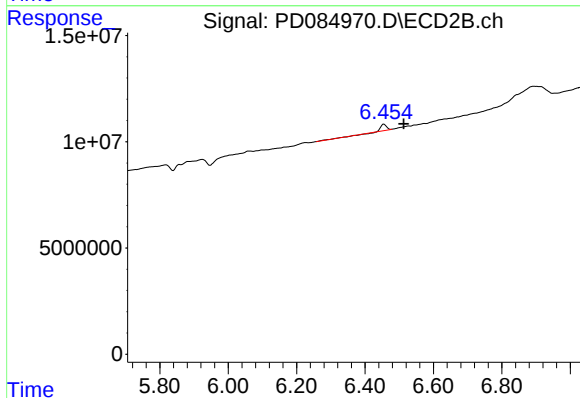


#19 Endosulfan Sulfate

R.T.: 6.455 min
Delta R.T.: -0.058 min
Response: 3830302
Conc: 1.07 ng/ml

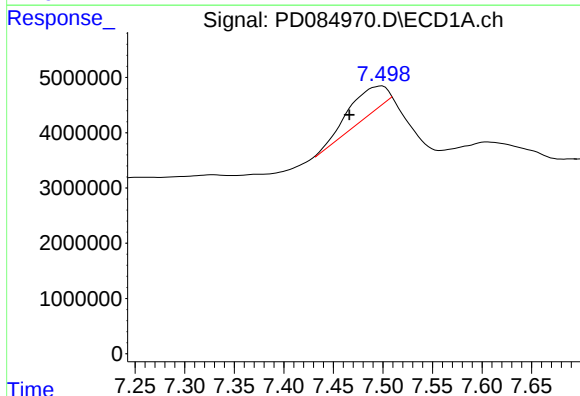


#20 Methoxychlor

R.T.: 7.498 min
Delta R.T.: 0.032 min
Response: 14139801
Conc: 27.14 ng/ml

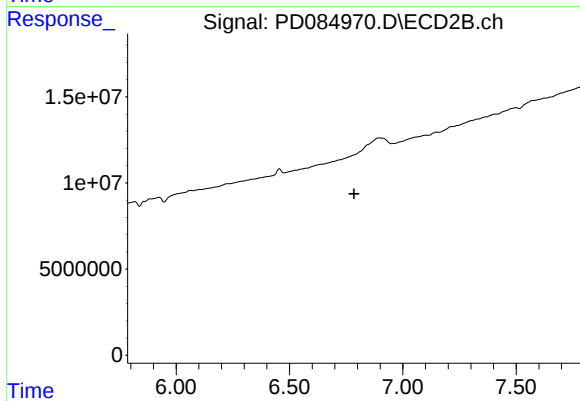

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.785 min
Response: 0
Conc: N.D.

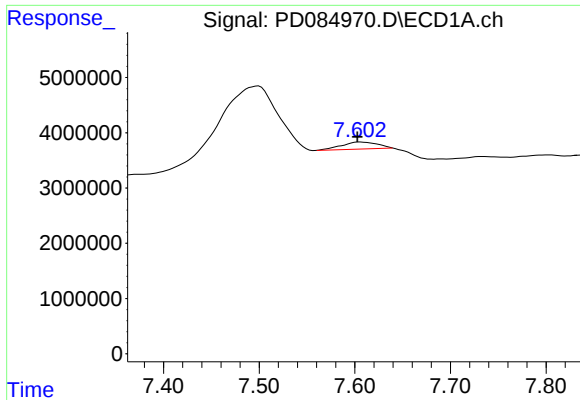

#21 Endrin ketone


R.T.: 7.606 min
Delta R.T.: 0.003 min
Response: 3437048
Conc: 2.81 ng/ml

Instrument :
ECD_D
ClientSampleId :

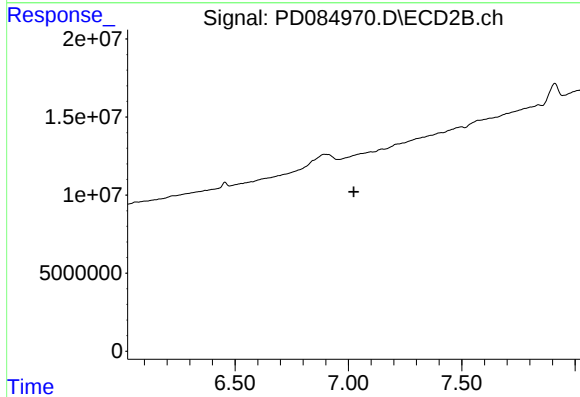


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.023 min
Response: 0
Conc: N.D.

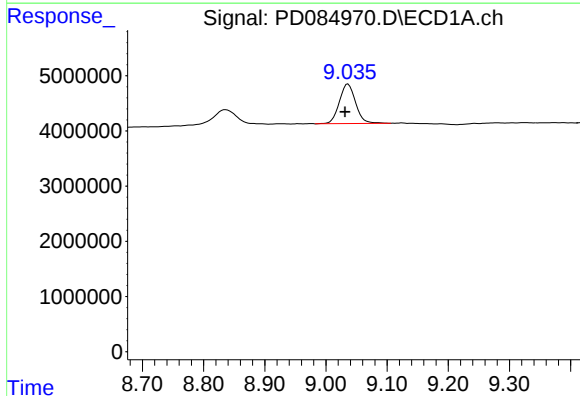

#27 Decachlorobiphenyl

R.T.: 9.036 min
Delta R.T.: 0.005 min
Response: 13239314
Conc: 10.14 ng/ml

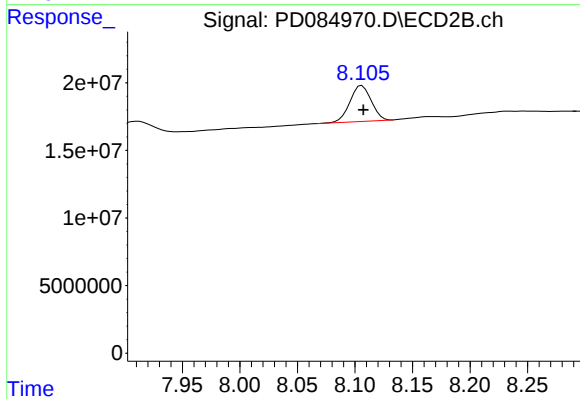

#27 Decachlorobiphenyl

R.T.: 8.106 min
Delta R.T.: -0.001 min
Response: 34410607
Conc: 9.90 ng/ml