

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090924\
 Data File : PD084958.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2024 13:59
 Operator : AR\AJ
 Sample : P3877-08MS
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCVY2MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/12/2024
 Supervised By : Ankita Jodhani 09/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 01:46:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	2.901	37810829	23251574	37.385m	6.570m#
27)	SA Decachlor...	9.032	8.105	18322431	38505578	14.029	11.074
Target Compounds							
2)	A alpha-BHC	3.983	3.417	127.6E6	299.6E6	75.074	59.083
3)	MA gamma-BHC...	4.256f	3.747	74292.7E6	1334.1E6	45920.473m	275.312m#
4)	MA Heptachlor	4.909	4.104	71036978	171.8E6	46.170m	40.351m
5)	MB Aldrin	5.251	4.388	84911966	102.5E6	53.091	23.068 #
6)	B beta-BHC	4.471	4.041	175.3E6	102.4E6	241.269m	47.220m#
7)	B delta-BHC	4.743	4.282	165.4E6	418.4E6	100.858	84.278
8)	B Heptachlo...	5.668	4.894	54399012	242.5E6	36.473m	57.247m#
9)	A Endosulfan I	6.051	5.272	89723321	200.6E6	65.215m	52.322m
10)	B trans-Chl...	5.923	5.148	74395819	191.5E6	52.749	46.553m
11)	B cis-Chlor...	6.003	5.214	74102442	208.6E6	50.118m	49.725m
12)	B 4,4'-DDE	6.173	5.399	137.8E6	255.5E6	110.490	65.129m#
13)	MA Dieldrin	6.323	5.538	183.7E6	382.4E6	124.561m	89.001m#
14)	MA Endrin	6.550	5.814	123.9E6	342.4E6	109.784m	92.474m
15)	B Endosulfa...	6.761	6.107	118.5E6	363.9E6	89.780m	98.141m
16)	A 4,4'-DDD	6.682	5.956	107.9E6	249.1E6	109.267	73.400 #
17)	MA 4,4'-DDT	6.995	6.210	100.2E6	292.2E6	111.933m	91.347m
18)	B Endrin al...	6.890	6.287	95245818	222.4E6	105.465	77.876 #
19)	B Endosulfa...	7.124	6.511	142.0E6	277.9E6	123.229	77.821 #
20)	A Methoxychlor	7.465	6.782	988.8E6	670.9E6	1898.182m	405.539m#
21)	B Endrin ke...	7.603	7.022	114.4E6	340.5E6	93.532	77.334

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090924\
Data File : PD084958.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2024 13:59
Operator : AR\AJ
Sample : P3877-08MS
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:46:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

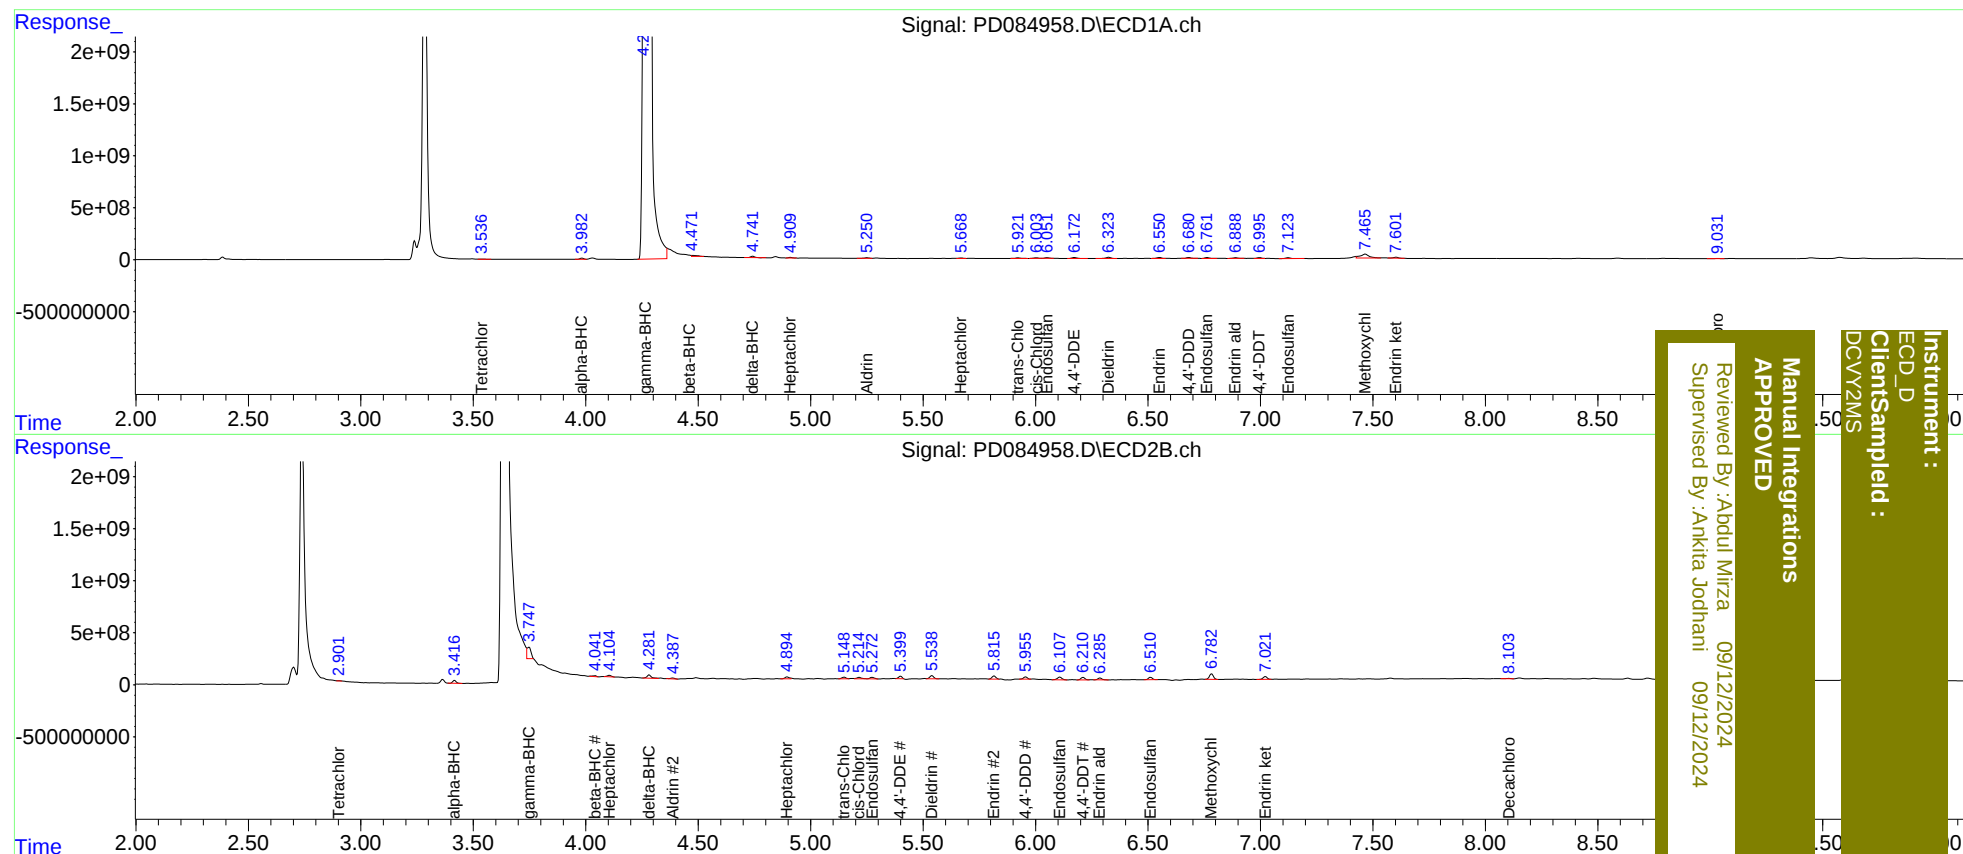

Reviewed By: Abdul Mirza 09/12/2024
Supervised By: Ankita Jodhani 09/12/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
DCVY2MS