

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090924\
 Data File : PD084965.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2024 15:33
 Operator : AR\AJ
 Sample : P3877-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCVZ4

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/12/2024
 Supervised By :Ankita Jodhani 09/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 01:49:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.527	2.919	19606296	623.5E6	19.385m	176.189m#
2)	SA Decachlor...	9.033	8.105	15095016	30970148	11.558m	8.907m
Target Compounds							
2)	A alpha-BHC	3.984	3.415	28475202	82220887	16.749	16.216m
7)	B delta-BHC	4.742	4.280	37034847	124.4E6	22.582m	25.066m
9)	A Endosulfan I	6.056	5.283	20102179	30775402	14.611	8.028 #
17)	MA 4,4'-DDT	6.997	6.210	16555374	72408087	18.495m	22.635m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090924\
Data File : PD084965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2024 15:33
Operator : AR\AJ
Sample : P3877-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:49:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

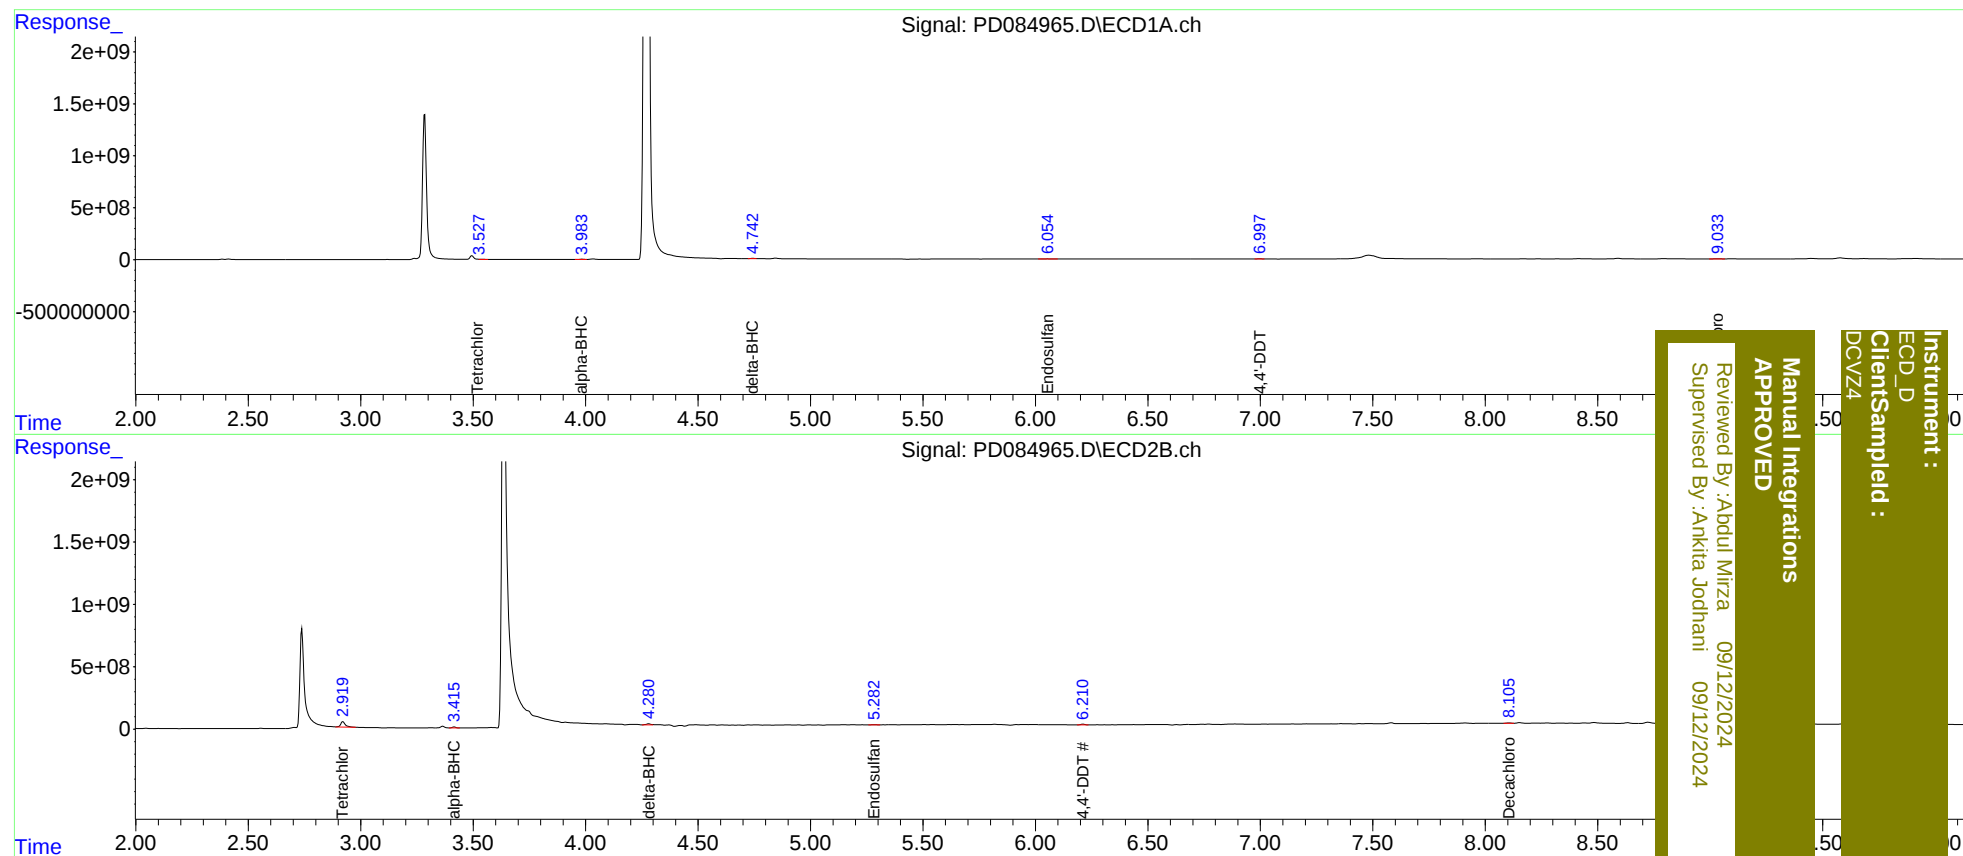

Reviewed By: Abdul Mirza 09/12/2024
Supervised By: Ankita Jodhani 09/12/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
DCVZA