

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090924\
 Data File : PD084952.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2024 12:39
 Operator : AR\AJ
 Sample : P3877-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCVX7

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/12/2024
 Supervised By :Ankita Jodhani 09/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 01:44:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.919	42007013	277.8E6	41.533m	78.493m#
2)	SA Decachlor...	9.032	8.103	26005152	50727693	19.912m	14.589m#
Target Compounds							
2)	A alpha-BHC	3.984	3.416	60964317	221.6E6	35.858	43.698
7)	B delta-BHC	4.743	4.280	72853743	171.4E6	44.423m	34.519m
9)	A Endosulfan I	6.053	5.282	72751576	98955601	52.879m	25.815 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090924\
Data File : PD084952.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2024 12:39
Operator : AR\AJ
Sample : P3877-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:44:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

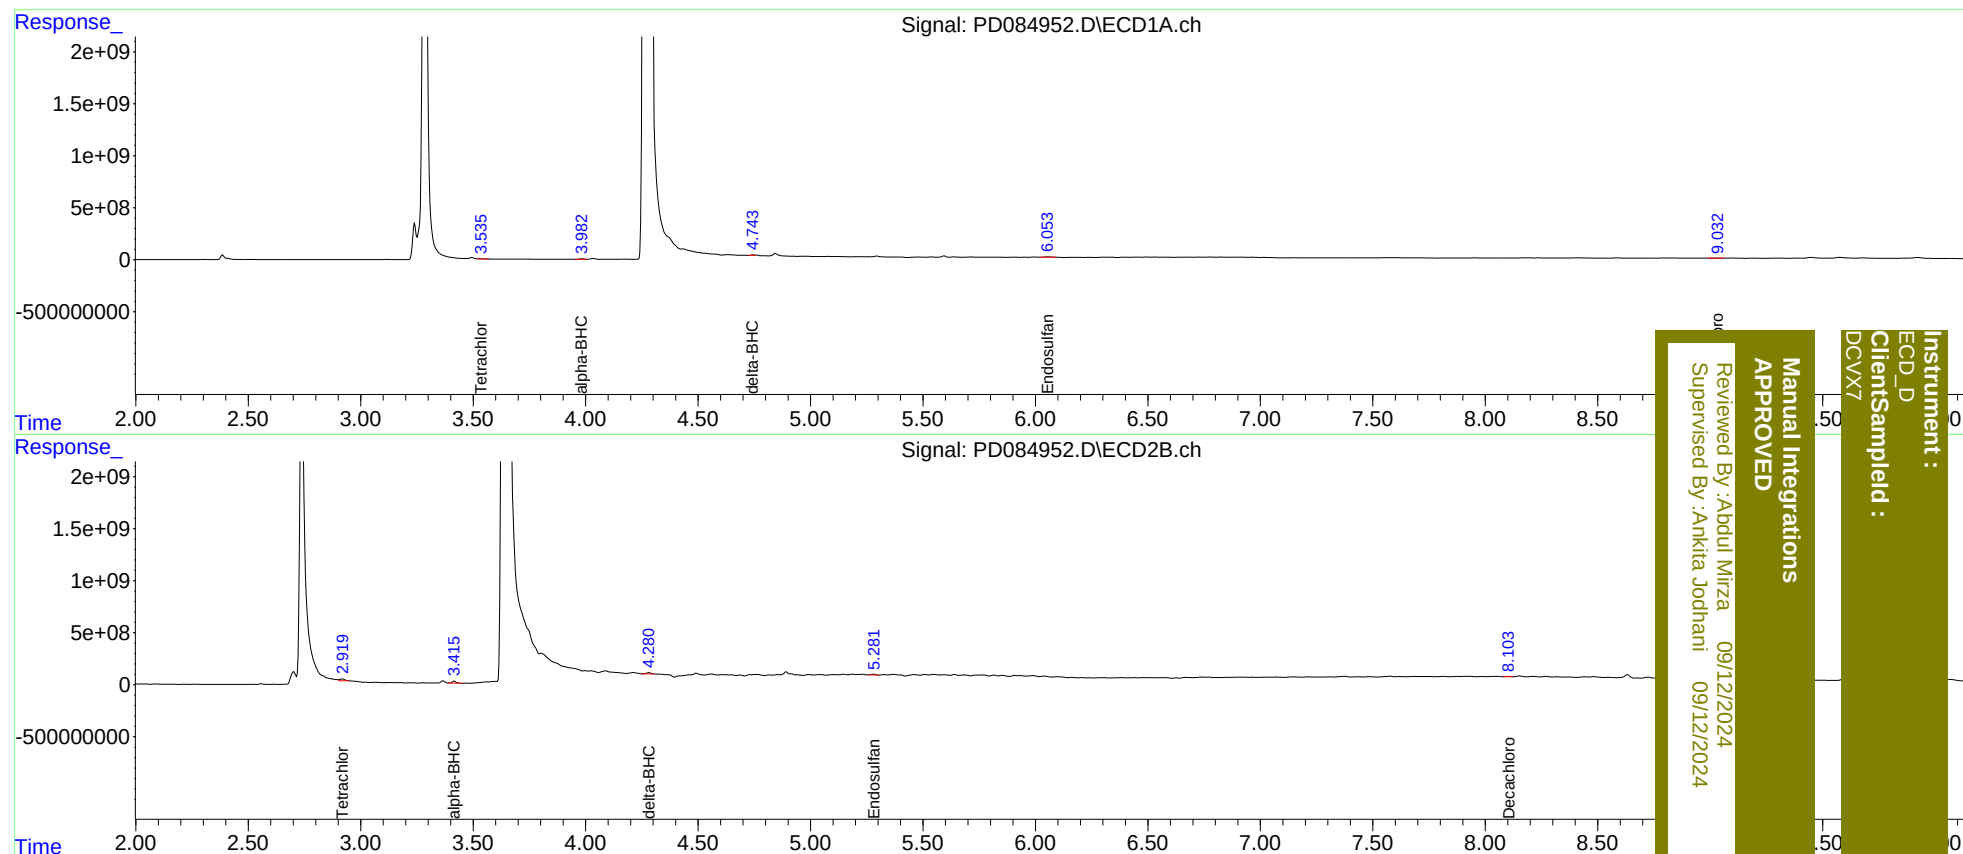

Reviewed By: Abdul Mirza 09/12/2024
Supervised By: Ankita Jodhani 09/12/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
DCVX7