

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090924\
 Data File : PD084956.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2024 13:32
 Operator : AR\AJ
 Sample : P3877-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCVY1

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/12/2024
 Supervised By :Ankita Jodhani 09/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 01:45:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.536	2.924	7985837	25617375	7.896m	7.239m
2) SA Decachlor...	9.031	8.125	13090129	31320901	10.023	9.008
Target Compounds						
2) A alpha-BHC	3.983	3.434	10044940	31240204	5.908	6.161m
9) A Endosulfan I	6.053	5.299	5768051	12218640	4.193m	3.187m
13) MA Dieldrin	6.321	5.560	3961919	11784509	2.686m	2.743m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090924\
Data File : PD084956.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2024 13:32
Operator : AR\AJ
Sample : P3877-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:45:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

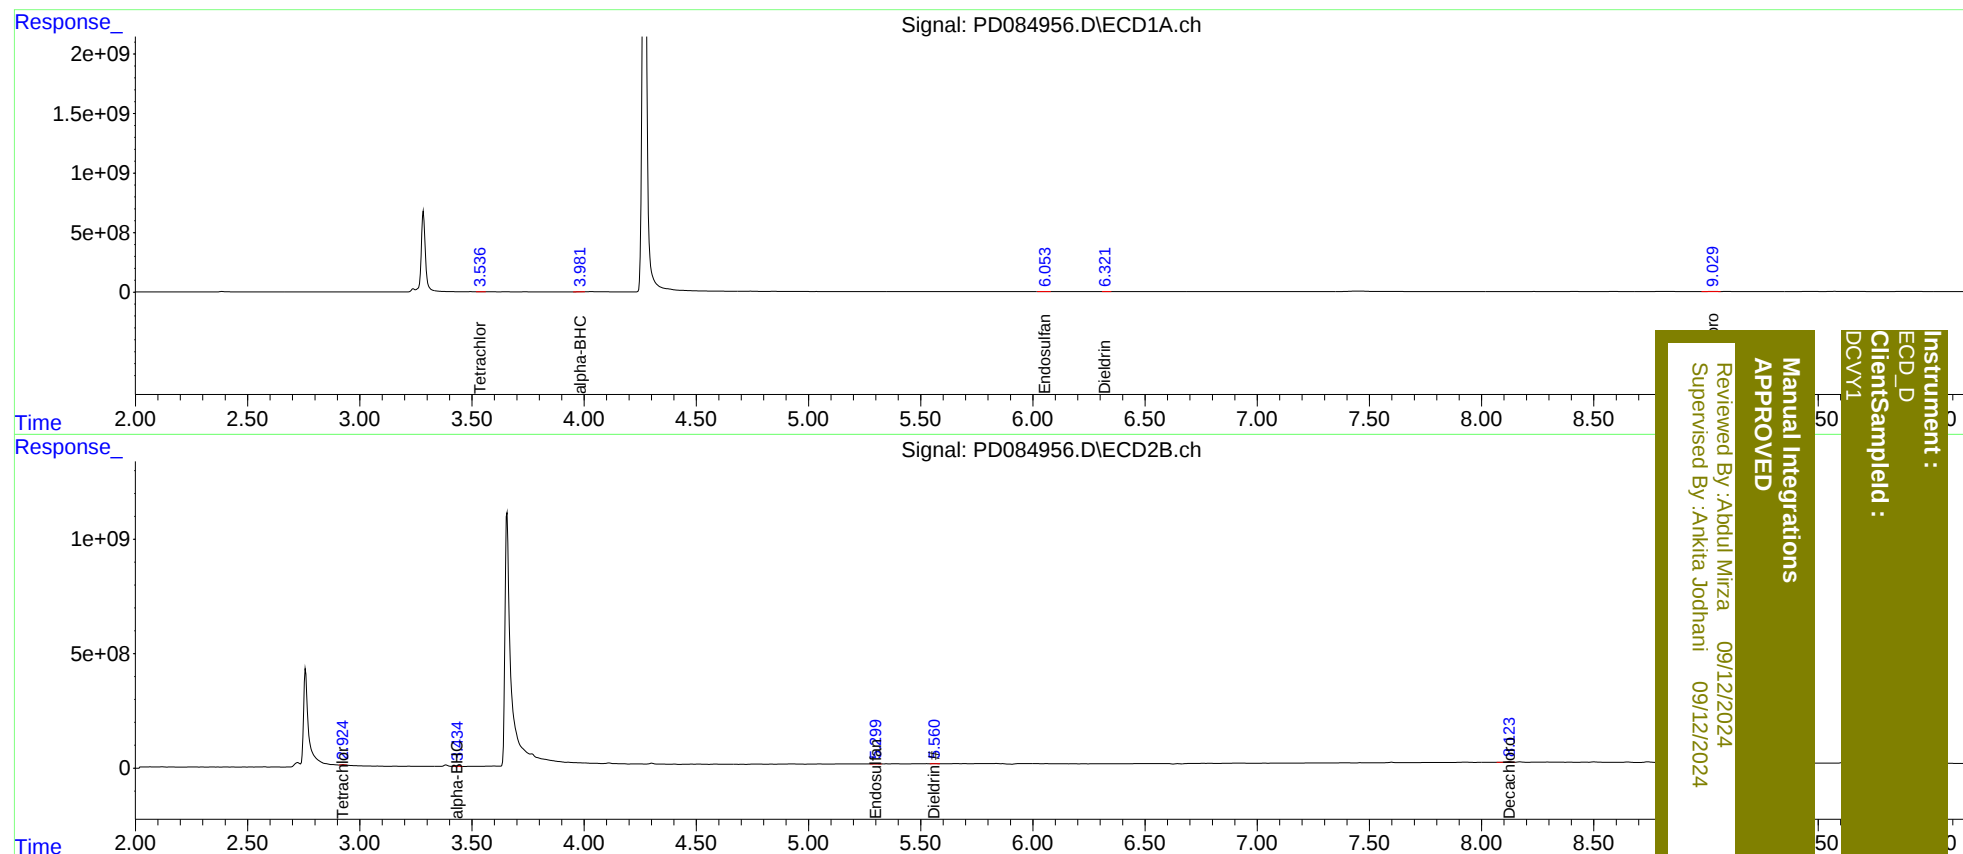

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 09/12/2024
Supervised By: Ankita Jodhani 09/12/2024

Instrument :
ECD_D
ClientSampled :
DCVY1