

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091019\
 Data File : PD054447.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Sep 2019 13:29
 Operator : SG\AJ
 Sample : K4708-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB5Q0

Manual Integrations
 APPROVED

Ankita
 9/10/2019 5:58:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 14:05:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090419CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 05 08:40:10 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.301	3.972	14281107	19982240	20.206	20.247
2) SA Decachlor...	7.990	9.007	26365172	37663454	38.958	40.260
Target Compounds						
16) A 4,4'-DDD	5.931	6.782	1200570	2346420	1.734m	2.202m#
17) MA 4,4'-DDT	6.167	7.079	1001830	1244176	1.592m	1.197m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091019\
Data File : PD054447.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Sep 2019 13:29
Operator : SG\AJ
Sample : K4708-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 14:05:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090419CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 05 08:40:10 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

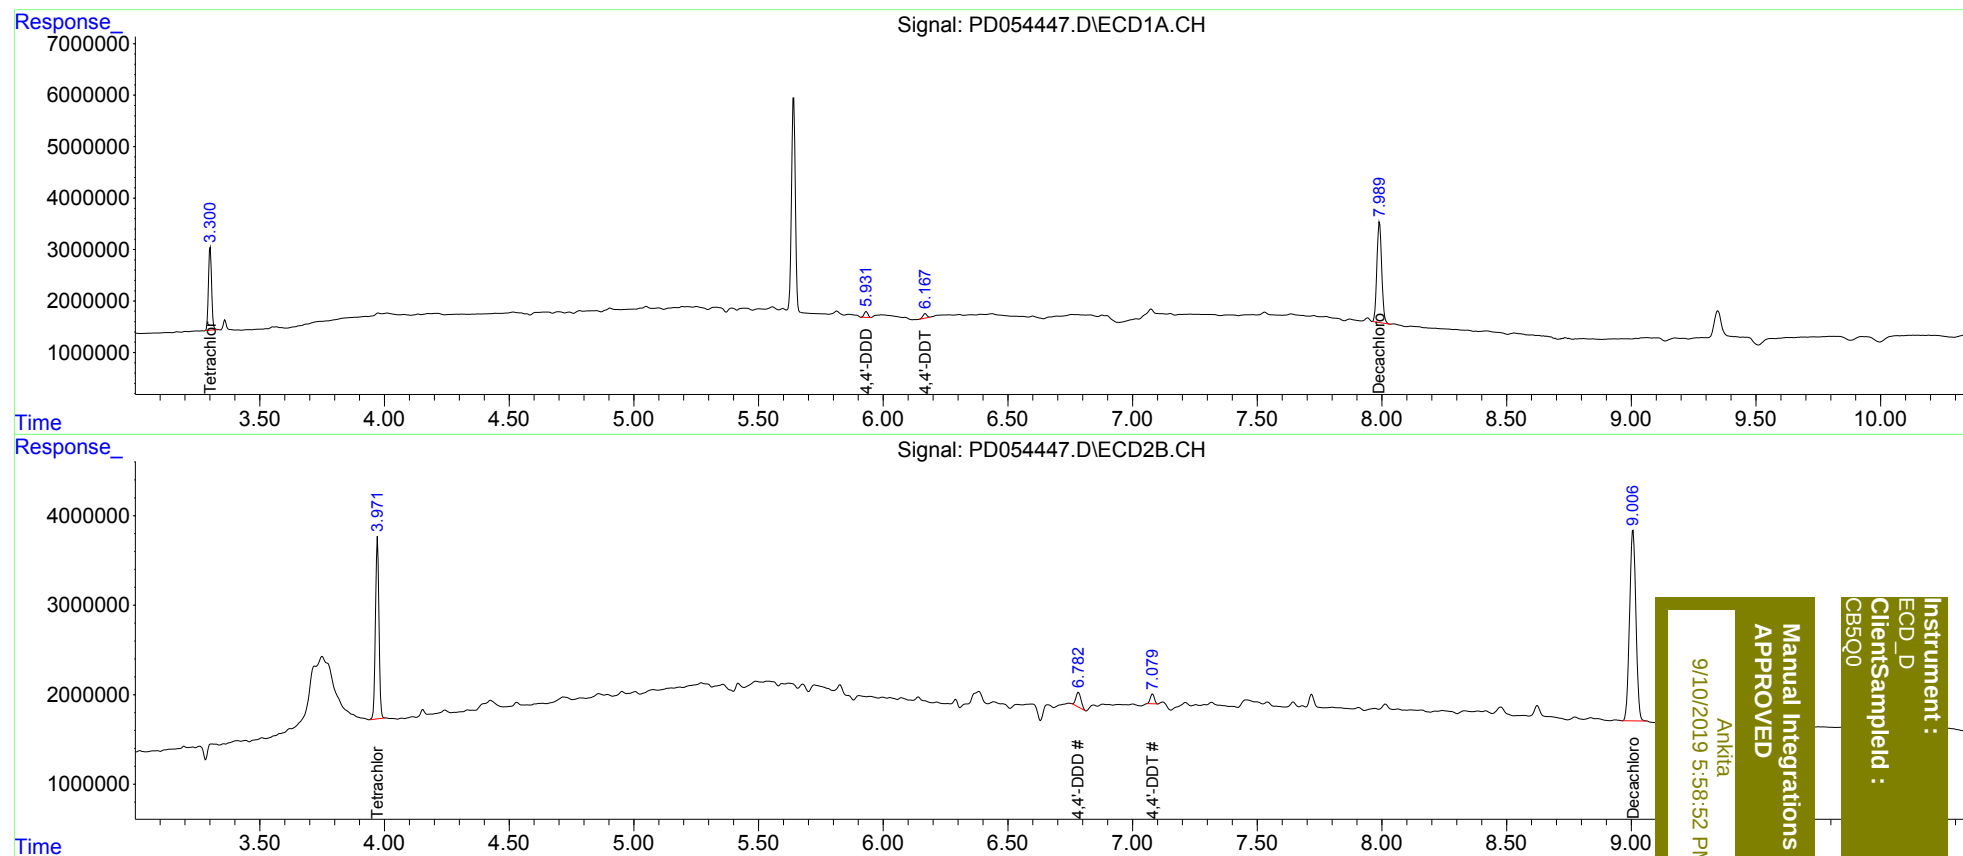

Instrument :
ECD_D
ClientSampled :
CBSQ0

Manual Integrations
APPROVED
Ankita
9/10/2019 5:58:52 PM