

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091019\
 Data File : PD054453.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Sep 2019 16:32
 Operator : SG\AJ
 Sample : K4708-09
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB5Q6

Manual Integrations
 APPROVED

Ankita
 9/10/2019 5:59:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 17:24:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090419CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 05 08:40:10 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.302	3.971	13335400	18751705	18.868	19.000
27) SA Decachlor...	7.990	9.005	25235808	35643057	37.290	38.100
Target Compounds						
10) B trans-Chl...	5.194	6.069	267254	214989	0.280m	0.156m#
11) B cis-Chlor...	5.252	6.140	187809	464075	0.209m	0.353m#
12) B 4,4'-DDE	5.420	6.294	824537	1195955	0.894m	0.865m
16) A 4,4'-DDD	5.932	6.780	635251	977071	0.918m	0.917m
17) MA 4,4'-DDT	6.168	7.079	691511	1312062	1.099m	1.263m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091019\
Data File : PD054453.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Sep 2019 16:32
Operator : SG\AJ
Sample : K4708-09
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 17:24:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090419CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 05 08:40:10 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

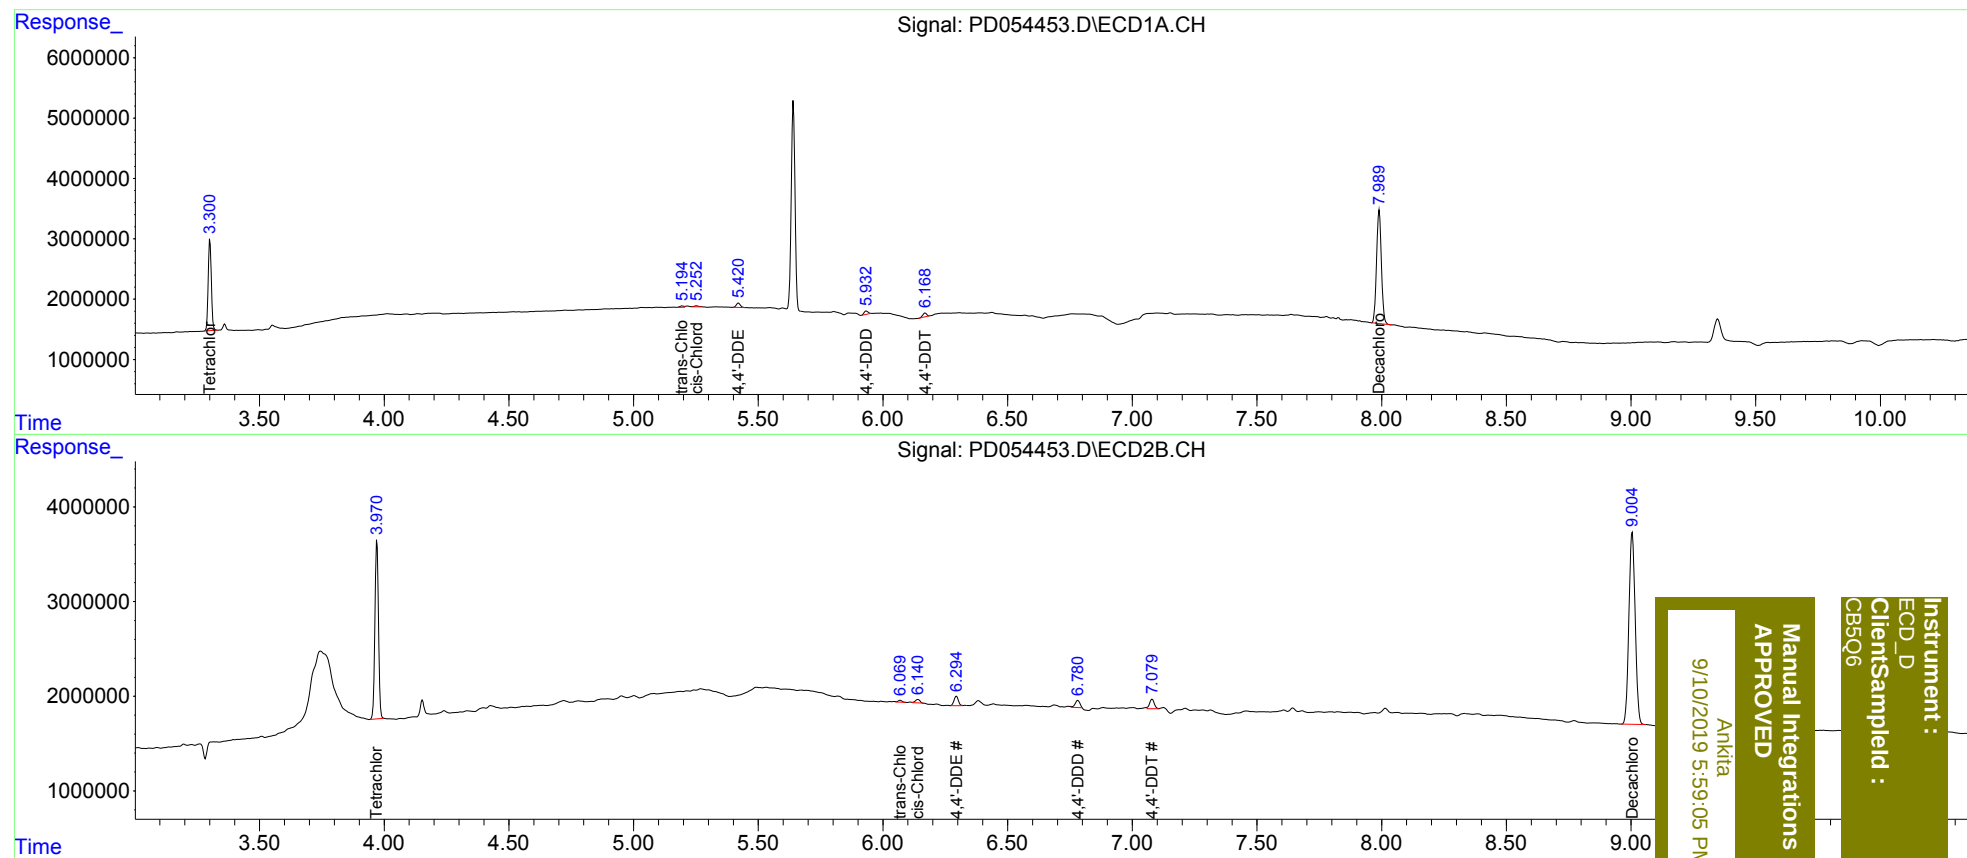

9/10/2019 5:59:05 PM
Ankita

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
CBSQ6