

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091019\
 Data File : PD054434.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Sep 2019 10:28
 Operator : SG\AJ
 Sample : K4708-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB5P9

Manual Integrations
 APPROVED

Ankita
 9/10/2019 5:58:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 13:37:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090419CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 05 08:40:10 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.302	3.972	13904165	19608838	19.673	19.868
27) SA Decachlor...	7.988	9.006	25202821	35889039	37.241m	38.363
Target Compounds						
12) B 4,4'-DDE	5.420	6.294	686522	962814	0.744m	0.697m
16) A 4,4'-DDD	5.931	6.782	565997	906595	0.818m	0.851m
17) MA 4,4'-DDT	6.166	7.078	528803	877304	0.840m	0.844m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091019\
Data File : PD054434.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Sep 2019 10:28
Operator : SG\AJ
Sample : K4708-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 13:37:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090419CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 05 08:40:10 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

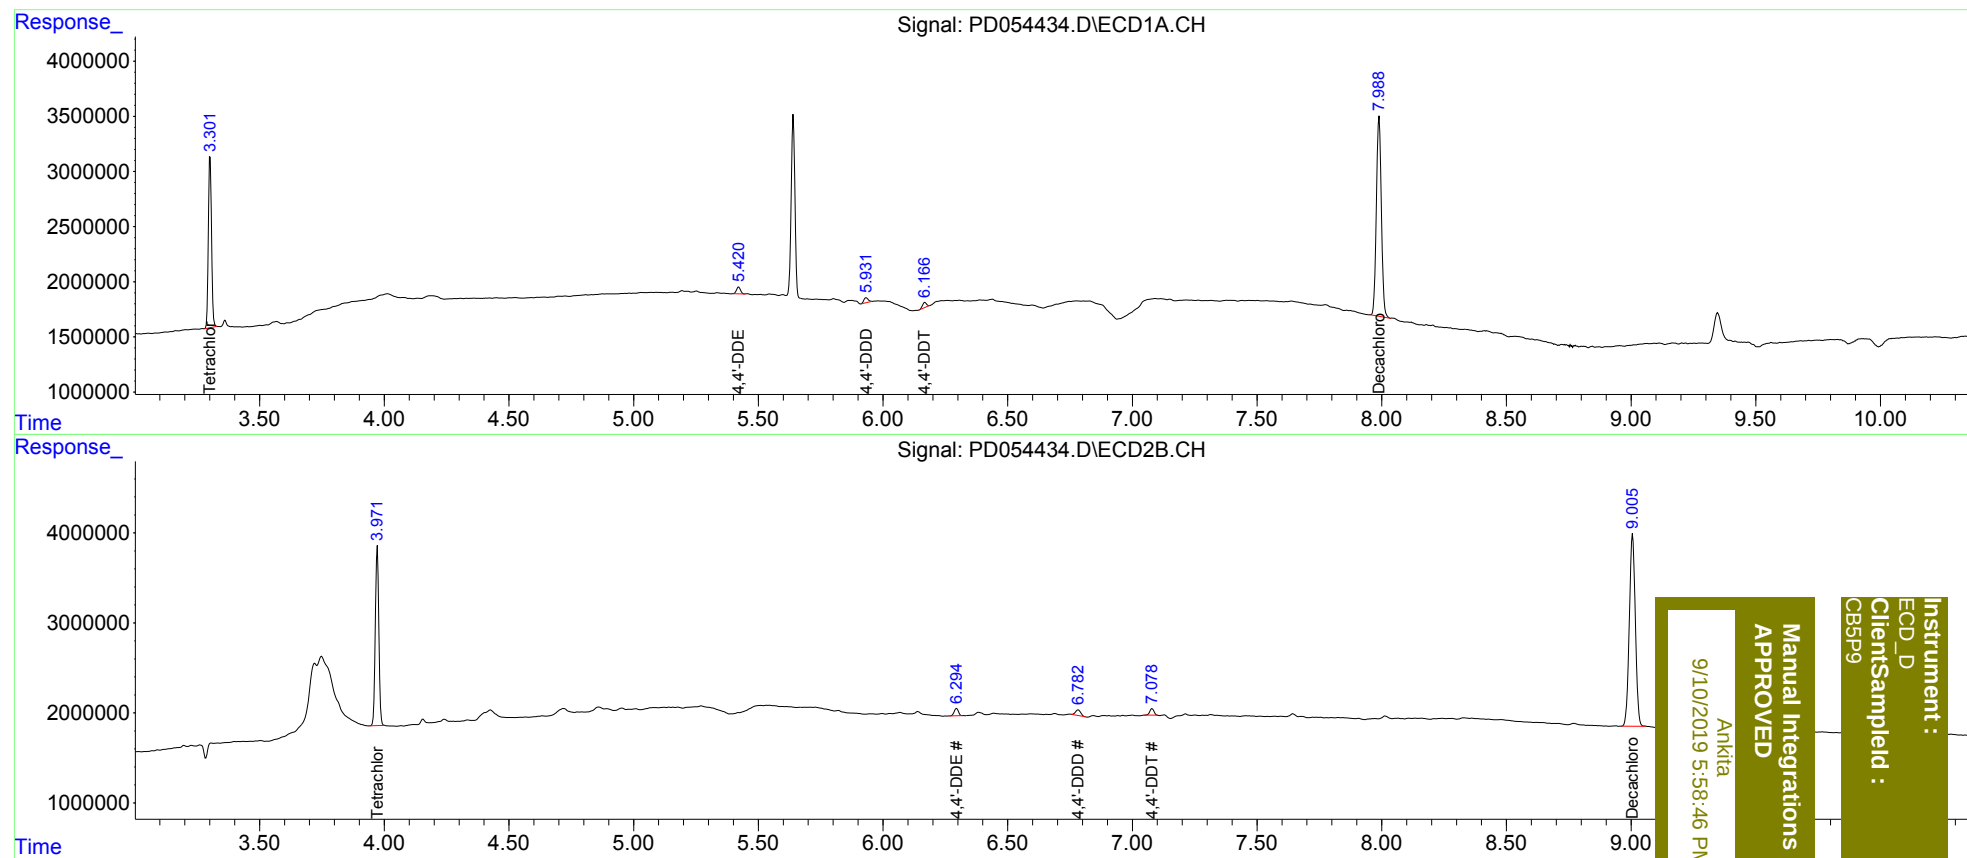

Manual Integrations
APPROVED
Ankit
9/10/2019 5:58:46 PM

Instrument :
ECD_D
ClientSampleId :
CB5P9