

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091020\
Data File : PD059153.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2020 15:20
Operator : DD\AJ
Sample : INDA328
Misc :
ALS Vial : 24 Sample Multiplier: 1


Instrument :
ECD_D
LabSampleId :
INDA328

Manual Integrations
APPROVED

Ankita
9/11/2020 11:48:59 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 04:28:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090420CLP.M
Quant Title : GC Extractables
QLast Update : Sat Sep 05 02:06:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

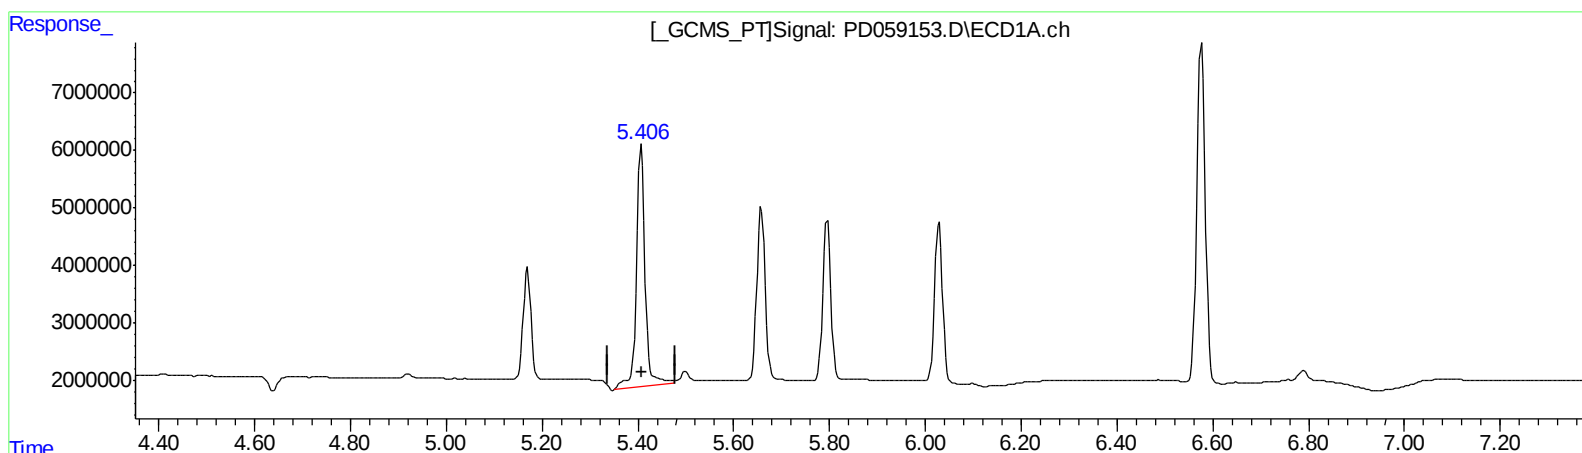

(13) Dieldrin (MA)
5.407min 47.472 ng/ml
response 53425202

(13) Dieldrin #2 (MA)
6.318min 41.449 ng/ml
response 76739828

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091020\
Data File : PD059153.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2020 15:20
Operator : DD\AJ
Sample : INDA328
Misc :
ALS Vial : 24 Sample Multiplier: 1


Instrument :
ECD_D
LabSampleId :
INDA328

Manual Integrations
APPROVED

Ankita
9/11/2020 11:48:59 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 04:28:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090420CLP.M
Quant Title : GC Extractables
QLast Update : Sat Sep 05 02:06:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

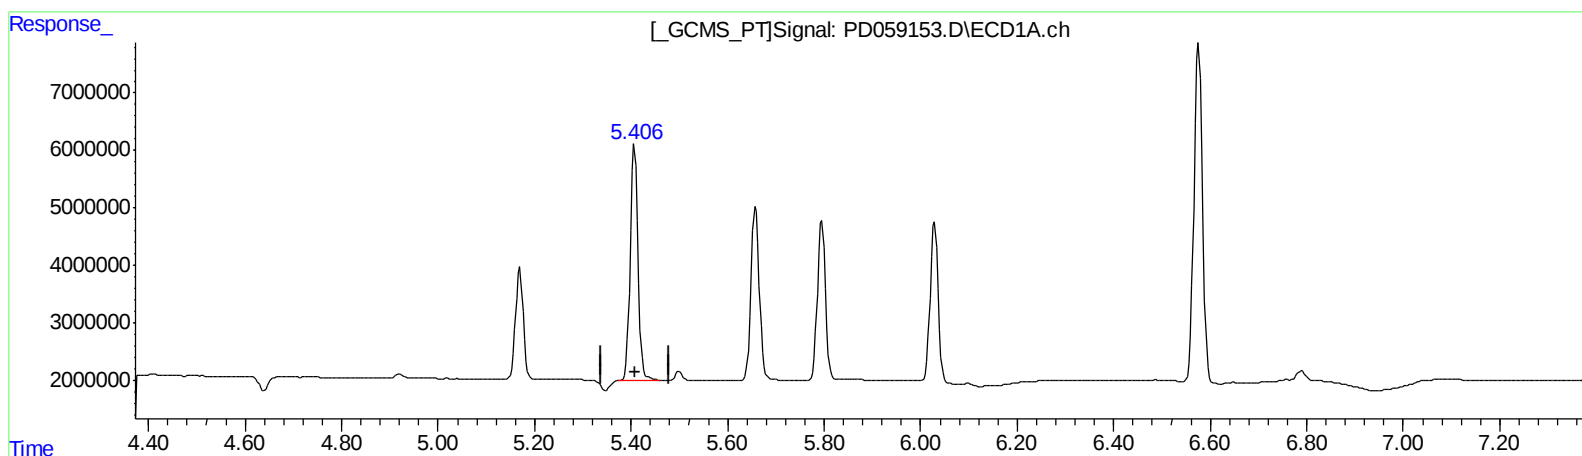

(13) Dieldrin (MA)
5.406min 41.001 ng/ml m
response 46142531

(13) Dieldrin #2 (MA)
6.318min 41.449 ng/ml
response 76739828

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091020\
 Data File : PD059153.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2020 15:20
 Operator : DD\AJ
 Sample : INDA328
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 LabSampleId :
 INDA328

Manual Integrations
 APPROVED

Ankita
 9/11/2020 11:48:59 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 04:28:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090420CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 05 02:06:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.206	3.865	20224384	35252322	20.064	21.512
27) SA Decachlor...	7.837	8.858	38878352	54083505	39.670	40.213
Target Compounds						
2) A alpha-BHC	3.627	4.247	30499954	50231465	19.440	20.692
3) MA gamma-BHC...	3.898	4.527	29917481	45921189	18.889	20.835
4) MA Heptachlor	4.177	5.027	22836261	43523091	20.333	20.659
9) A Endosulfan I	5.170	6.062	21766007	35462102	20.390	20.870
13) MA Dieldrin	5.406	6.318	46142531	76739828	41.001m	41.449
14) MA Endrin	5.658	6.534	36986224	64891665	39.905	40.255
16) A 4,4'-DDD	5.795	6.662	32367982	60145063	40.665	42.165
17) MA 4,4'-DDT	6.029	6.959	32429705	57902134	38.247	39.469
20) A Methoxychlor	6.576	7.419	72912008	158.1E6	204.645	204.877

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

AJ
 09/15/20