

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091021\
 Data File : PD065662.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2021 14:03
 Operator : AR\AJ
 Sample : M3693-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 04:02:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 09 15:08:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.494	4.013	10797675	95404985	11.018	13.017
28)	SA Decachlor...	8.237	9.085	17124522	54078521	9.933	10.135
Target Compounds							
5)	MB Aldrin	0.000	5.505	0	3313453	N.D.	0.393 #
7)	B delta-BHC	0.000	5.095	0	2203376	N.D.	0.237 #
9)	A Endosulfan I	0.000	6.228f	0	1459465	N.D.	0.207 #
11)	B alpha-Chl...	0.000	6.194	0	1738445	N.D.	0.236 #
12)	B 4,4'-DDE	5.650	6.356	620979	14089928	0.435	1.950 #
22)	Mirex	0.000	8.239f	0	969693	N.D.	0.183 #
24)	Chlordane-2	0.000	5.505f	0	3313453	N.D.	11.773 #
26)	Chlordane-4	0.000	6.194	0	1738445	N.D.	1.440 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091021\
Data File : PD065662.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2021 14:03
Operator : AR\AJ
Sample : M3693-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 04:02:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
Quant Title : GC Extractables
QLast Update : Thu Sep 09 15:08:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

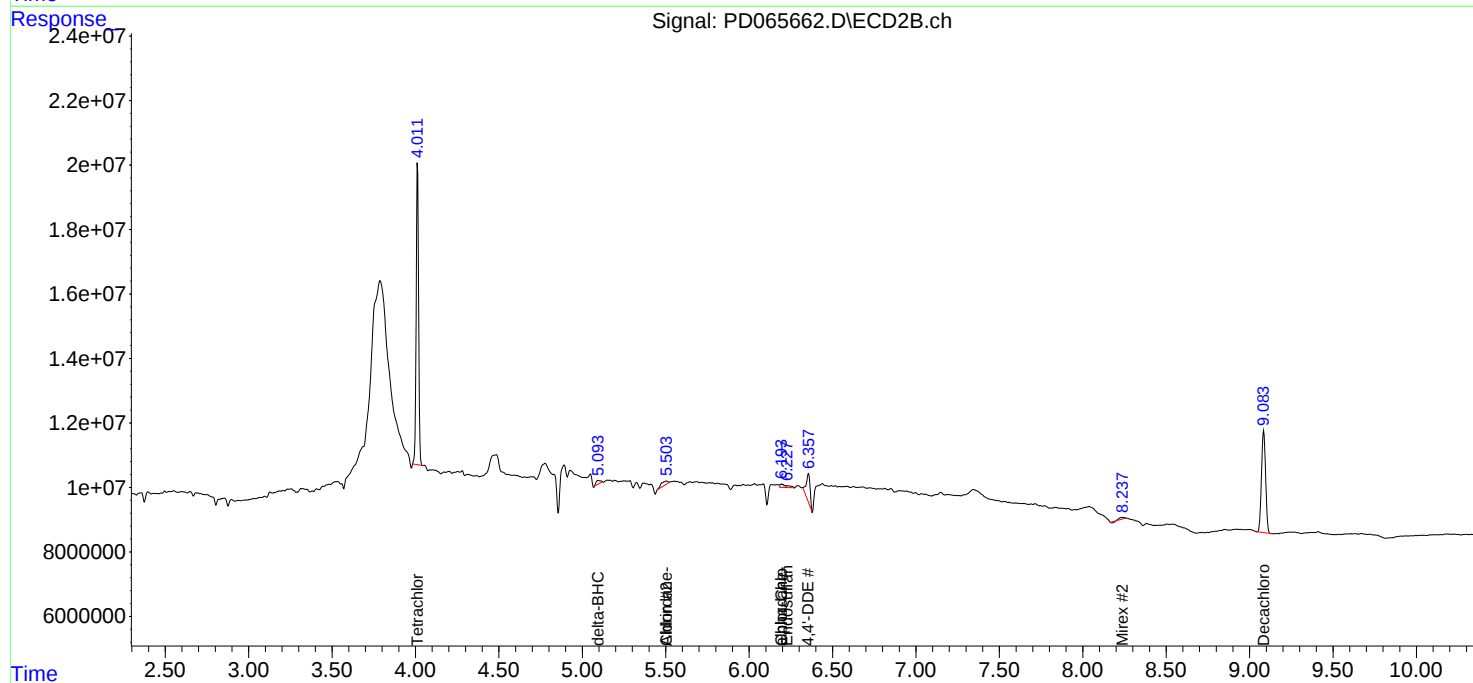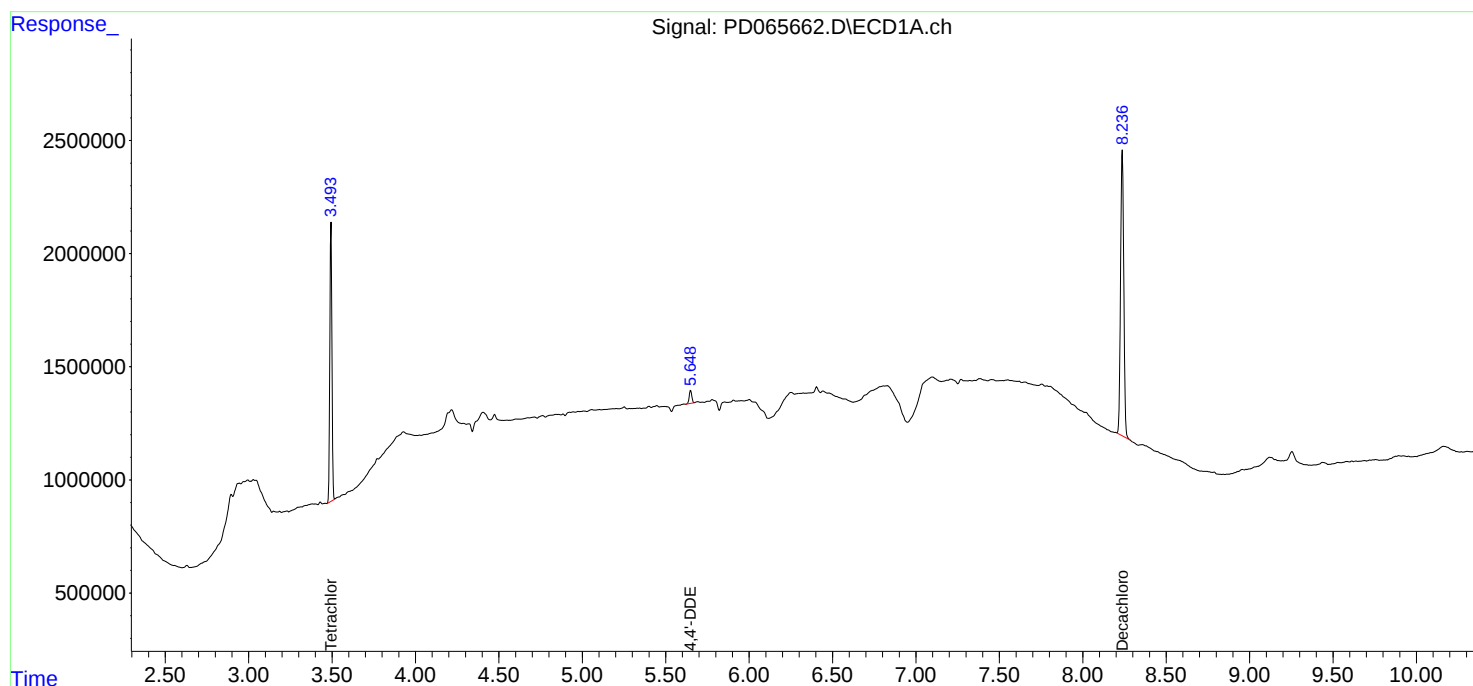


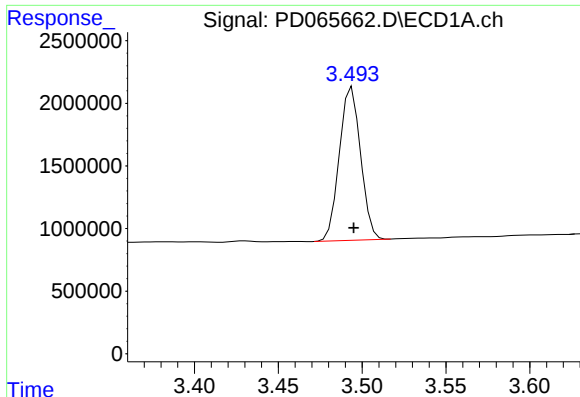

#1 Tetrachloro-m-xylene


R.T.: 3.494 min
Delta R.T.: -0.001 min
Response: 10797675
Conc: 11.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

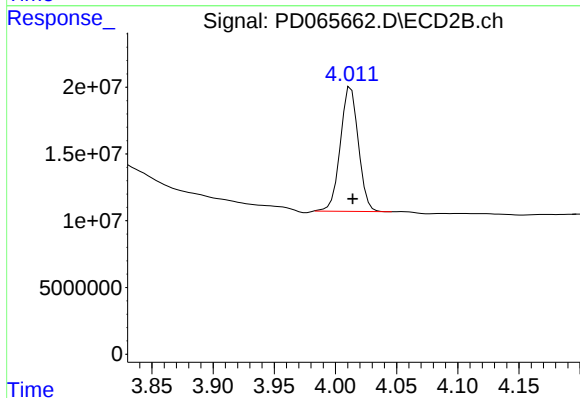


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: -0.001 min
Response: 95404985
Conc: 13.02 ng/ml

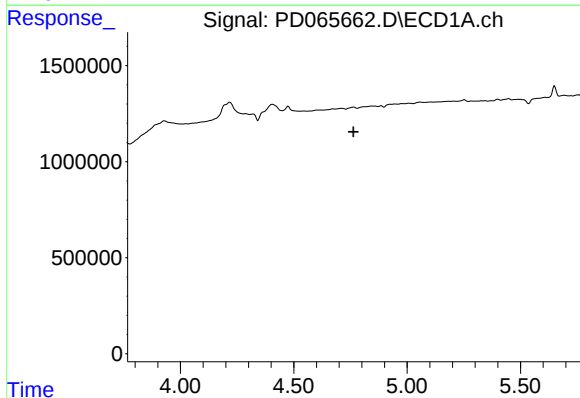


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.764 min
Response: 0
Conc: N.D.

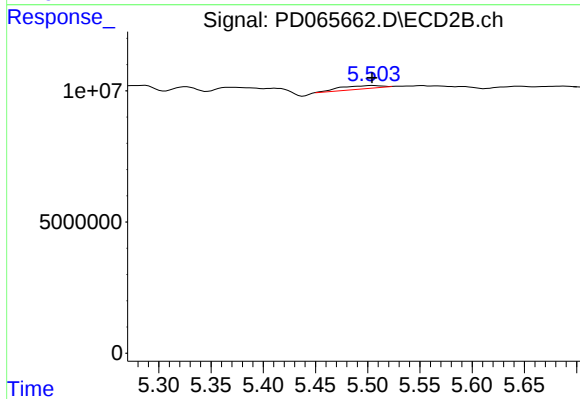

#5 Aldrin


R.T.: 5.505 min
Delta R.T.: 0.000 min
Response: 3313453
Conc: 0.39 ng/ml

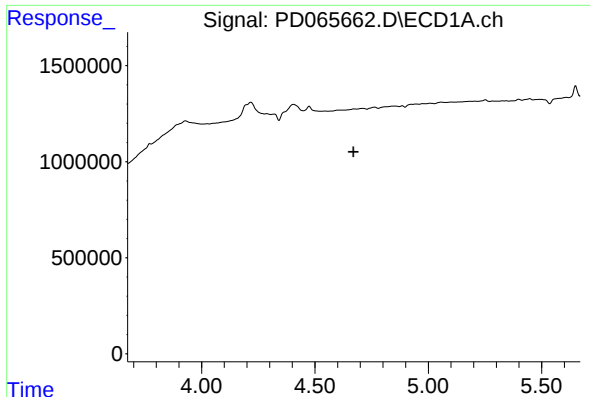

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

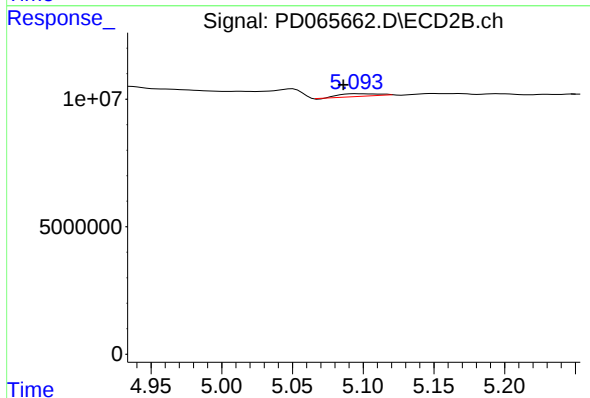


#7 delta-BHC

R.T.: 5.095 min
Delta R.T.: 0.009 min
Response: 2203376
Conc: 0.24 ng/ml

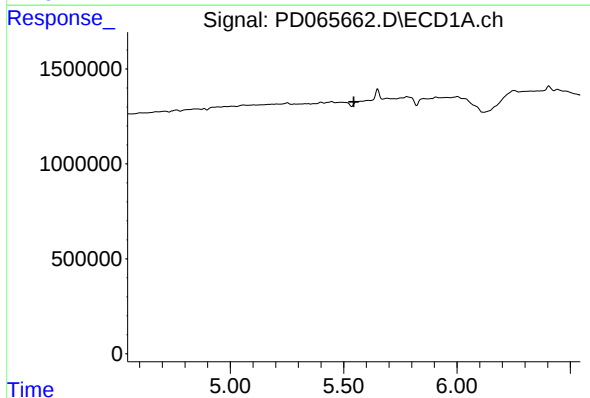


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.545 min
Response: 0
Conc: N.D.

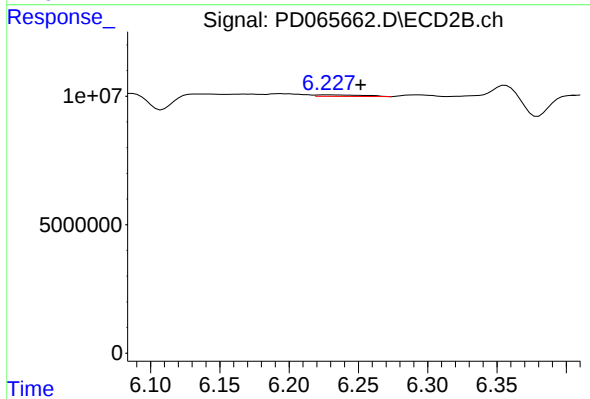

#9 Endosulfan I


R.T.: 6.228 min
Delta R.T.: -0.024 min
Response: 1459465
Conc: 0.21 ng/ml

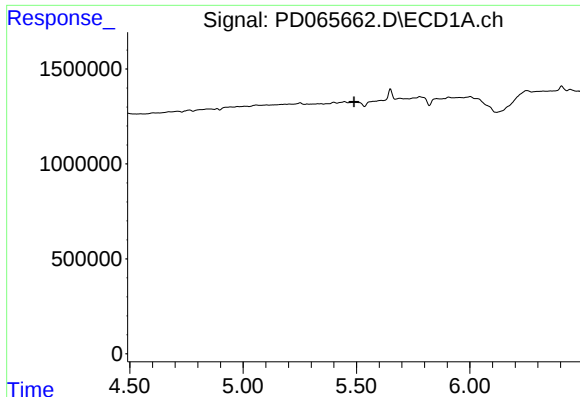

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.490 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

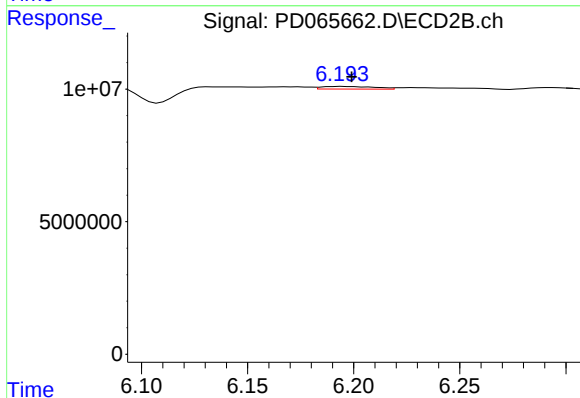


#11 alpha-Chlordane

R.T.: 6.194 min
Delta R.T.: -0.005 min
Response: 1738445
Conc: 0.24 ng/ml

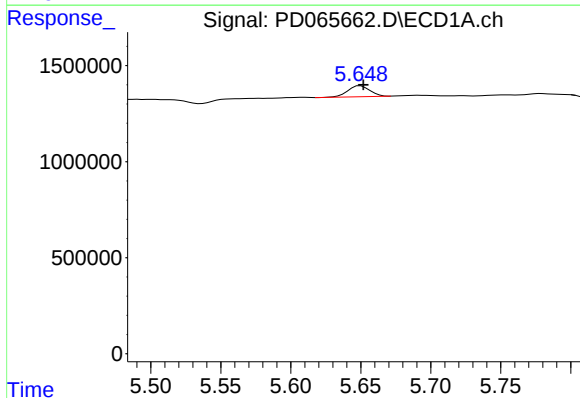


#12 4,4'-DDE

R.T.: 5.650 min
Delta R.T.: -0.002 min
Response: 620979
Conc: 0.44 ng/ml

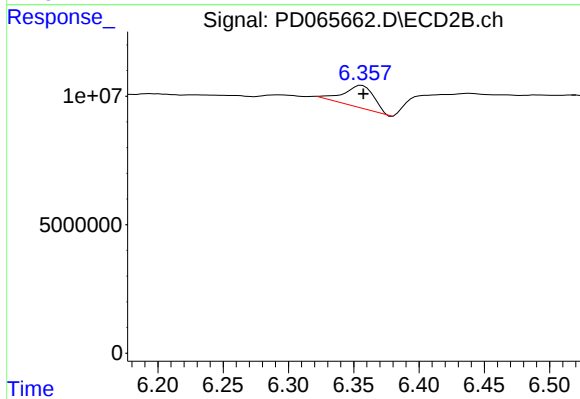

#12 4,4'-DDE


R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 14089928
Conc: 1.95 ng/ml

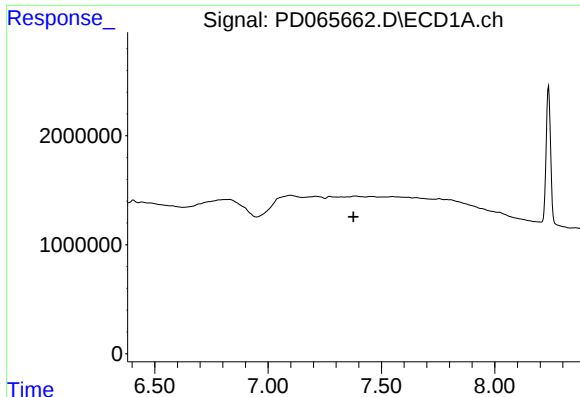

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.377 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

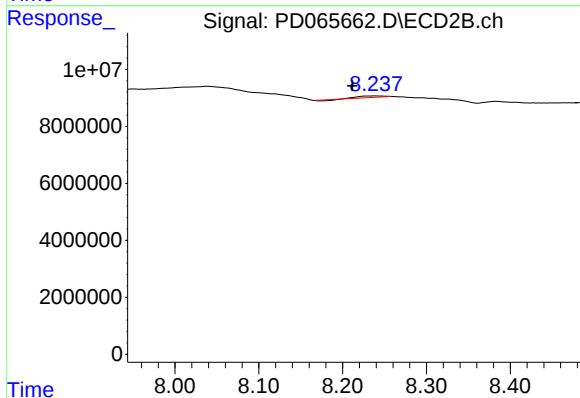


#22 Mirex

R.T.: 8.239 min
Delta R.T.: 0.028 min
Response: 969693
Conc: 0.18 ng/ml

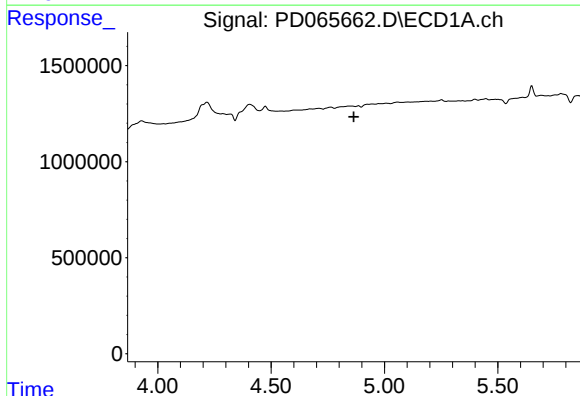


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 4.865 min
Response: 0
Conc: N.D.

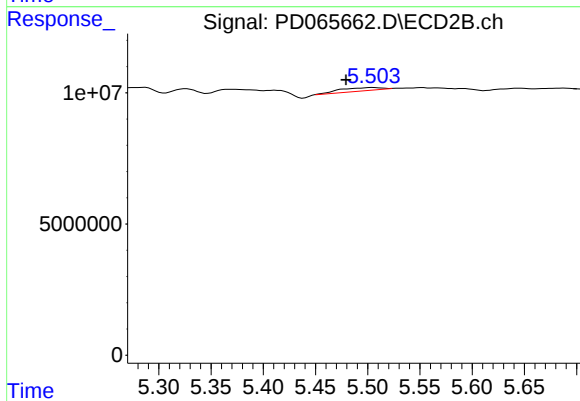

#24 Chlordane-2


R.T.: 5.505 min
Delta R.T.: 0.025 min
Response: 3313453
Conc: 11.77 ng/ml

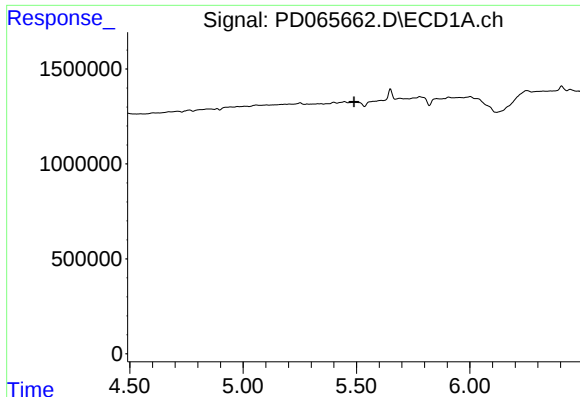

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.490 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

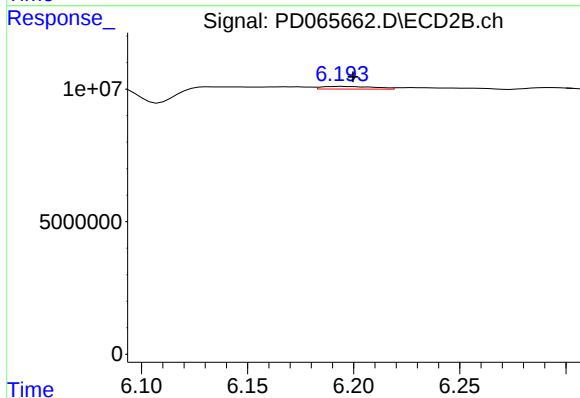


#26 Chlordane-4

R.T.: 6.194 min
Delta R.T.: -0.005 min
Response: 1738445
Conc: 1.44 ng/ml

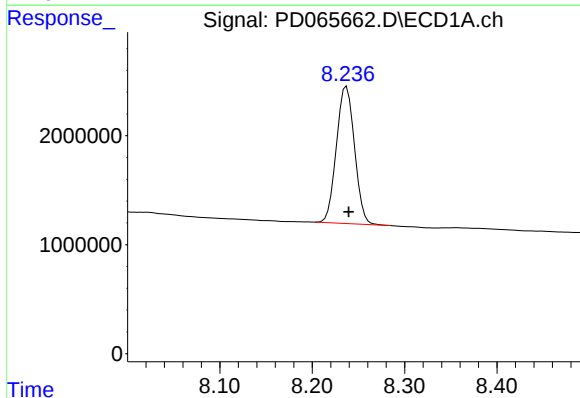

#28 Decachlorobiphenyl

R.T.: 8.237 min
Delta R.T.: -0.002 min
Response: 17124522
Conc: 9.93 ng/ml

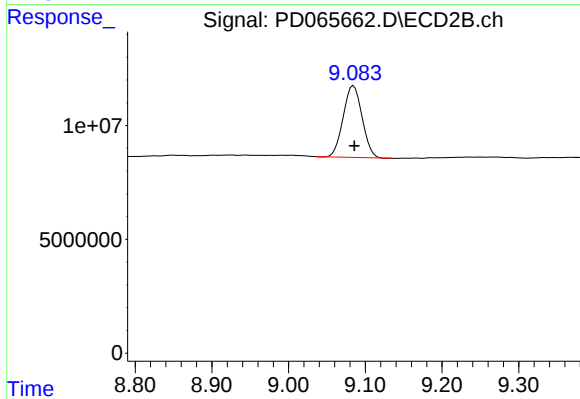

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: -0.001 min
Response: 54078521
Conc: 10.13 ng/ml