

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091021\
 Data File : PD065669.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2021 15:48
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 04:03:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 09 15:08:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.494	4.013	19742656	166.1E6	20.145	22.659
28)	SA Decachlor...	8.237	9.085	33222567	112.1E6	19.270	21.011
Target Compounds							
4)	MA Heptachlor	0.000	5.210	0	1407006	N.D.	0.155 #
8)	B Heptachlo...	0.000	5.917f	0	3680934	N.D.	0.511 #
15)	B Endosulfa...	0.000	6.941	0	1331093	N.D.	0.208 #
23)	Chlordane-1	4.392f	0.000	807349	0	19.525	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091021\
Data File : PD065669.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2021 15:48
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 04:03:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
Quant Title : GC Extractables
QLast Update : Thu Sep 09 15:08:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

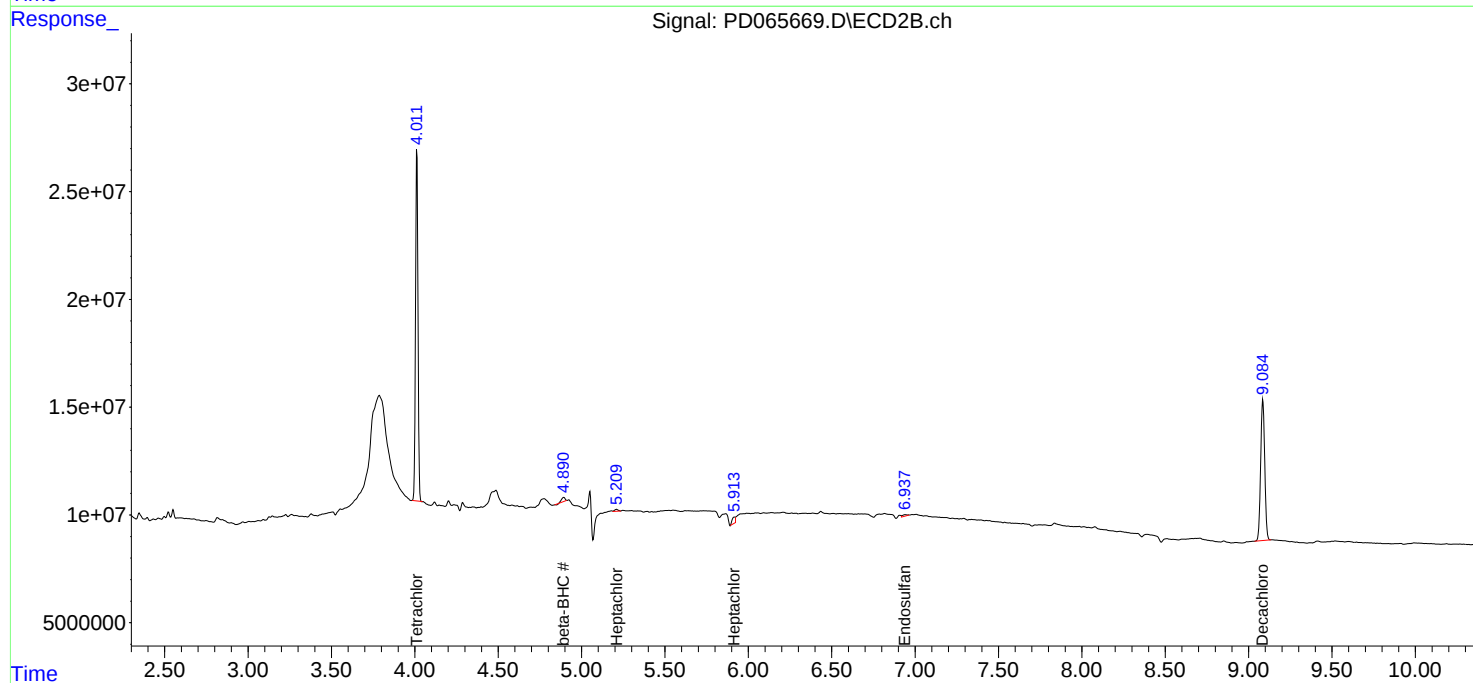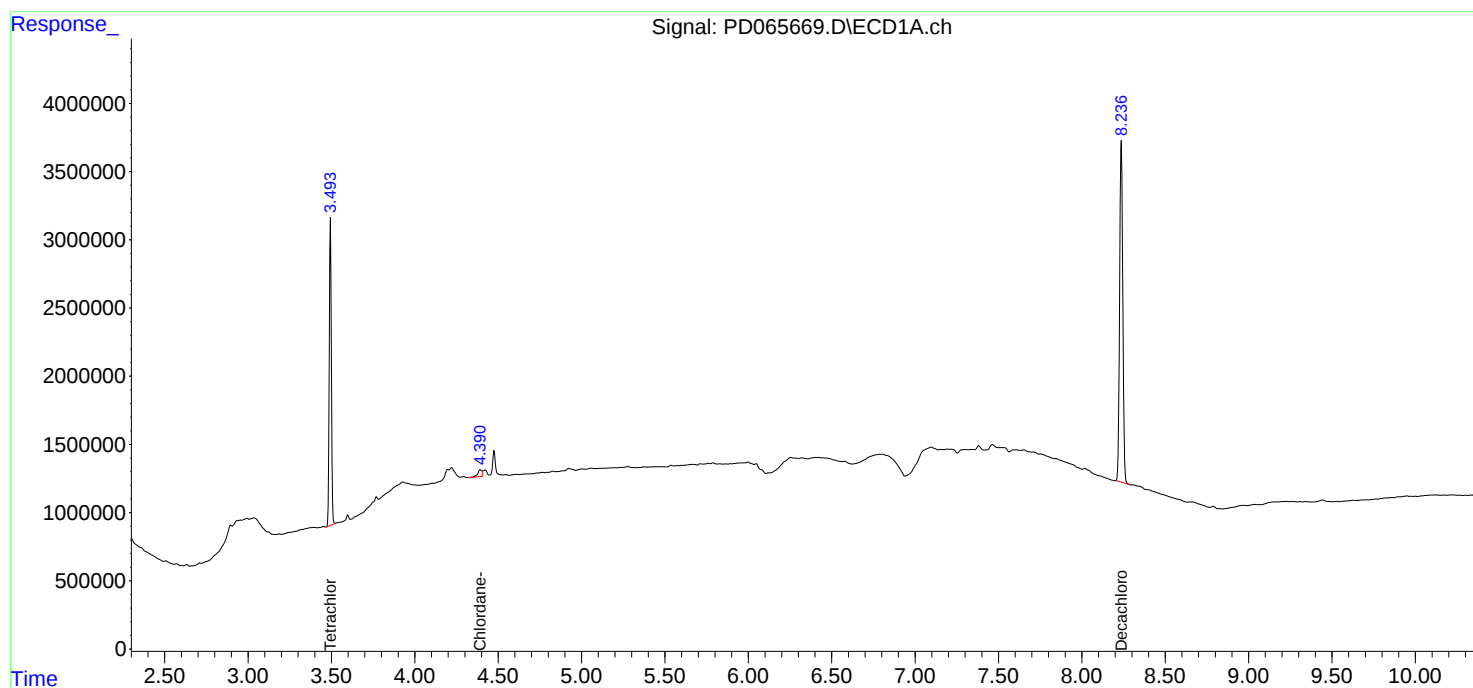


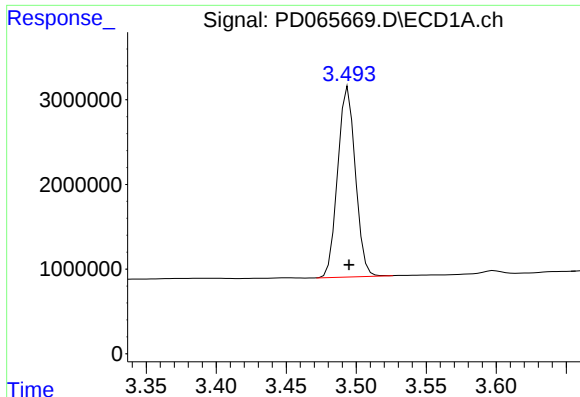

#1 Tetrachloro-m-xylene


R.T.: 3.494 min
Delta R.T.: 0.000 min
Response: 19742656
Conc: 20.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

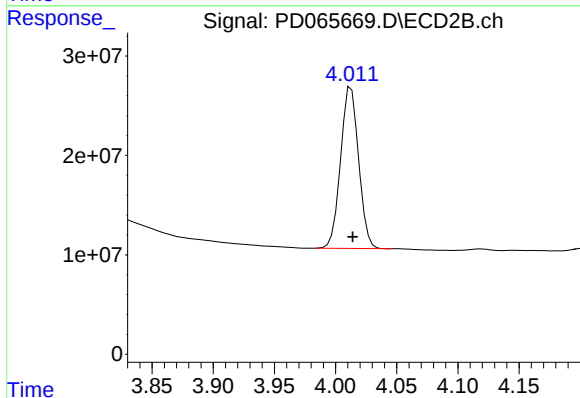


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: -0.001 min
Response: 166076442
Conc: 22.66 ng/ml

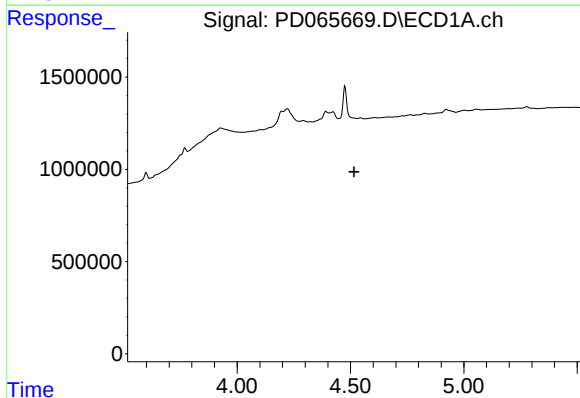


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.516 min
Response: 0
Conc: N.D.

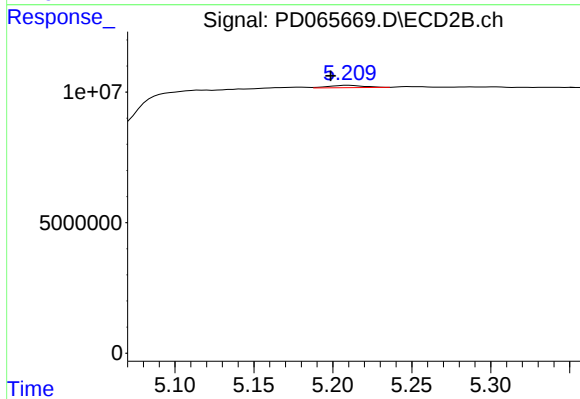

#4 Heptachlor


R.T.: 5.210 min
Delta R.T.: 0.012 min
Response: 1407006
Conc: 0.15 ng/ml

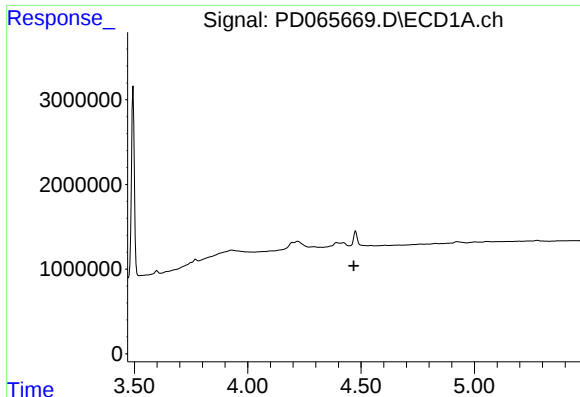

#6 beta-BHC


R.T.: 4.476 min
Delta R.T.: 0.008 min
Response: 2128075
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

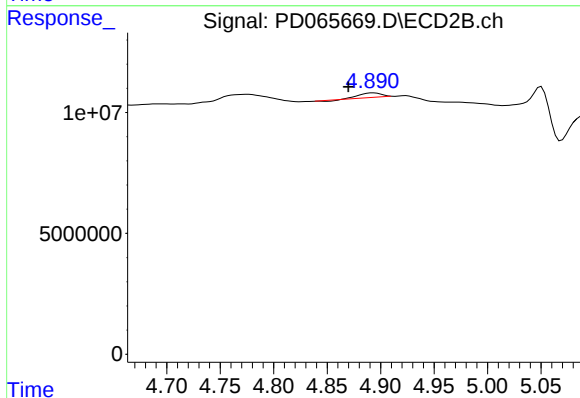


#6 beta-BHC

R.T.: 4.893 min
Delta R.T.: 0.024 min
Response: 2784443
Conc: 0.60 ng/ml

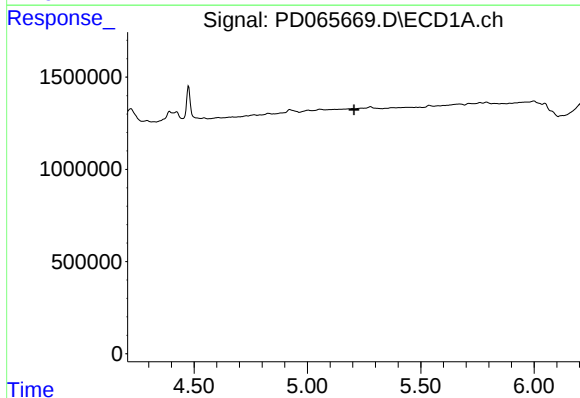


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.206 min
Response: 0
Conc: N.D.

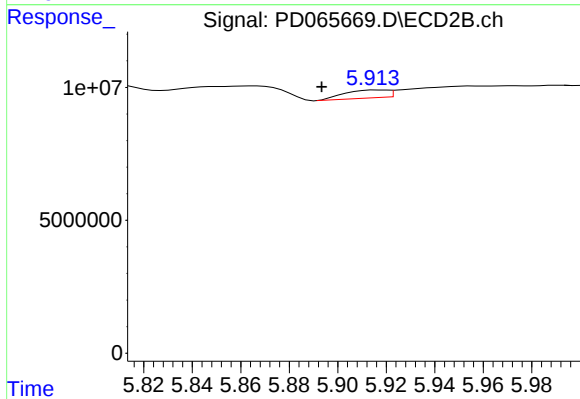

#8 Heptachlor epoxide


R.T.: 5.917 min
Delta R.T.: 0.023 min
Response: 3680934
Conc: 0.51 ng/ml

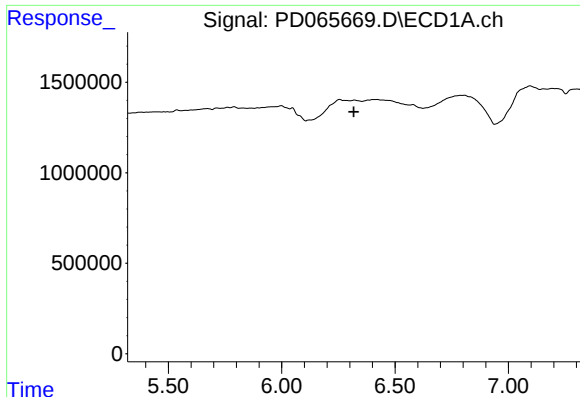

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.318 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

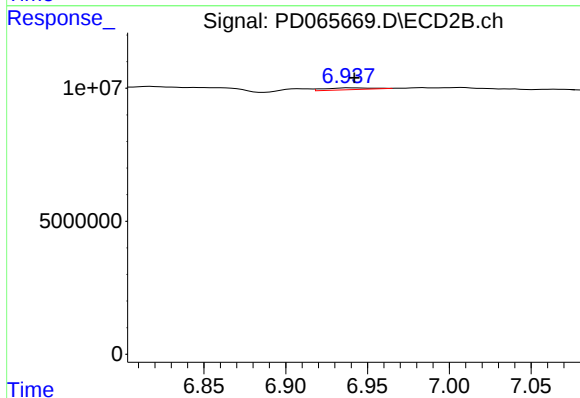


#15 Endosulfan II

R.T.: 6.941 min
Delta R.T.: -0.001 min
Response: 1331093
Conc: 0.21 ng/ml

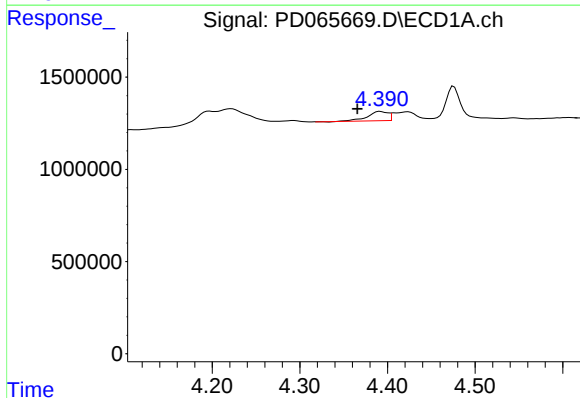


#23 Chlordane-1

R.T.: 4.392 min
Delta R.T.: 0.026 min
Response: 807349
Conc: 19.52 ng/ml

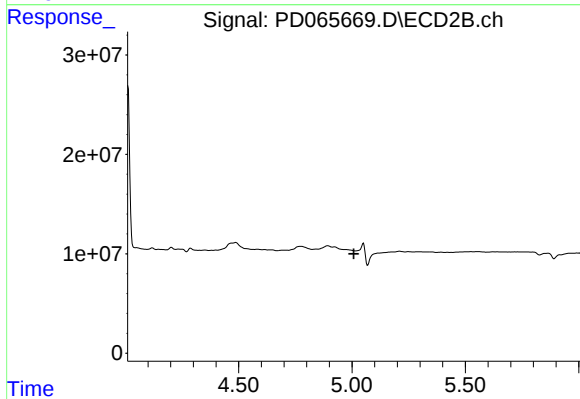

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.008 min
Response: 0
Conc: N.D.

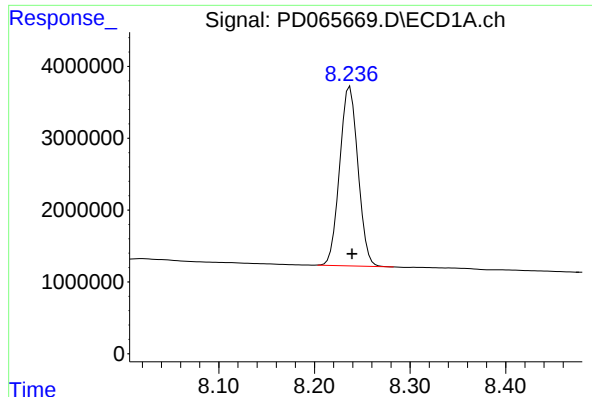

#28 Decachlorobiphenyl

R.T.: 8.237 min
Delta R.T.: -0.002 min
Response: 33222567
Conc: 19.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

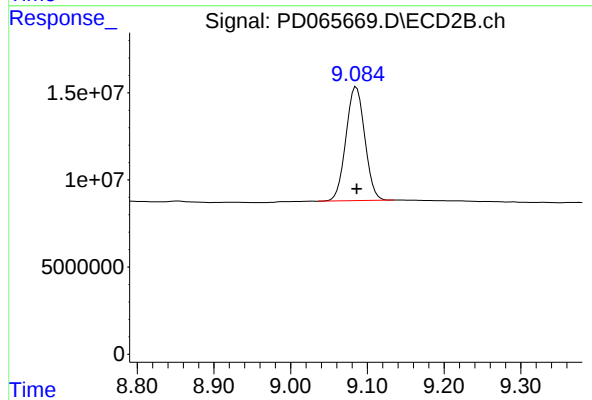

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 112115121
Conc: 21.01 ng/ml