

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091021\
 Data File : PD065672.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2021 16:31
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 04:03:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 09 15:08:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.494	4.013	19661116	164.4E6	20.062	22.426
28)	SA Decachlor...	8.237	9.086	31092556	106.4E6	18.034	19.932
Target Compounds							
8)	B Heptachlo...	0.000	5.910f	0	846312	N.D.	0.118 #
21)	B Endrin ke...	0.000	7.744f	0	414935	N.D.	0.055 #
23)	Chlordane-1	4.393f	0.000	1615113	0	39.060	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091021\
Data File : PD065672.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2021 16:31
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 04:03:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
Quant Title : GC Extractables
QLast Update : Thu Sep 09 15:08:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

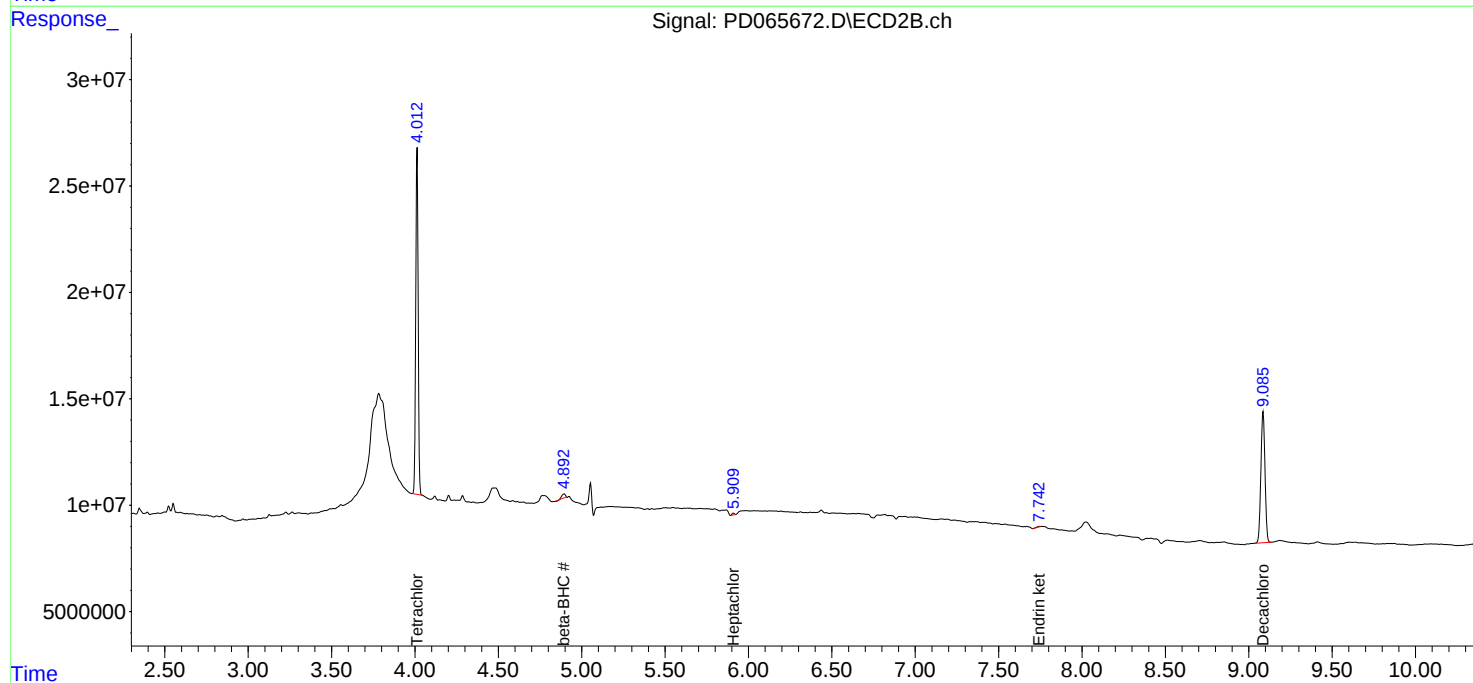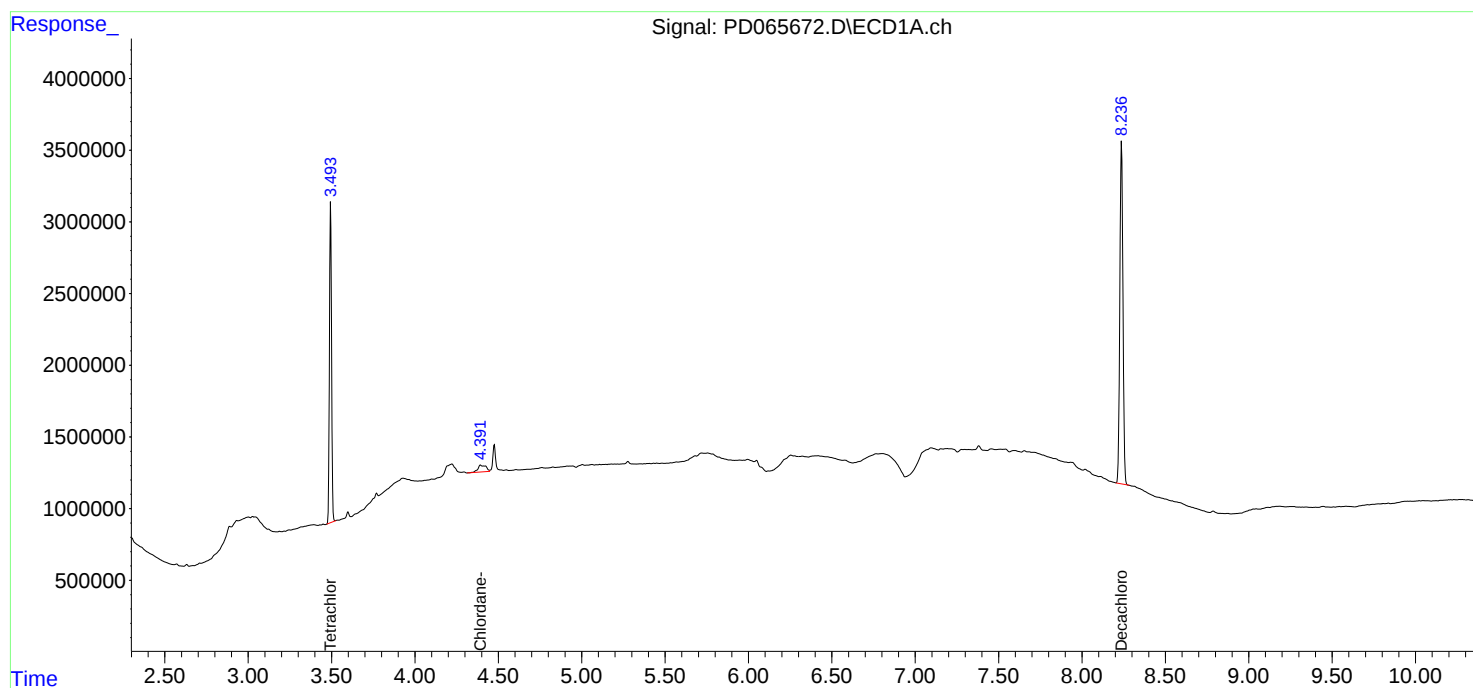


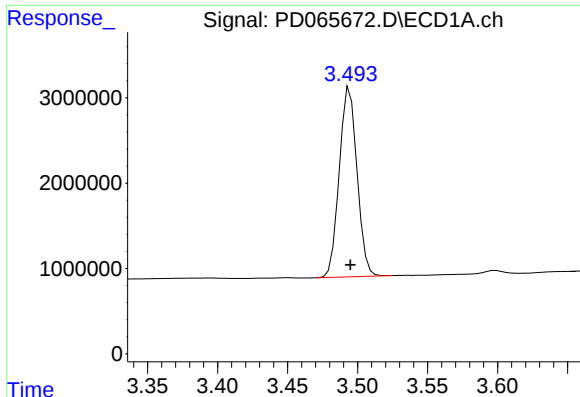

#1 Tetrachloro-m-xylene


R.T.: 3.494 min
Delta R.T.: 0.000 min
Response: 19661116
Conc: 20.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

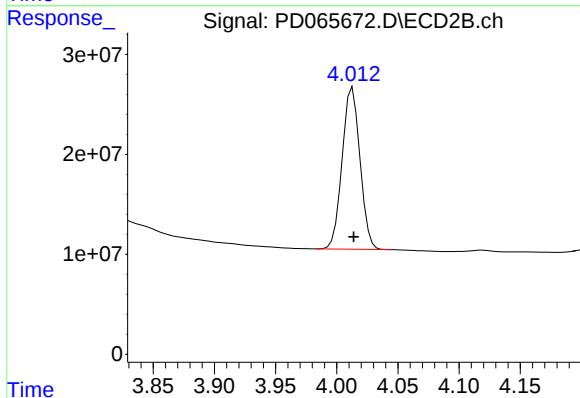


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: -0.001 min
Response: 164369660
Conc: 22.43 ng/ml

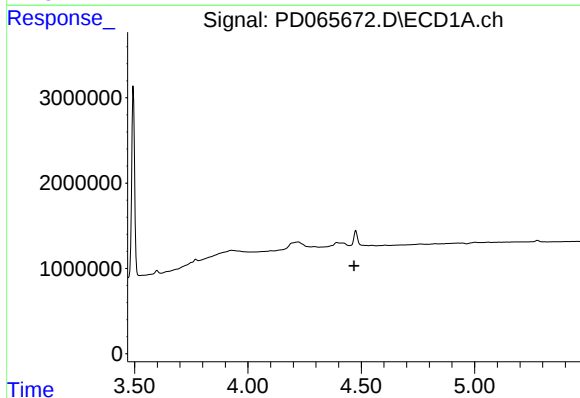


#6 beta-BHC

R.T.: 4.476 min
Delta R.T.: 0.008 min
Response: 2199139
Conc: N.D.

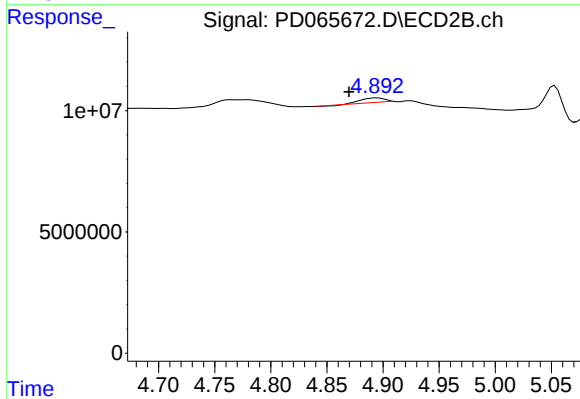

#6 beta-BHC


R.T.: 4.895 min
Delta R.T.: 0.025 min
Response: 3017535
Conc: 0.65 ng/ml

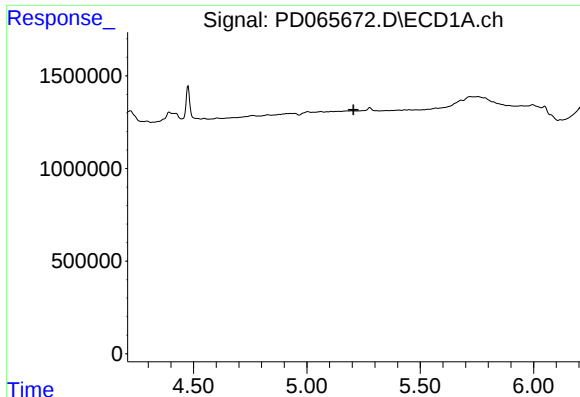

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.206 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

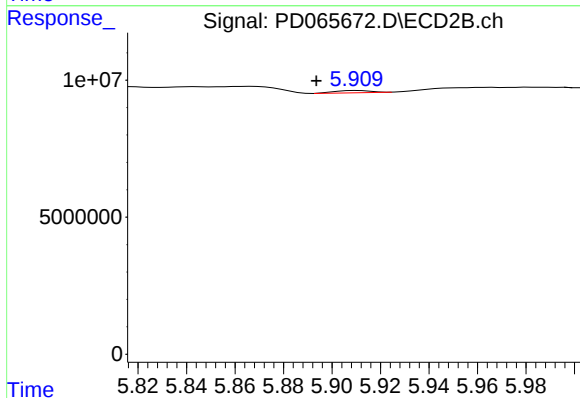


#8 Heptachlor epoxide

R.T.: 5.910 min
Delta R.T.: 0.017 min
Response: 846312
Conc: 0.12 ng/ml

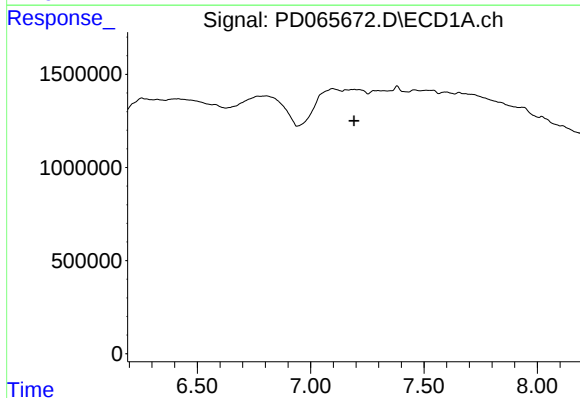


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.192 min
Response: 0
Conc: N.D.

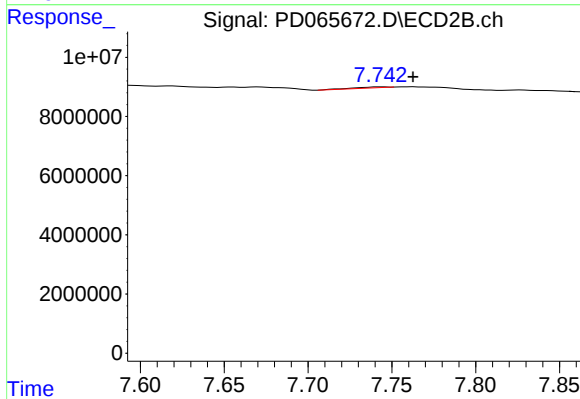

#21 Endrin ketone


R.T.: 7.744 min
Delta R.T.: -0.019 min
Response: 414935
Conc: 0.05 ng/ml

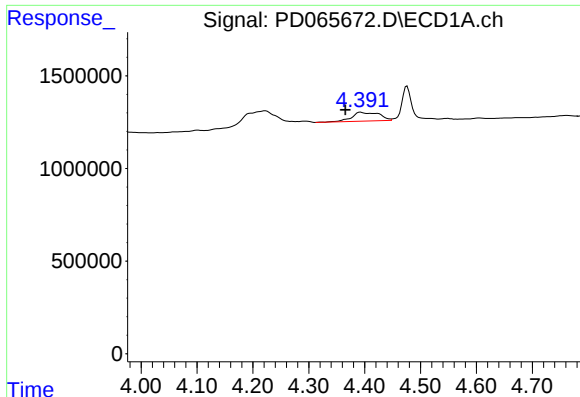

#23 Chlordane-1


R.T.: 4.393 min
Delta R.T.: 0.027 min
Response: 1615113
Conc: 39.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

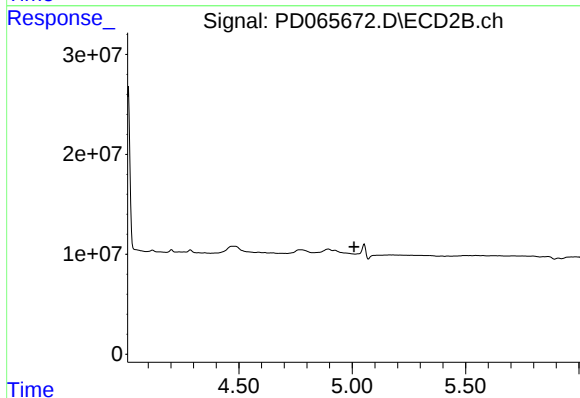


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.008 min
Response: 0
Conc: N.D.

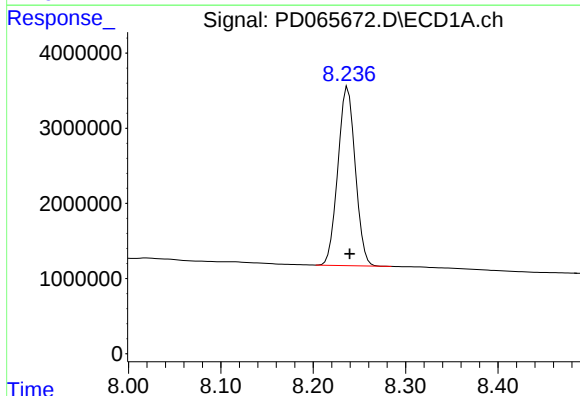

#28 Decachlorobiphenyl

R.T.: 8.237 min
Delta R.T.: -0.002 min
Response: 31092556
Conc: 18.03 ng/ml

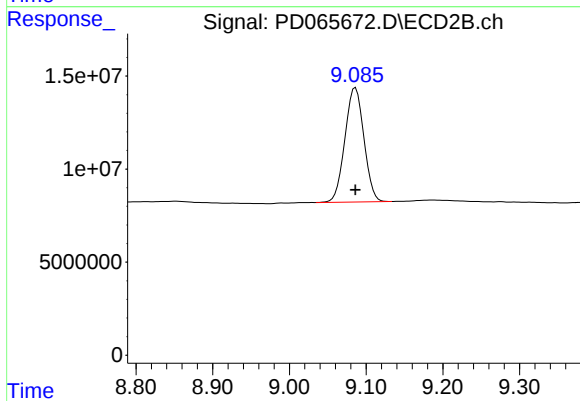

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.000 min
Response: 106355051
Conc: 19.93 ng/ml