

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091021\
 Data File : PD065658.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2021 13:08
 Operator : AR\AJ
 Sample : M3685-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 327

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 04:01:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 09 15:08:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.494	4.012	10231199	68588239	10.440	9.358
28)	SA Decachlor...	8.235	9.086	26260693	79247704	15.232m	14.852
Target Compounds							
4)	MA Heptachlor	4.515	5.197	4418784	24005115	2.911	2.640m
7)	B delta-BHC	4.672	5.078	1112477	11087868	0.746	1.193m#
10)	B gamma-Chl...	5.432	6.124	88139467	715.0E6	57.707m	95.214m#
11)	B alpha-Chl...	5.487	6.199	204.1E6	1643.1E6	135.611m	223.102 #
12)	B 4,4'-DDE	5.649	6.356	28393815	201.8E6	19.913m	27.935 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091021\
Data File : PD065658.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2021 13:08
Operator : AR\AJ
Sample : M3685-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
327

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 04:01:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
Quant Title : GC Extractables
QLast Update : Thu Sep 09 15:08:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

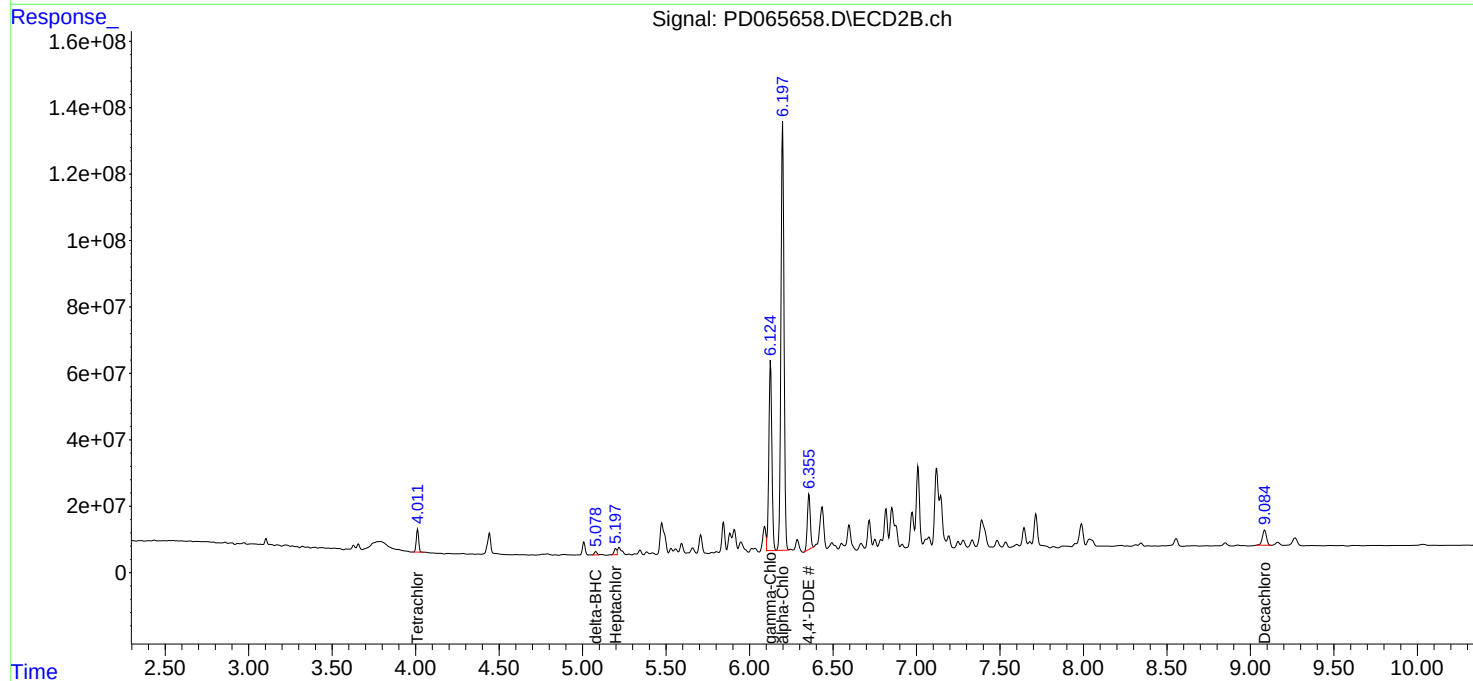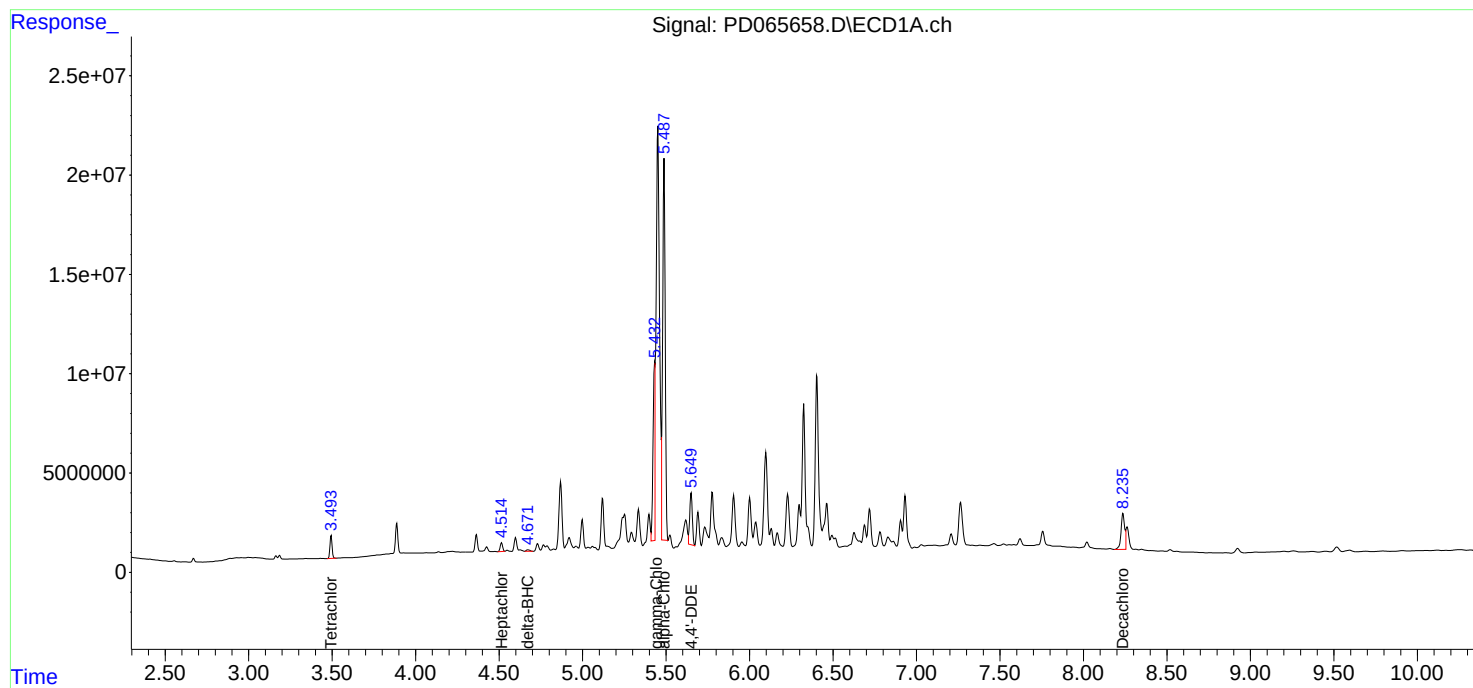


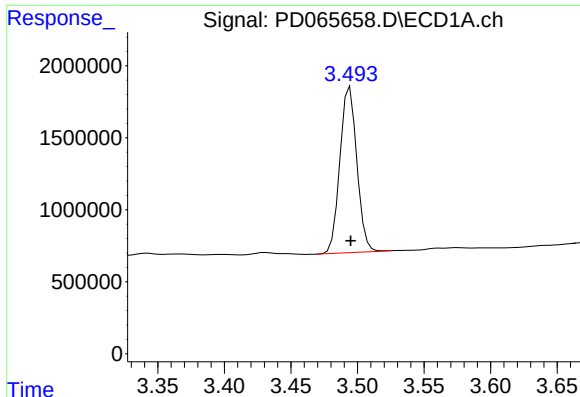

#1 Tetrachloro-m-xylene


R.T.: 3.494 min
Delta R.T.: 0.000 min
Response: 10231199
Conc: 10.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
327

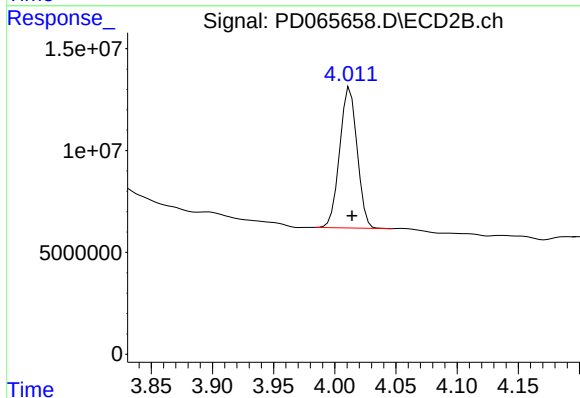


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: -0.002 min
Response: 68588239
Conc: 9.36 ng/ml

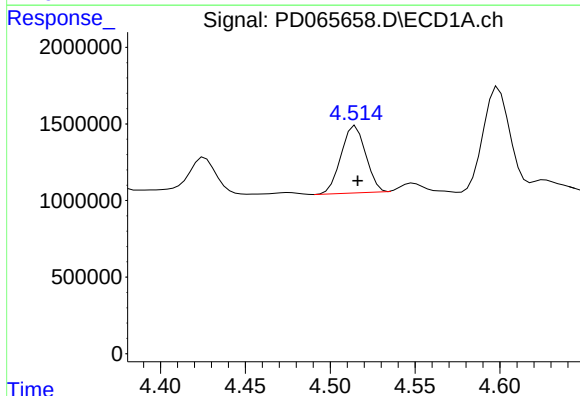


#4 Heptachlor

R.T.: 4.515 min
Delta R.T.: -0.001 min
Response: 4418784
Conc: 2.91 ng/ml

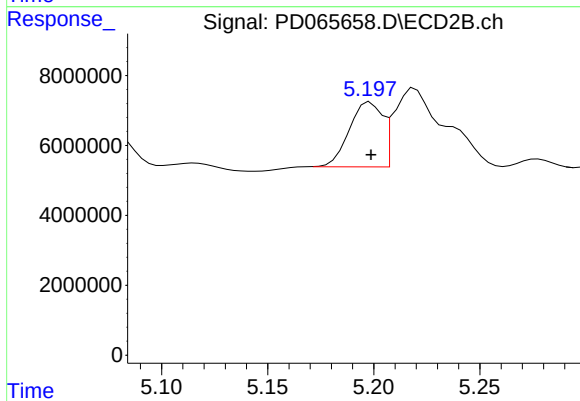

#4 Heptachlor


R.T.: 5.197 min
Delta R.T.: -0.002 min
Response: 24005115
Conc: 2.64 ng/ml m

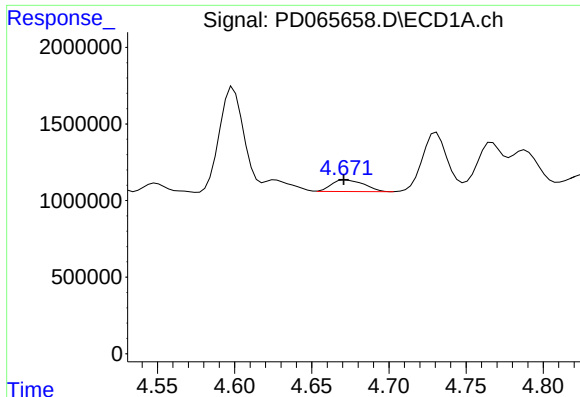

#7 delta-BHC


R.T.: 4.672 min
Delta R.T.: 0.001 min
Response: 1112477
Conc: 0.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
327

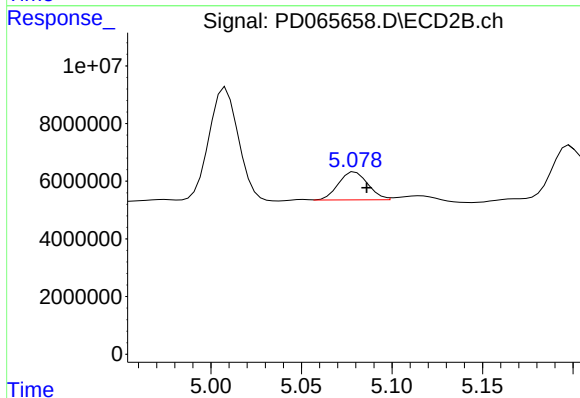


#7 delta-BHC

R.T.: 5.078 min
Delta R.T.: -0.008 min
Response: 11087868
Conc: 1.19 ng/ml m

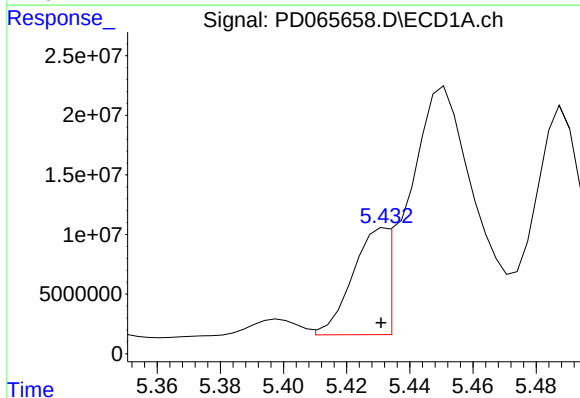


#10 gamma-Chlordane

R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 88139467
Conc: 57.71 ng/ml m

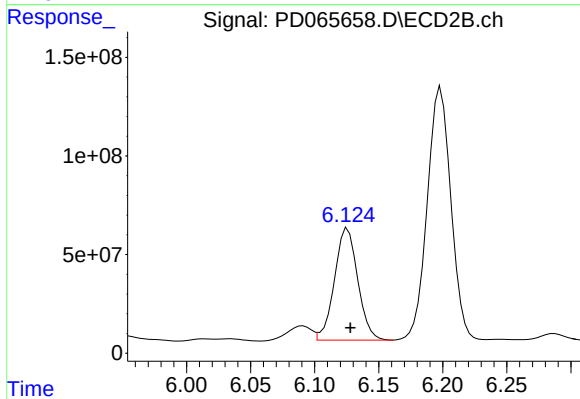

#10 gamma-Chlordane


R.T.: 6.124 min
Delta R.T.: -0.003 min
Response: 714990107
Conc: 95.21 ng/ml m

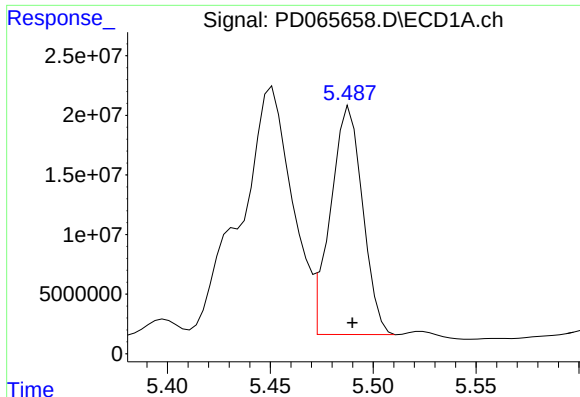

#11 alpha-Chlordane


R.T.: 5.487 min
Delta R.T.: -0.003 min
Response: 204142098
Conc: 135.61 ng/ml m

Instrument :
ECD_D
ClientSampleId :
327

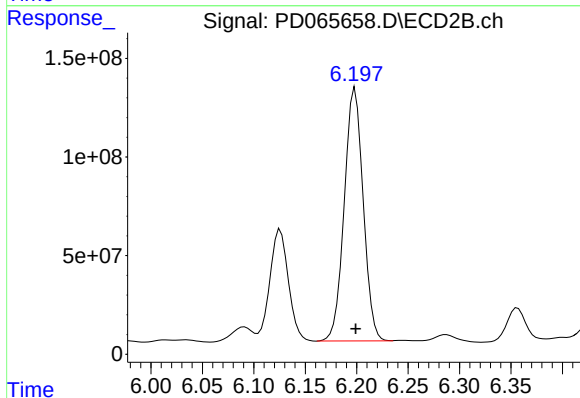


#11 alpha-Chlordane

R.T.: 6.199 min
Delta R.T.: 0.000 min
Response: 1643141802
Conc: 223.10 ng/ml

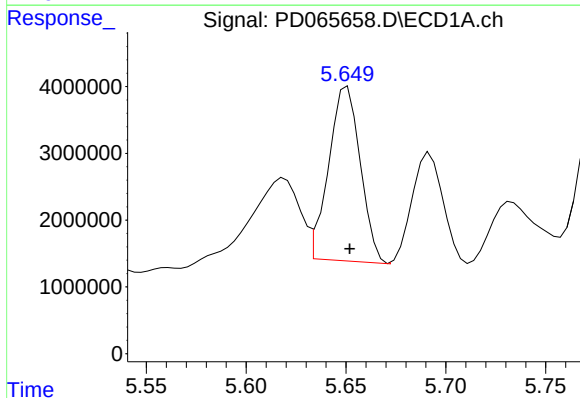


#12 4,4'-DDE

R.T.: 5.649 min
Delta R.T.: -0.003 min
Response: 28393815
Conc: 19.91 ng/ml m

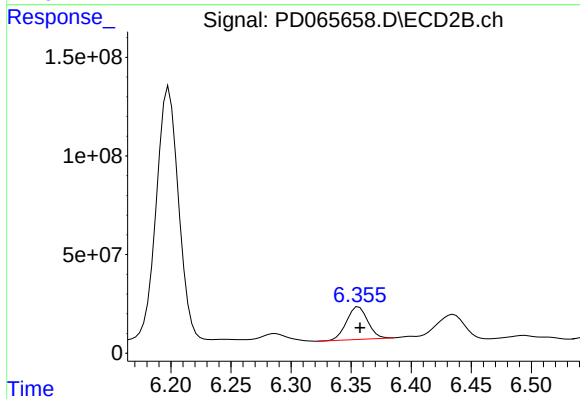

#12 4,4'-DDE


R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 201827537
Conc: 27.94 ng/ml

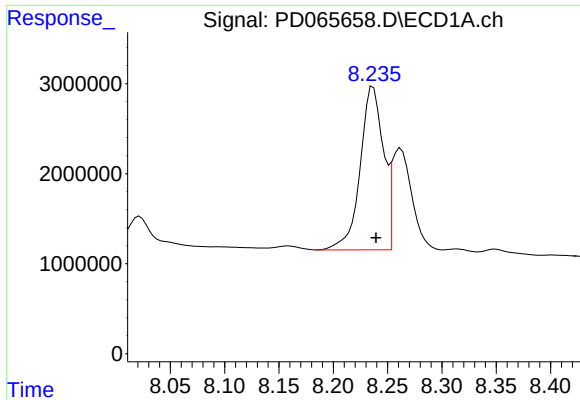

#28 Decachlorobiphenyl

R.T.: 8.235 min
Delta R.T.: -0.004 min
Response: 26260693
Conc: 15.23 ng/ml m

Instrument :
ECD_D
ClientSampleId :
327

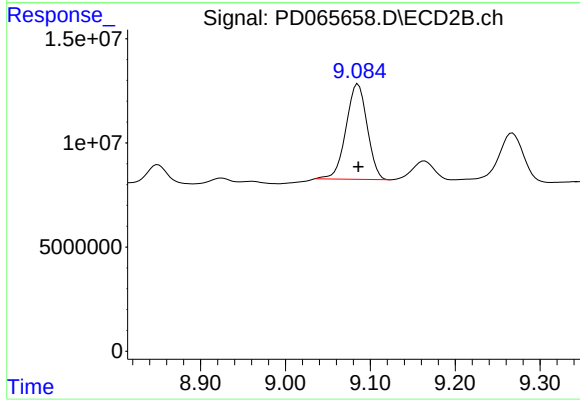

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.000 min
Response: 79247704
Conc: 14.85 ng/ml