

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091021\
 Data File : PD065668.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2021 15:34
 Operator : AR\AJ
 Sample : M3685-01DL 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 327DL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 04:03:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 09 15:08:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.494	4.012	2542544	21213851	2.594	2.894
28) SA Decachlor...	8.237	9.085	6508999	20520445	3.775	3.846
Target Compounds						
4) MA Heptachlor	4.514	5.197	1191750	5646528	0.785	0.621m
10) B gamma-Chl...	5.432	6.124	14463428	212.1E6	9.469m	28.245m#
11) B alpha-Chl...	5.487	6.199	48125403	489.3E6	31.970m	66.433 #
12) B 4,4'-DDE	5.649	6.356	7401291	70282171	5.191m	9.728 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091021\
Data File : PD065668.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2021 15:34
Operator : AR\AJ
Sample : M3685-01DL 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
327DL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 04:03:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
Quant Title : GC Extractables
QLast Update : Thu Sep 09 15:08:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

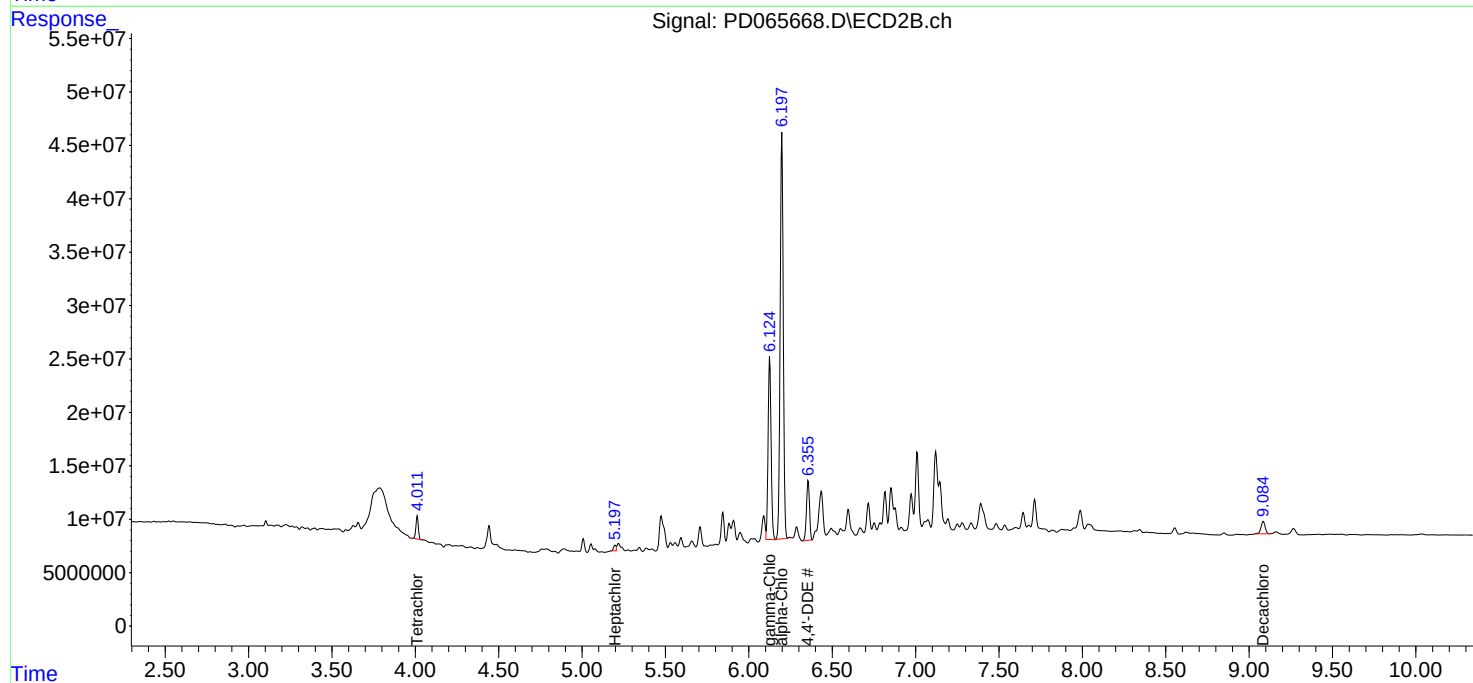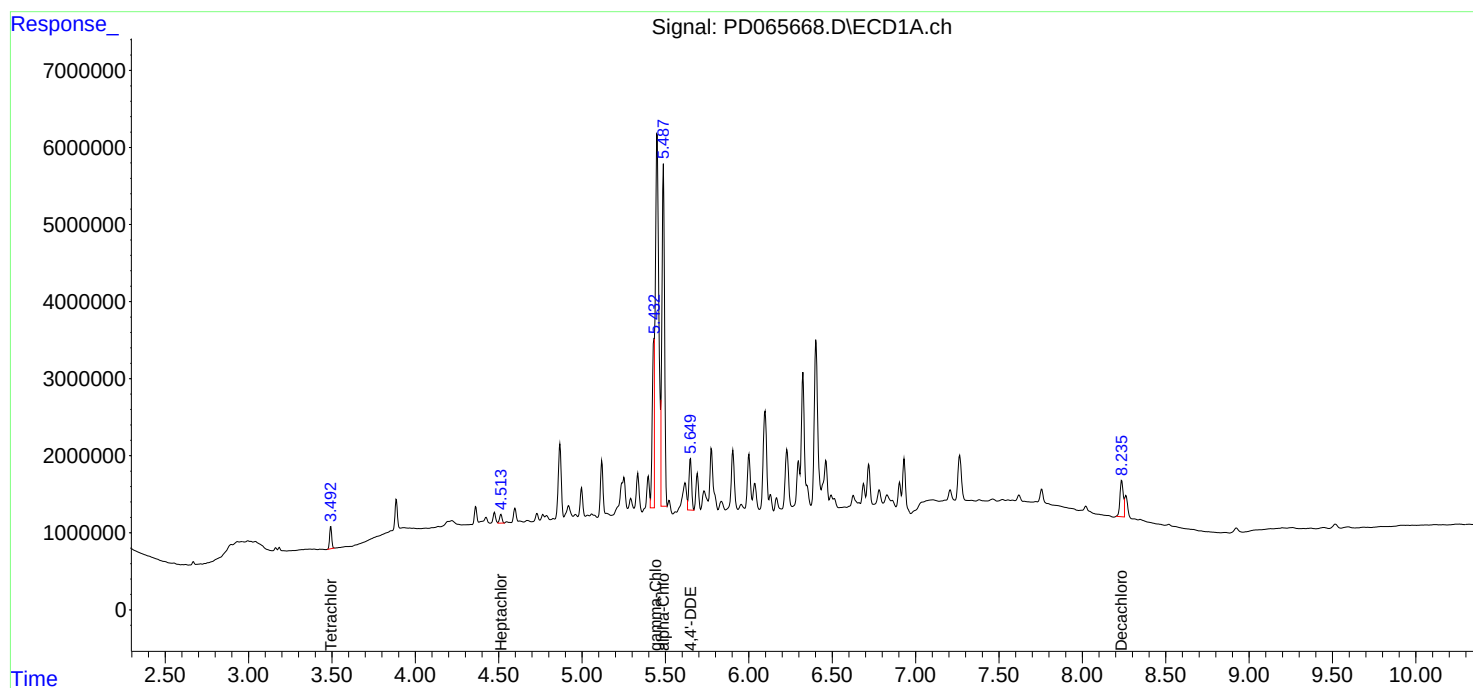


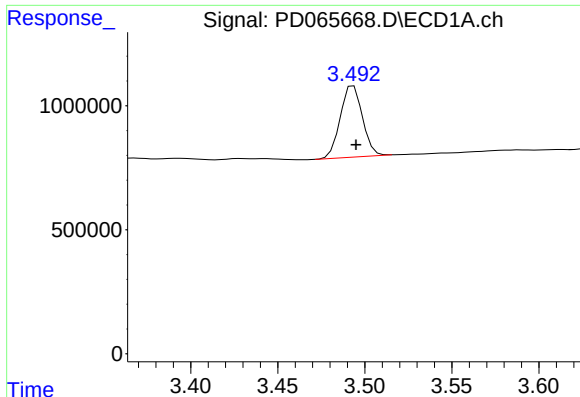

#1 Tetrachloro-m-xylene


R.T.: 3.494 min
Delta R.T.: -0.002 min
Response: 2542544
Conc: 2.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
327DL

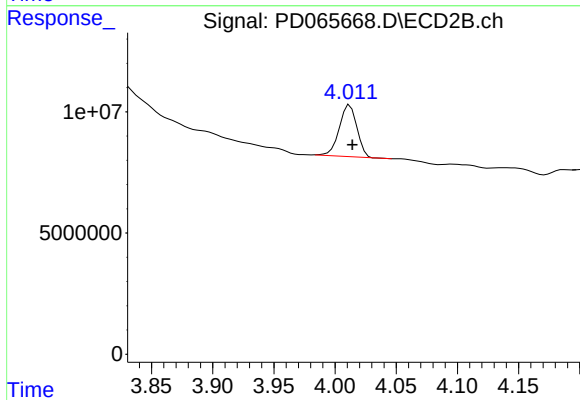


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: -0.002 min
Response: 21213851
Conc: 2.89 ng/ml

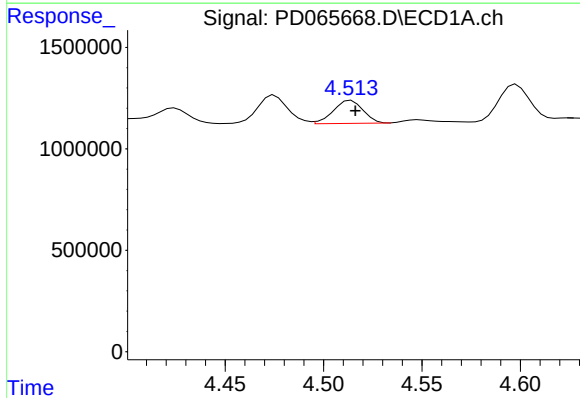


#4 Heptachlor

R.T.: 4.514 min
Delta R.T.: -0.002 min
Response: 1191750
Conc: 0.79 ng/ml

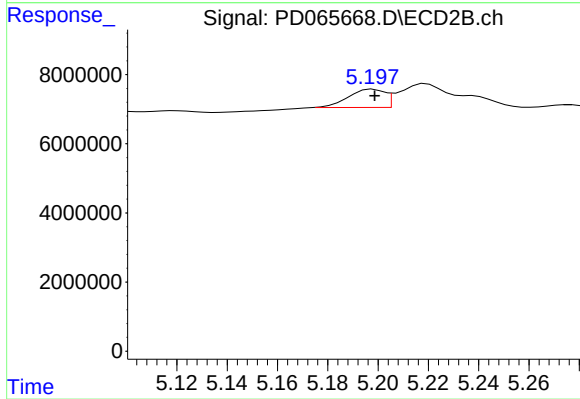

#4 Heptachlor


R.T.: 5.197 min
Delta R.T.: -0.002 min
Response: 5646528
Conc: 0.62 ng/ml m

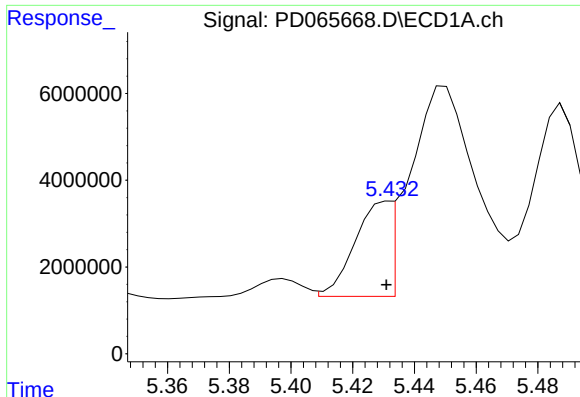

#10 gamma-Chlordane


R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 14463428
Conc: 9.47 ng/ml m

Instrument :
ECD_D
ClientSampleId :
327DL

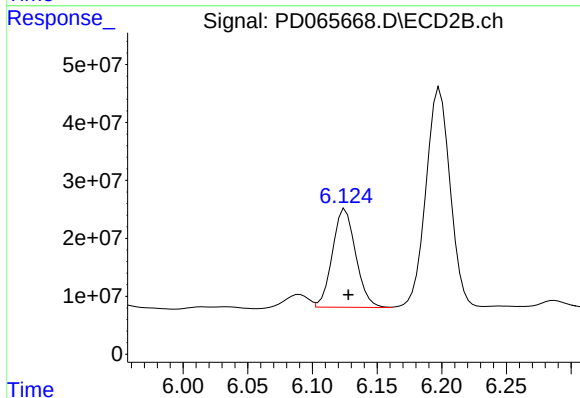


#10 gamma-Chlordane

R.T.: 6.124 min
Delta R.T.: -0.004 min
Response: 212101884
Conc: 28.25 ng/ml m

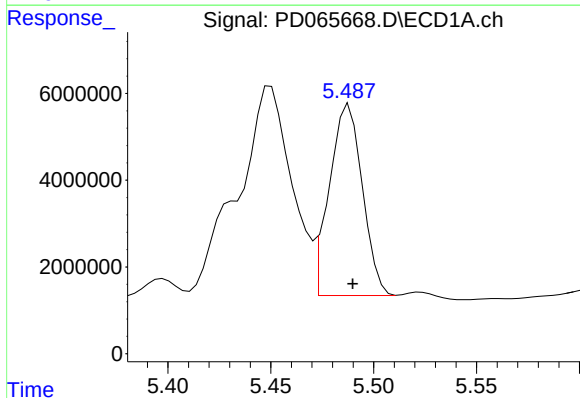


#11 alpha-Chlordane

R.T.: 5.487 min
Delta R.T.: -0.003 min
Response: 48125403
Conc: 31.97 ng/ml m

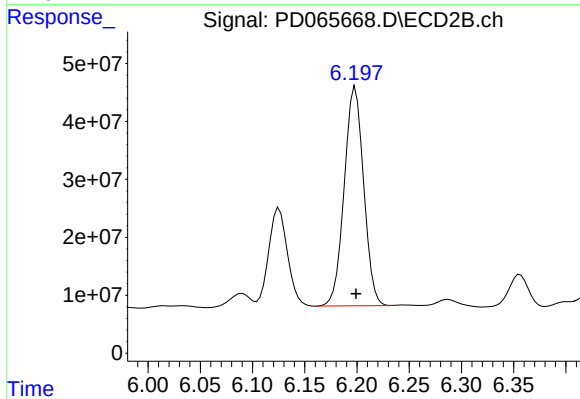

#11 alpha-Chlordane


R.T.: 6.199 min
Delta R.T.: 0.000 min
Response: 489280706
Conc: 66.43 ng/ml

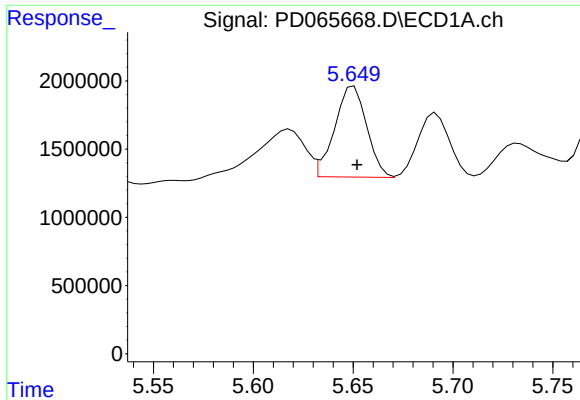

#12 4,4'-DDE


R.T.: 5.649 min
Delta R.T.: -0.003 min
Response: 7401291
Conc: 5.19 ng/ml m

Instrument :
ECD_D
ClientSampleId :
327DL

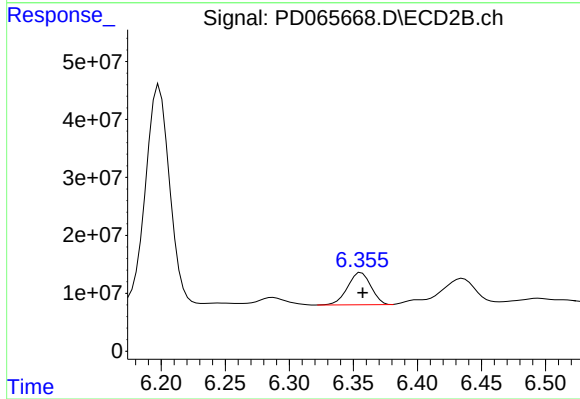


#12 4,4'-DDE

R.T.: 6.356 min
Delta R.T.: -0.001 min
Response: 70282171
Conc: 9.73 ng/ml

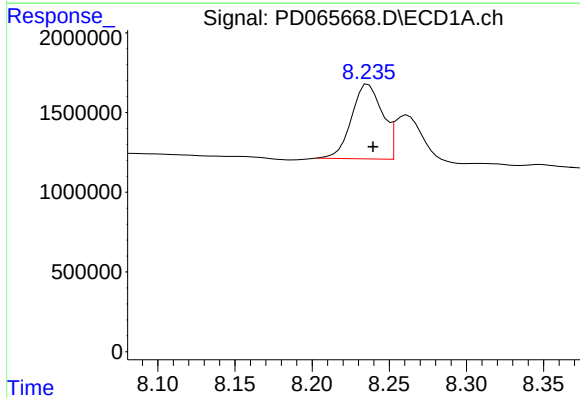

#28 Decachlorobiphenyl

R.T.: 8.237 min
Delta R.T.: -0.003 min
Response: 6508999
Conc: 3.78 ng/ml

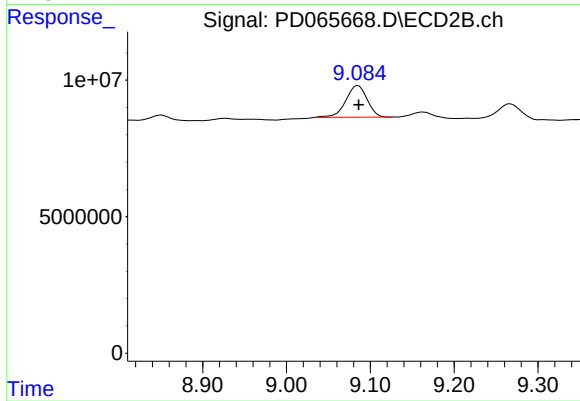

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 20520445
Conc: 3.85 ng/ml