

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091022\
 Data File : PD071802.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2022 22:09
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 21:34:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091022.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 10 21:28:14 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.803	3.562	71429922	741.7E6	24.232	26.108
28)	SA Decachlor...	7.991	9.084	64599782	235.6E6	25.710	26.533
Target Compounds							
23)	Chlordane-1	3.815	4.724	24809969	247.9E6	248.060	268.092
24)	Chlordane-2	4.398	5.257	30514442	178.5E6	260.556	270.743
25)	Chlordane-3	5.034	5.969	81478484	550.0E6	237.635	261.870
26)	Chlordane-4	5.098	6.047	75533050	642.2E6	239.103	262.465
27)	Chlordane-5	6.000	6.908	30631387	126.0E6	251.615	259.643



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091022\
Data File : PD071802.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2022 22:09
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 21:34:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091022.M
Quant Title : GC Extractables
QLast Update : Sat Sep 10 21:28:14 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

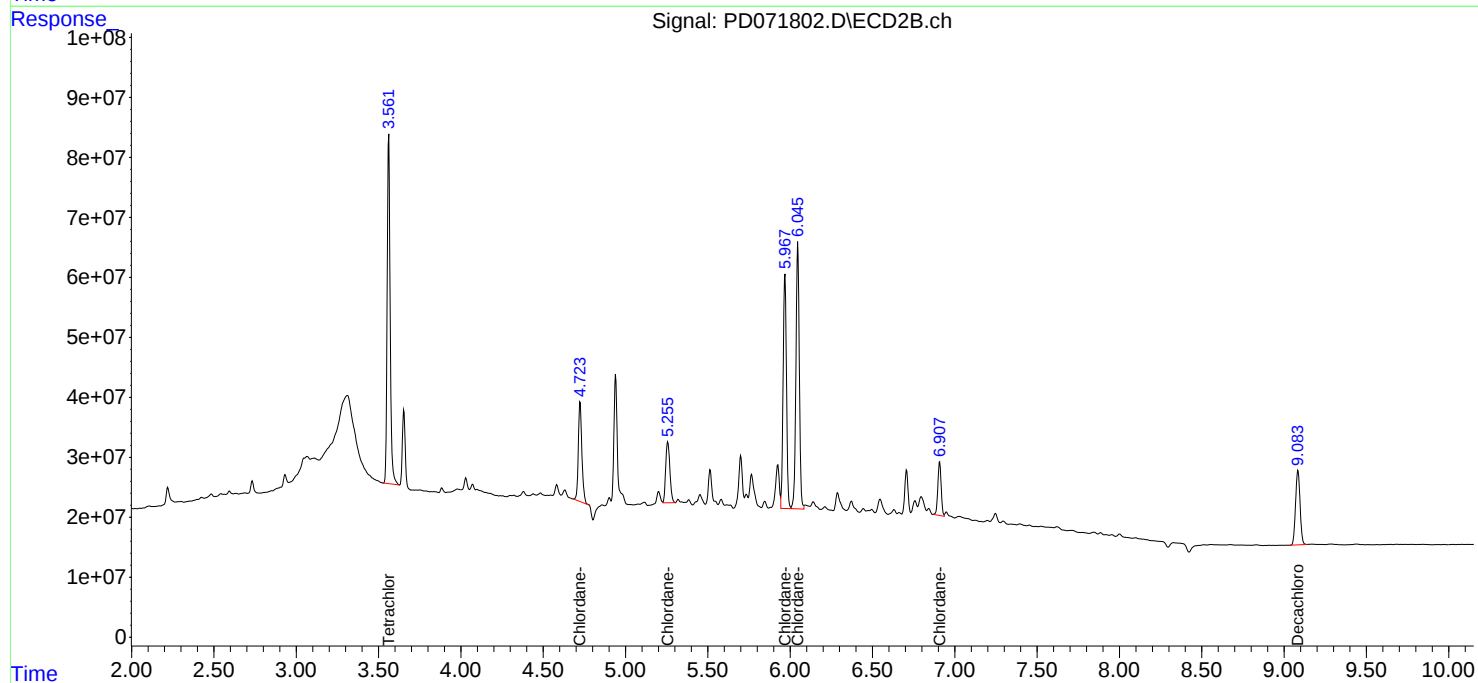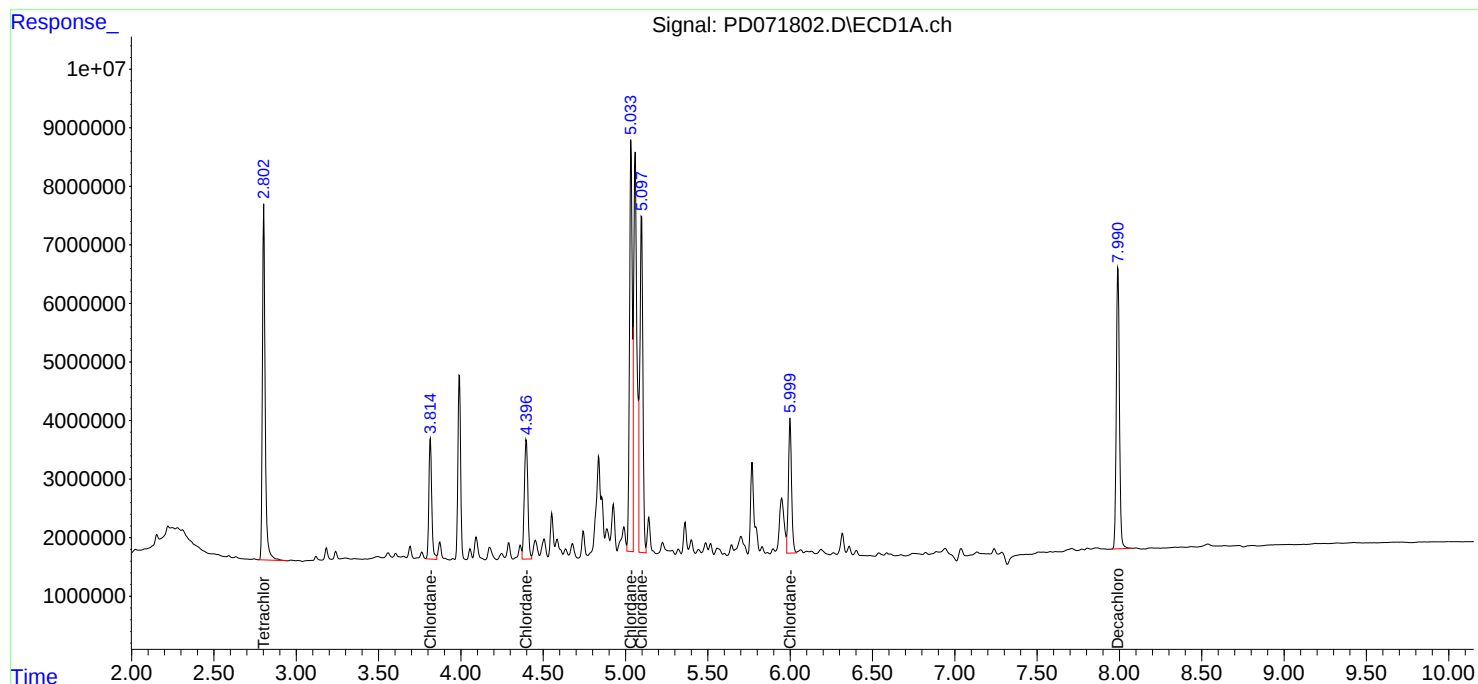


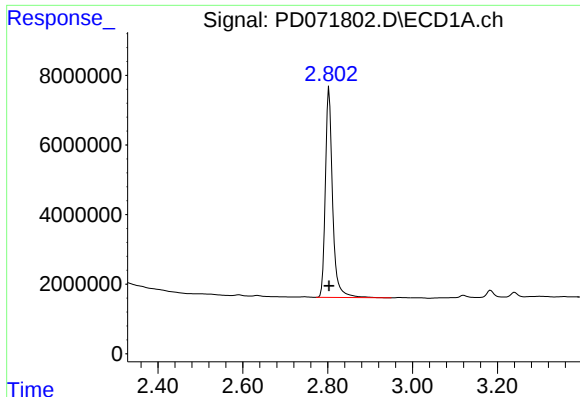

#1 Tetrachloro-m-xylene


R.T.: 2.803 min
Delta R.T.: 0.000 min
Response: 71429922
Conc: 24.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

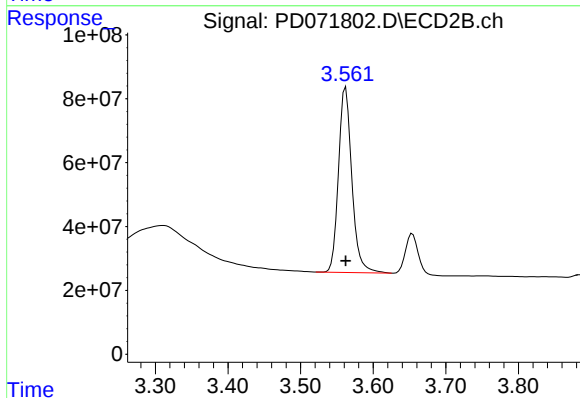


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 741650537
Conc: 26.11 ng/ml

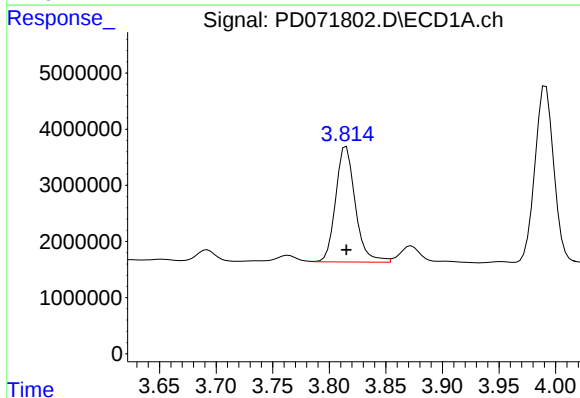


#23 Chlordane-1

R.T.: 3.815 min
Delta R.T.: 0.000 min
Response: 24809969
Conc: 248.06 ng/ml

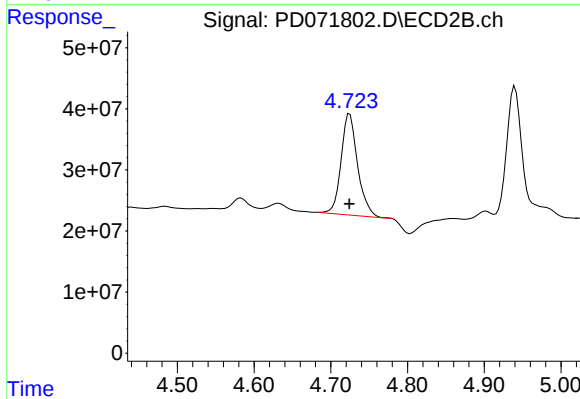

#23 Chlordane-1


R.T.: 4.724 min
Delta R.T.: 0.000 min
Response: 247939952
Conc: 268.09 ng/ml

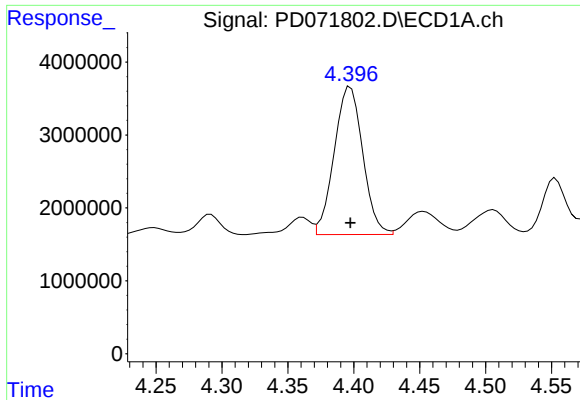

#24 Chlordane-2


R.T.: 4.398 min
Delta R.T.: 0.000 min
Response: 30514442
Conc: 260.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

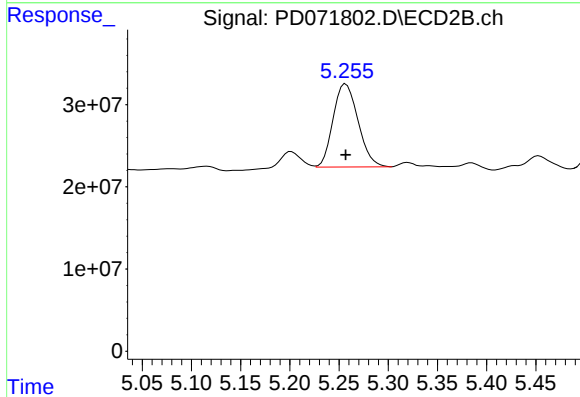


#24 Chlordane-2

R.T.: 5.257 min
Delta R.T.: 0.000 min
Response: 178529222
Conc: 270.74 ng/ml

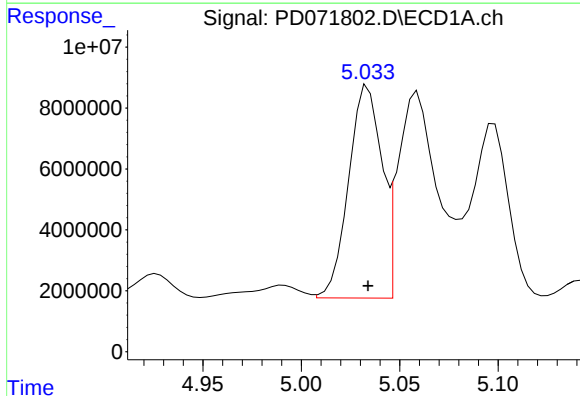


#25 Chlordane-3

R.T.: 5.034 min
Delta R.T.: 0.000 min
Response: 81478484
Conc: 237.63 ng/ml

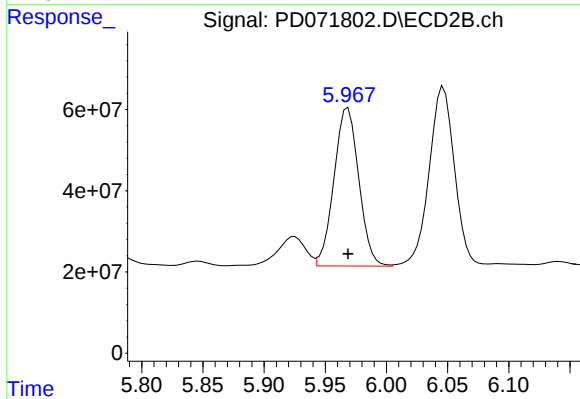

#25 Chlordane-3


R.T.: 5.969 min
Delta R.T.: 0.000 min
Response: 550044873
Conc: 261.87 ng/ml

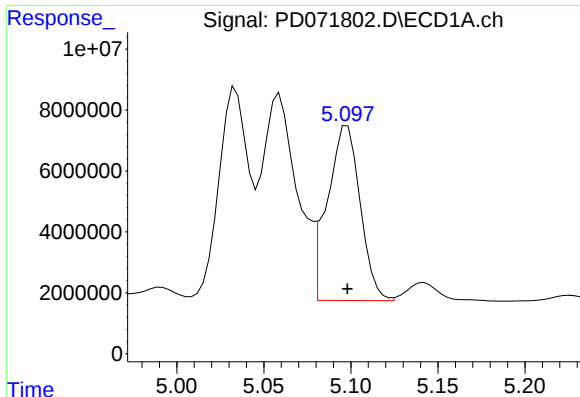

#26 Chlordane-4


R.T.: 5.098 min
Delta R.T.: 0.000 min
Response: 75533050
Conc: 239.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

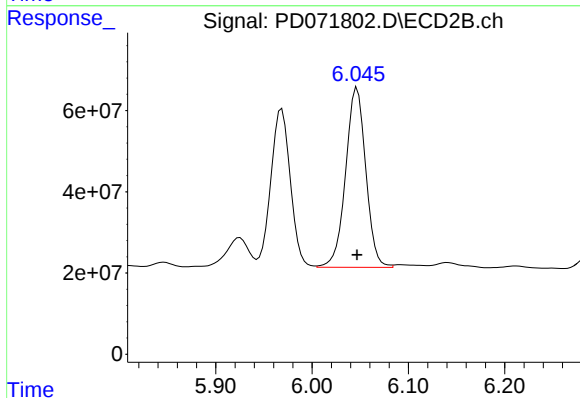


#26 Chlordane-4

R.T.: 6.047 min
Delta R.T.: 0.000 min
Response: 642213009
Conc: 262.47 ng/ml

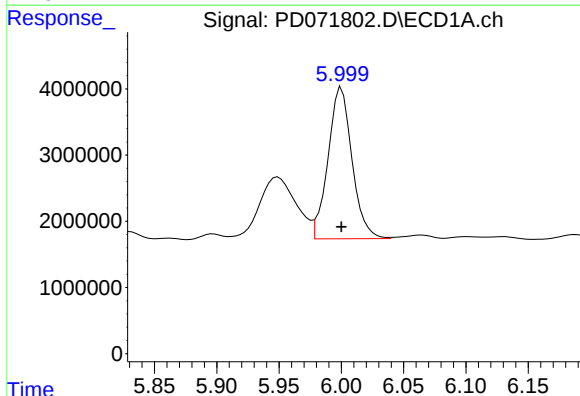


#27 Chlordane-5

R.T.: 6.000 min
Delta R.T.: 0.000 min
Response: 30631387
Conc: 251.61 ng/ml

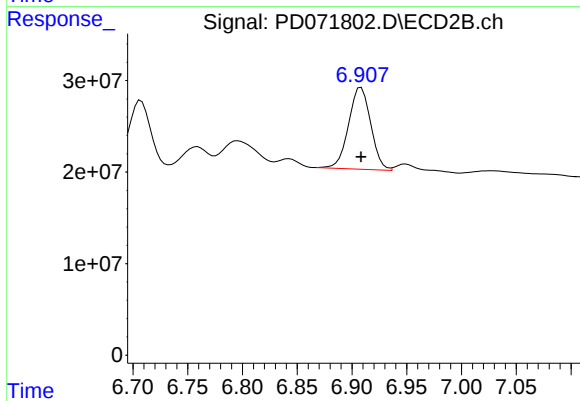

#27 Chlordane-5


R.T.: 6.908 min
Delta R.T.: 0.000 min
Response: 126027511
Conc: 259.64 ng/ml

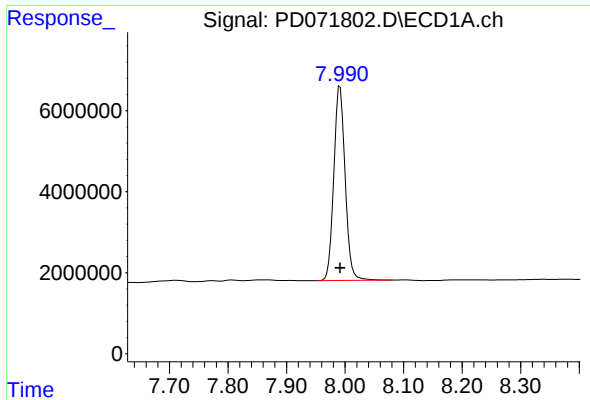

#28 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: 0.000 min
Response: 64599782
Conc: 25.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

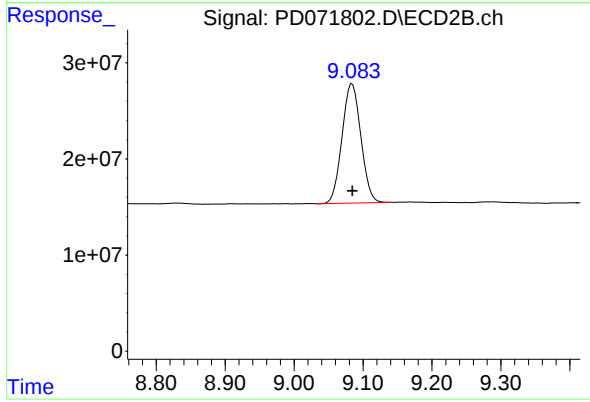

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.000 min
Response: 235641038
Conc: 26.53 ng/ml