

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091022\
 Data File : PD071793.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2022 20:07
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 22:17:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091022.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 10 22:11:50 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.804	3.562	58627439	727.6E6	23.976	25.354
28)	SA Decachlor...	7.993	9.086	58514103	222.9E6	23.227	23.972
Target Compounds							
9)	A Endosulfan I	5.156	6.102	35577709	197.1E6	11.194	13.371
10)	B gamma-Chl...	5.035	5.969	38813999	217.8E6	11.514	13.558
12)	B 4,4'-DDE	5.290	6.219	68706593	351.6E6	22.455	23.865
13)	MA Dieldrin	5.422	6.379	75317168	372.8E6	22.519	24.593
19)	B Endosulfa...	6.399	7.201	58094623	254.2E6	21.662	22.797
20)	A Methoxychlor	6.681	7.531	160.4E6	620.7E6	107.141	102.101
21)	B Endrin ke...	6.909	7.693	70787038	307.2E6	23.591	24.703



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091022\
Data File : PD071793.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2022 20:07
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 22:17:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091022.M
Quant Title : GC Extractables
QLast Update : Sat Sep 10 22:11:50 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

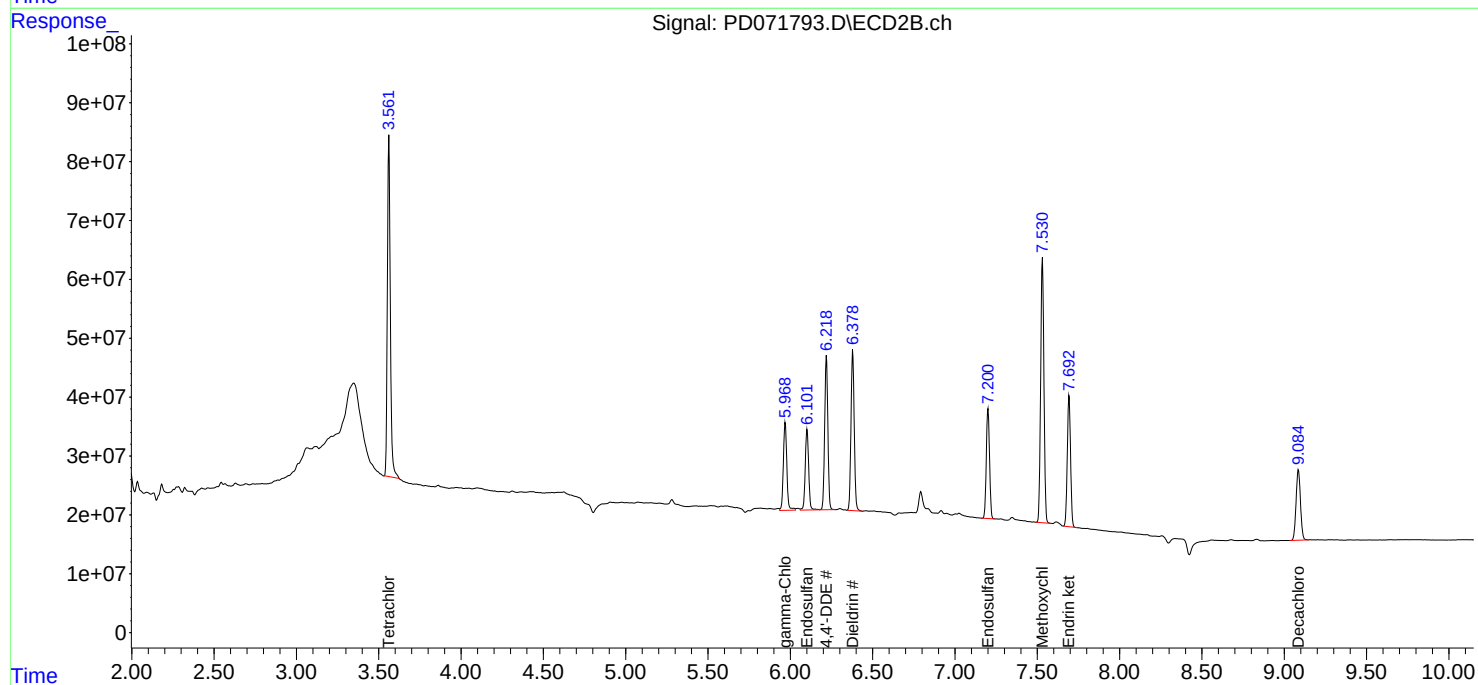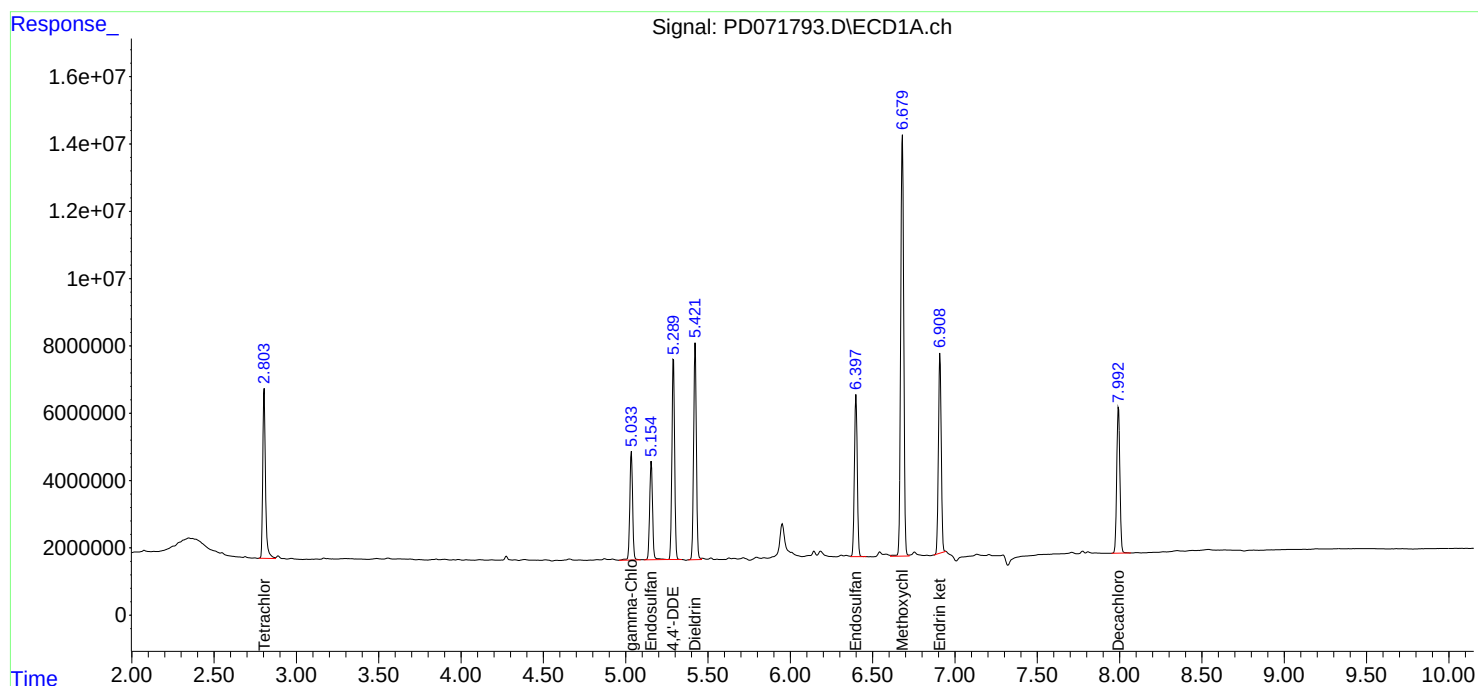


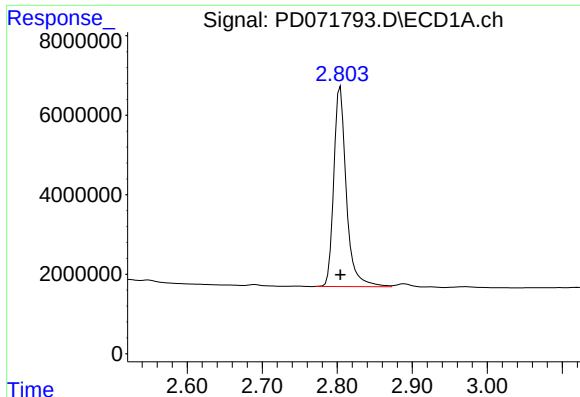

#1 Tetrachloro-m-xylene


R.T.: 2.804 min
Delta R.T.: 0.000 min
Response: 58627439
Conc: 23.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

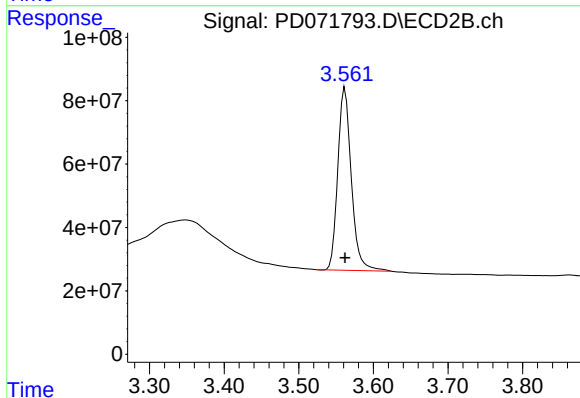


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 727550046
Conc: 25.35 ng/ml

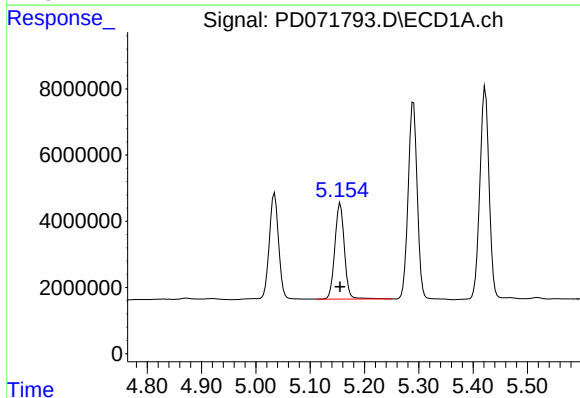


#9 Endosulfan I

R.T.: 5.156 min
Delta R.T.: 0.000 min
Response: 35577709
Conc: 11.19 ng/ml

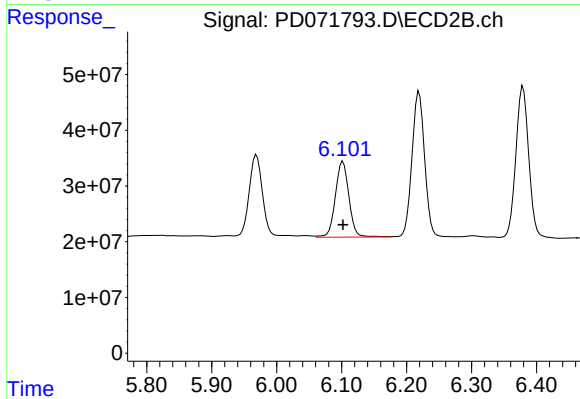

#9 Endosulfan I


R.T.: 6.102 min
Delta R.T.: 0.000 min
Response: 197118738
Conc: 13.37 ng/ml

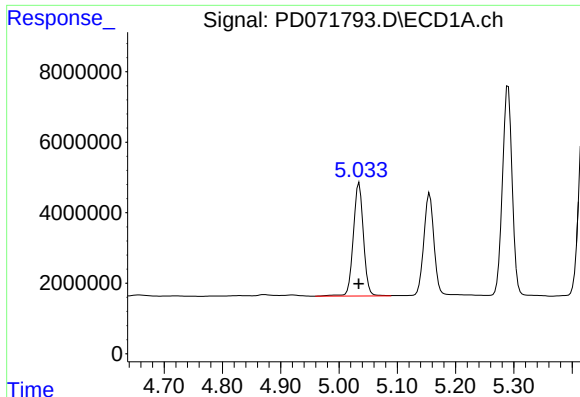

#10 gamma-Chlordane


R.T.: 5.035 min
Delta R.T.: 0.000 min
Response: 38813999
Conc: 11.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

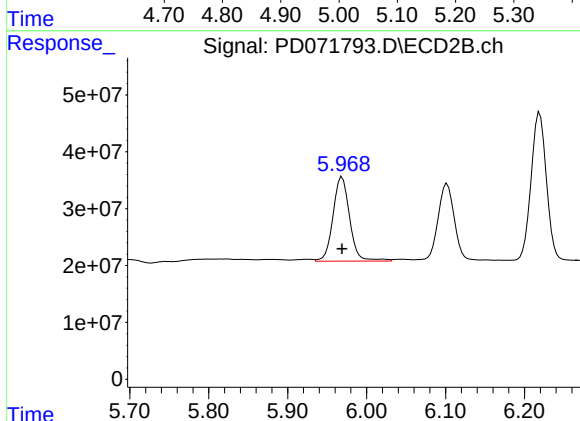


#10 gamma-Chlordane

R.T.: 5.969 min
Delta R.T.: 0.000 min
Response: 217844657
Conc: 13.56 ng/ml

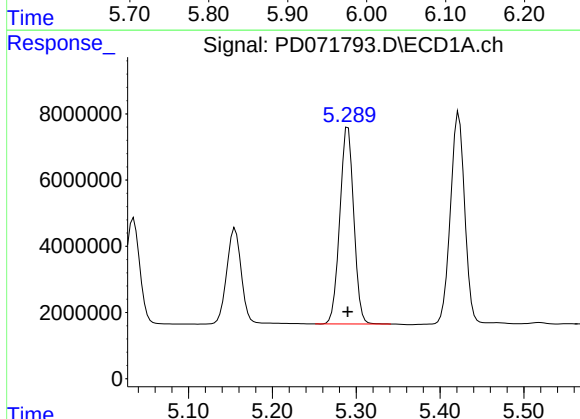


#12 4,4'-DDE

R.T.: 5.290 min
Delta R.T.: 0.000 min
Response: 68706593
Conc: 22.46 ng/ml

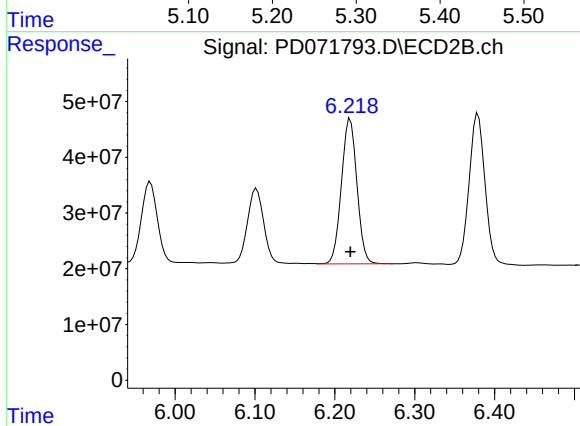

#12 4,4'-DDE


R.T.: 6.219 min
Delta R.T.: 0.000 min
Response: 351557861
Conc: 23.86 ng/ml

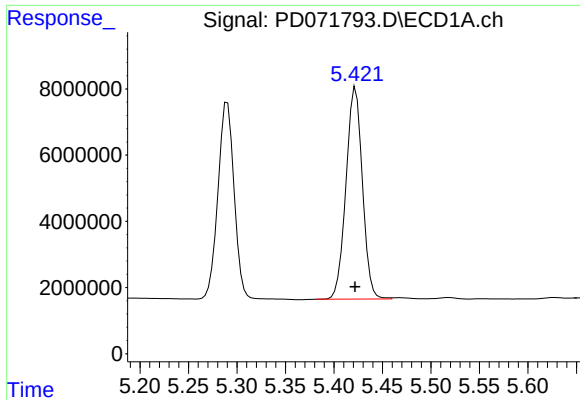

#13 Dieldrin


R.T.: 5.422 min
Delta R.T.: 0.000 min
Response: 75317168
Conc: 22.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

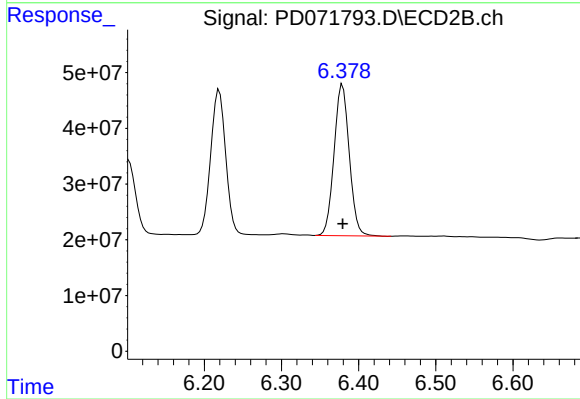


#13 Dieldrin

R.T.: 6.379 min
Delta R.T.: 0.000 min
Response: 372750847
Conc: 24.59 ng/ml

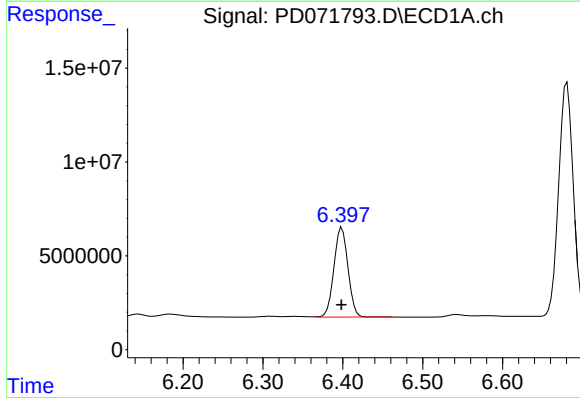


#19 Endosulfan Sulfate

R.T.: 6.399 min
Delta R.T.: 0.000 min
Response: 58094623
Conc: 21.66 ng/ml

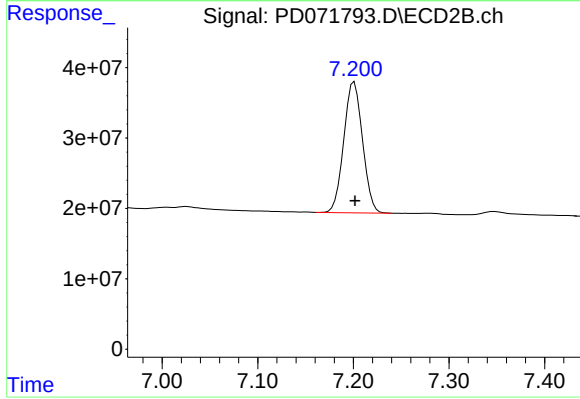

#19 Endosulfan Sulfate


R.T.: 7.201 min
Delta R.T.: 0.000 min
Response: 254239586
Conc: 22.80 ng/ml

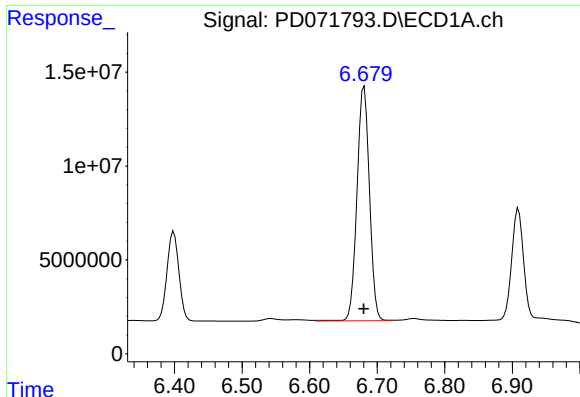

#20 Methoxychlor


R.T.: 6.681 min
Delta R.T.: 0.000 min
Response: 160427545
Conc: 107.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

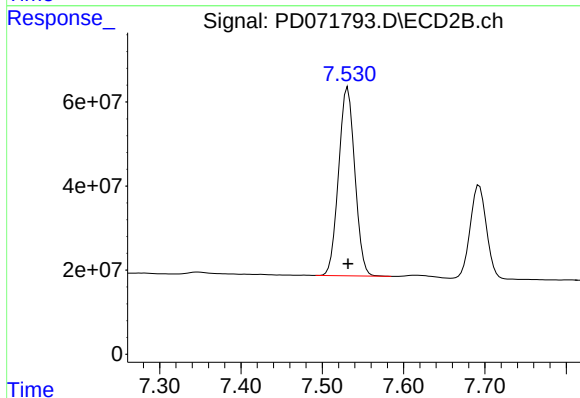


#20 Methoxychlor

R.T.: 7.531 min
Delta R.T.: 0.000 min
Response: 620682118
Conc: 102.10 ng/ml

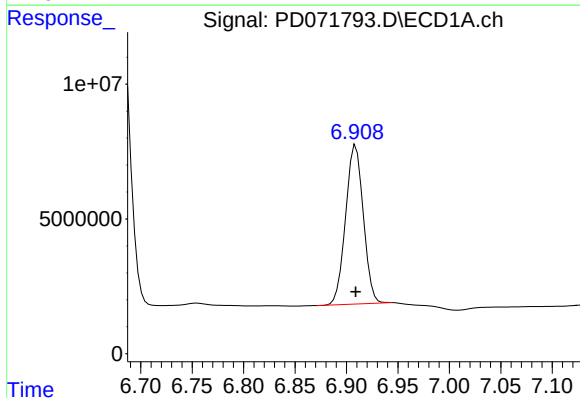


#21 Endrin ketone

R.T.: 6.909 min
Delta R.T.: 0.000 min
Response: 70787038
Conc: 23.59 ng/ml

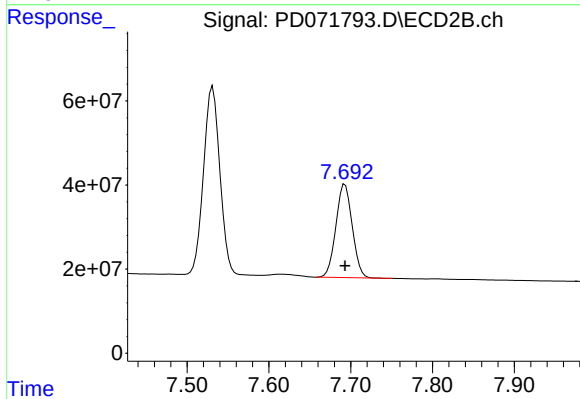

#21 Endrin ketone


R.T.: 7.693 min
Delta R.T.: 0.000 min
Response: 307234101
Conc: 24.70 ng/ml

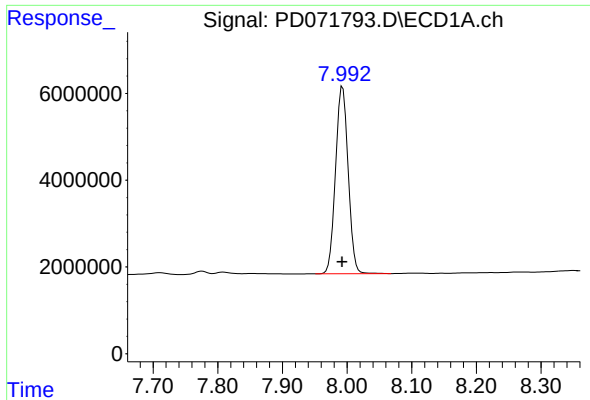

#28 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: 0.001 min
Response: 58514103
Conc: 23.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

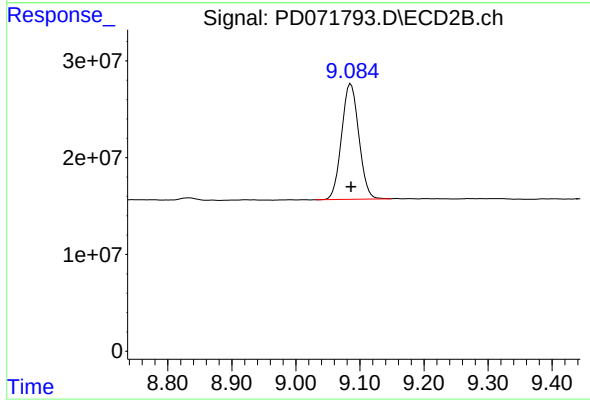

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.000 min
Response: 222873873
Conc: 23.97 ng/ml