

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091022\
 Data File : PD071799.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2022 21:28
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 21:30:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091022.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 10 21:28:14 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.804	3.562	301.7E6	2752.3E6	99.495	96.330
28)	SA Decachlor...	7.993	9.087	245.6E6	843.5E6	97.054	95.165
Target Compounds							
23)	Chlordane-1	3.816	4.725	101.0E6	873.1E6	987.723	947.125
24)	Chlordane-2	4.398	5.258	113.2E6	612.1E6	961.872	935.155
25)	Chlordane-3	5.035	5.970	356.3E6	2027.9E6	1000.153	962.561
26)	Chlordane-4	5.099	6.048	325.5E6	2349.8E6	996.167	958.647
27)	Chlordane-5	6.001	6.909	121.5E6	469.1E6	981.304	959.068



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091022\
Data File : PD071799.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2022 21:28
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 21:30:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091022.M
Quant Title : GC Extractables
QLast Update : Sat Sep 10 21:28:14 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

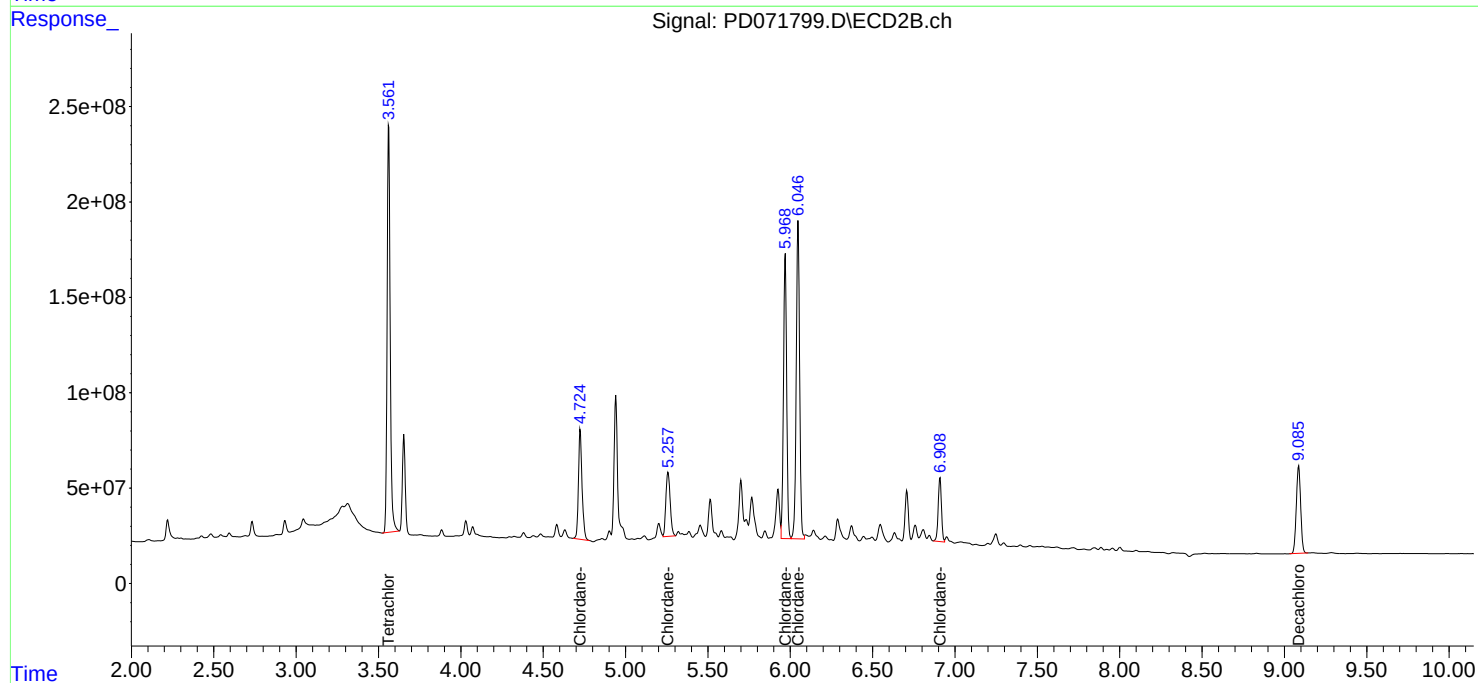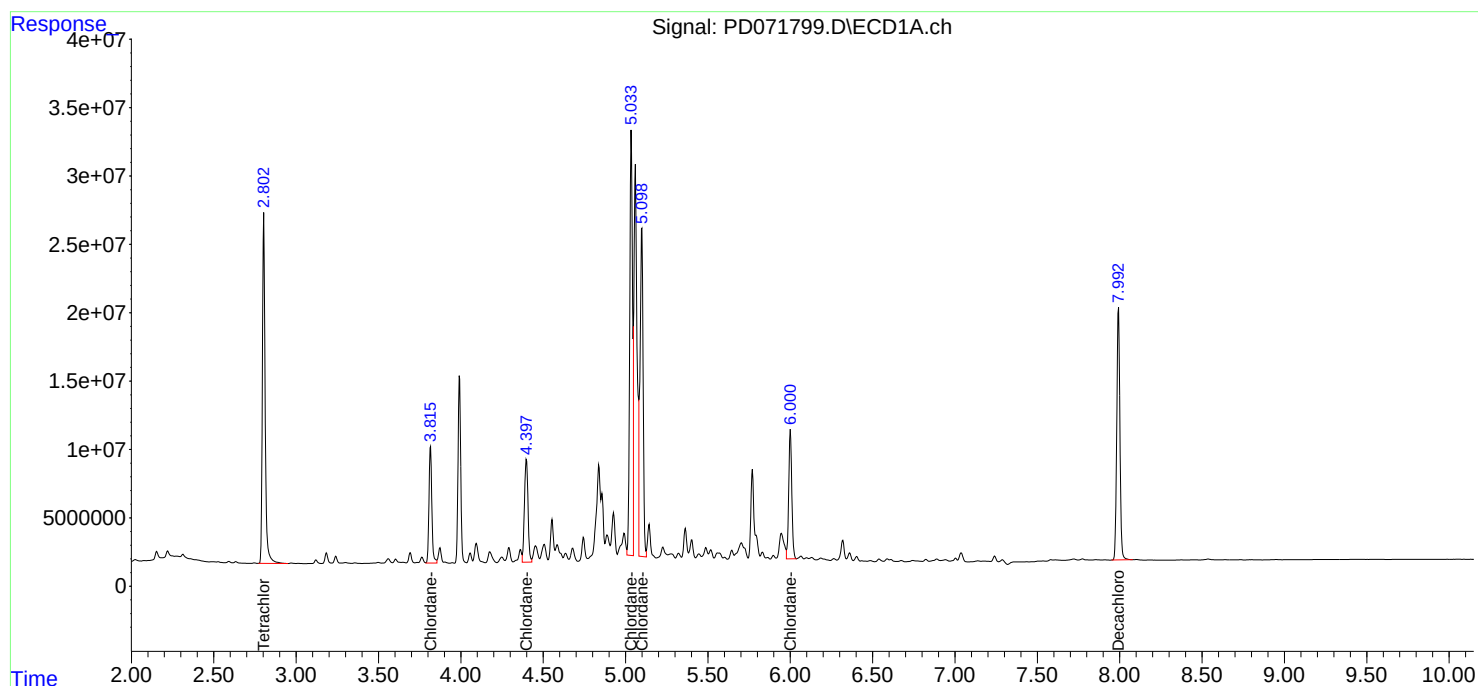


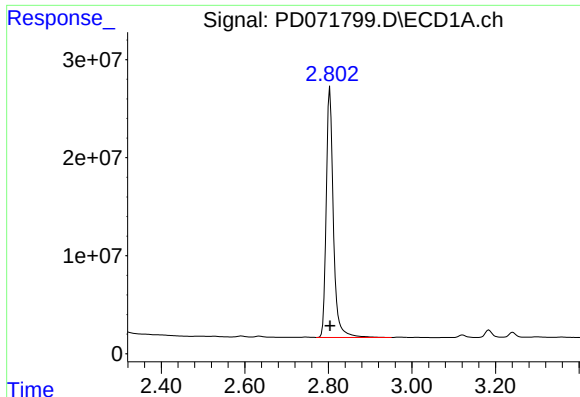

#1 Tetrachloro-m-xylene


R.T.: 2.804 min
Delta R.T.: 0.000 min
Response: 301728660
Conc: 99.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

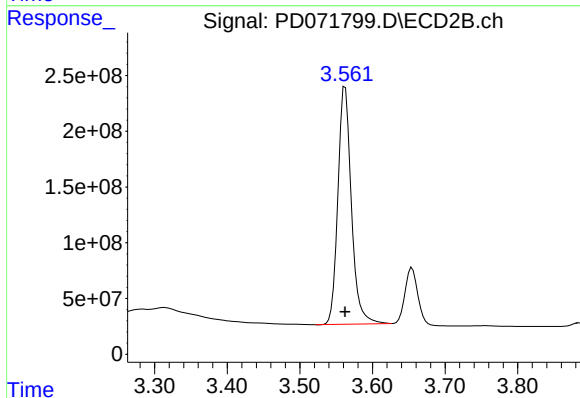


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 2752329765
Conc: 96.33 ng/ml

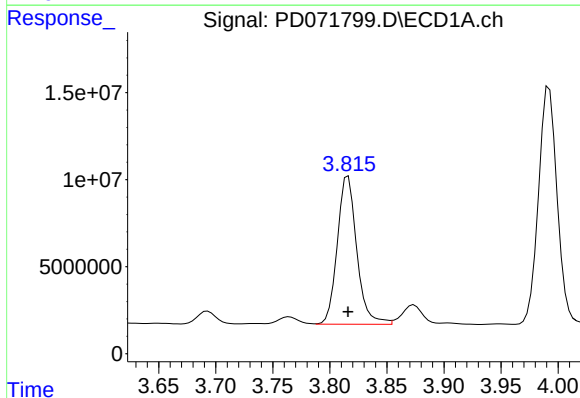


#23 Chlordane-1

R.T.: 3.816 min
Delta R.T.: 0.000 min
Response: 101023751
Conc: 987.72 ng/ml

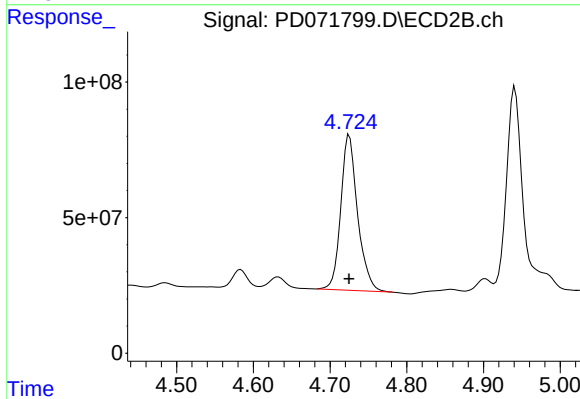

#23 Chlordane-1


R.T.: 4.725 min
Delta R.T.: 0.000 min
Response: 873113545
Conc: 947.13 ng/ml

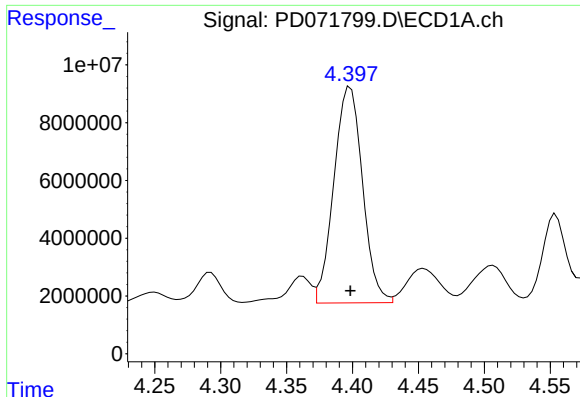

#24 Chlordane-2


R.T.: 4.398 min
Delta R.T.: 0.000 min
Response: 113230196
Conc: 961.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

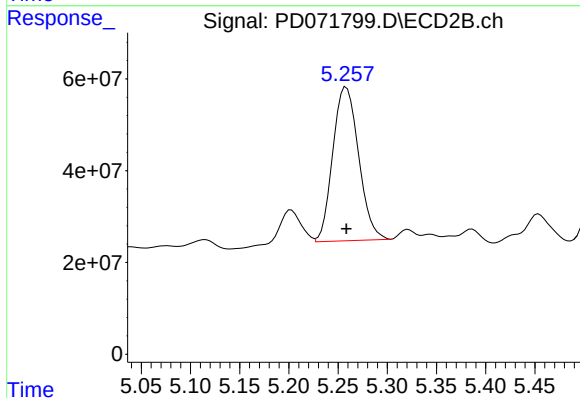


#24 Chlordane-2

R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 612102617
Conc: 935.15 ng/ml

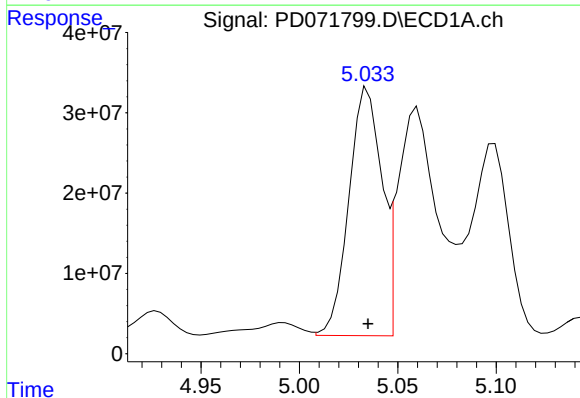


#25 Chlordane-3

R.T.: 5.035 min
Delta R.T.: 0.000 min
Response: 356324345
Conc: 1000.15 ng/ml

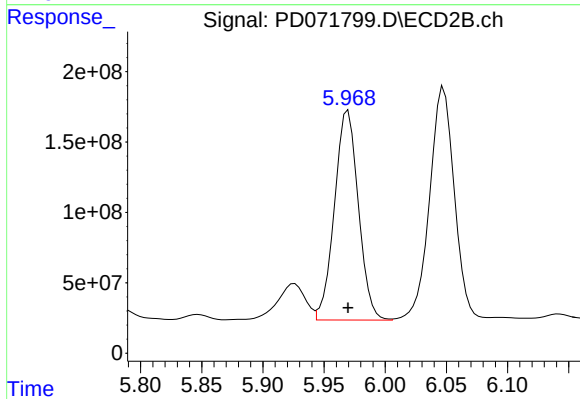

#25 Chlordane-3


R.T.: 5.970 min
Delta R.T.: 0.000 min
Response: 2027924997
Conc: 962.56 ng/ml

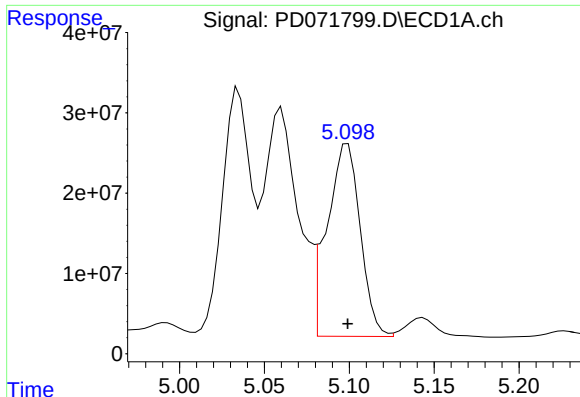

#26 Chlordane-4


R.T.: 5.099 min
Delta R.T.: 0.000 min
Response: 325486832
Conc: 996.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

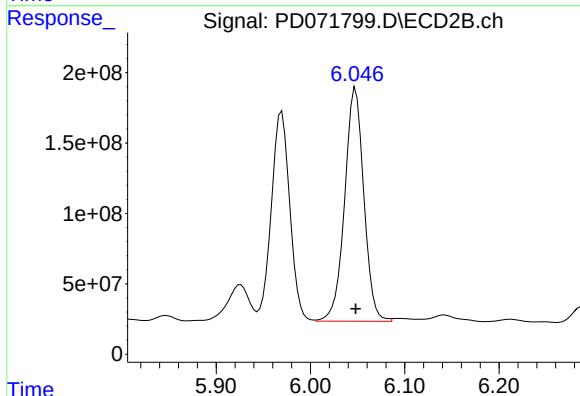


#26 Chlordane-4

R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 2349769010
Conc: 958.65 ng/ml

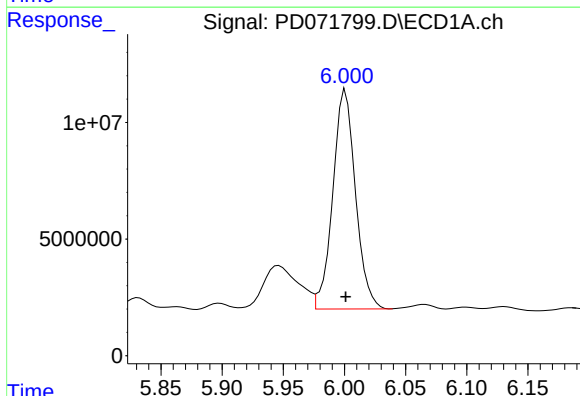


#27 Chlordane-5

R.T.: 6.001 min
Delta R.T.: 0.000 min
Response: 121519336
Conc: 981.30 ng/ml

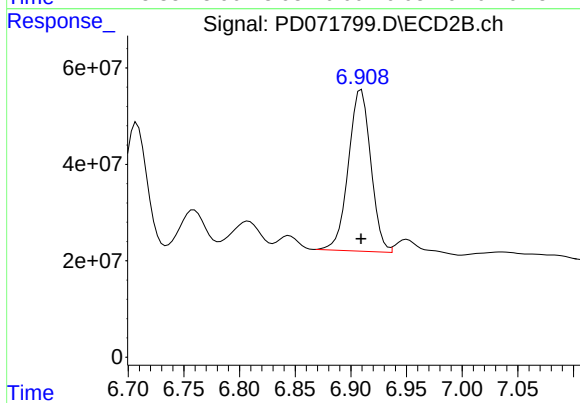

#27 Chlordane-5


R.T.: 6.909 min
Delta R.T.: 0.000 min
Response: 469080729
Conc: 959.07 ng/ml

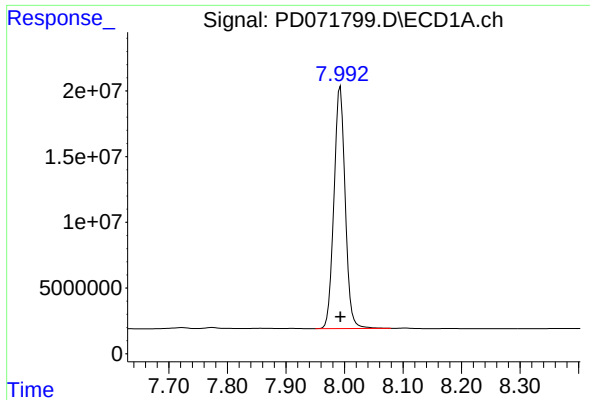

#28 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: 0.000 min
Response: 245642524
Conc: 97.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

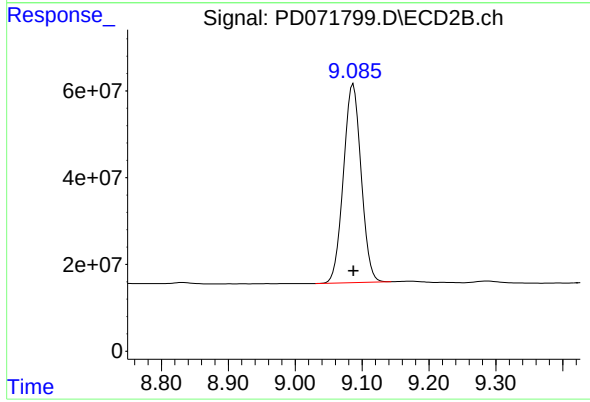

#28 Decachlorobiphenyl

R.T.: 9.087 min
Delta R.T.: 0.000 min
Response: 843455514
Conc: 95.17 ng/ml