

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091022\
 Data File : PD071800.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2022 21:42
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 21:32:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091022.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 10 21:28:14 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.804	3.562	215.1E6	2011.4E6	72.247	71.867
28)	SA Decachlor...	7.993	9.085	180.3E6	627.9E6	72.458	72.178
Target Compounds							
23)	Chlordane-1	3.816	4.725	72198463	647.9E6	720.008	717.869
24)	Chlordane-2	4.399	5.258	83216872	460.8E6	720.715	718.696
25)	Chlordane-3	5.035	5.969	249.8E6	1491.0E6	716.669	721.266
26)	Chlordane-4	5.099	6.047	231.0E6	1737.2E6	720.756	721.979
27)	Chlordane-5	6.001	6.909	87571339	344.4E6	720.888	718.836



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091022\
Data File : PD071800.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2022 21:42
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 21:32:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091022.M
Quant Title : GC Extractables
QLast Update : Sat Sep 10 21:28:14 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

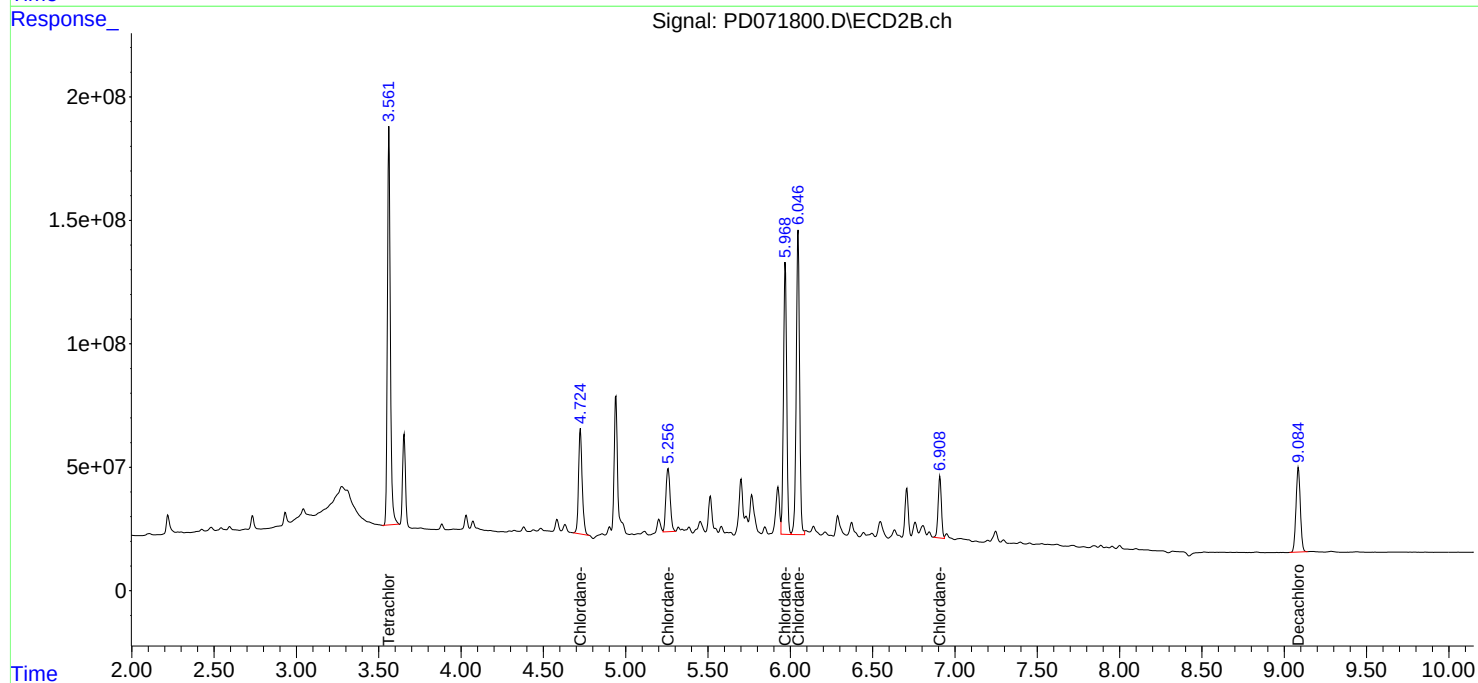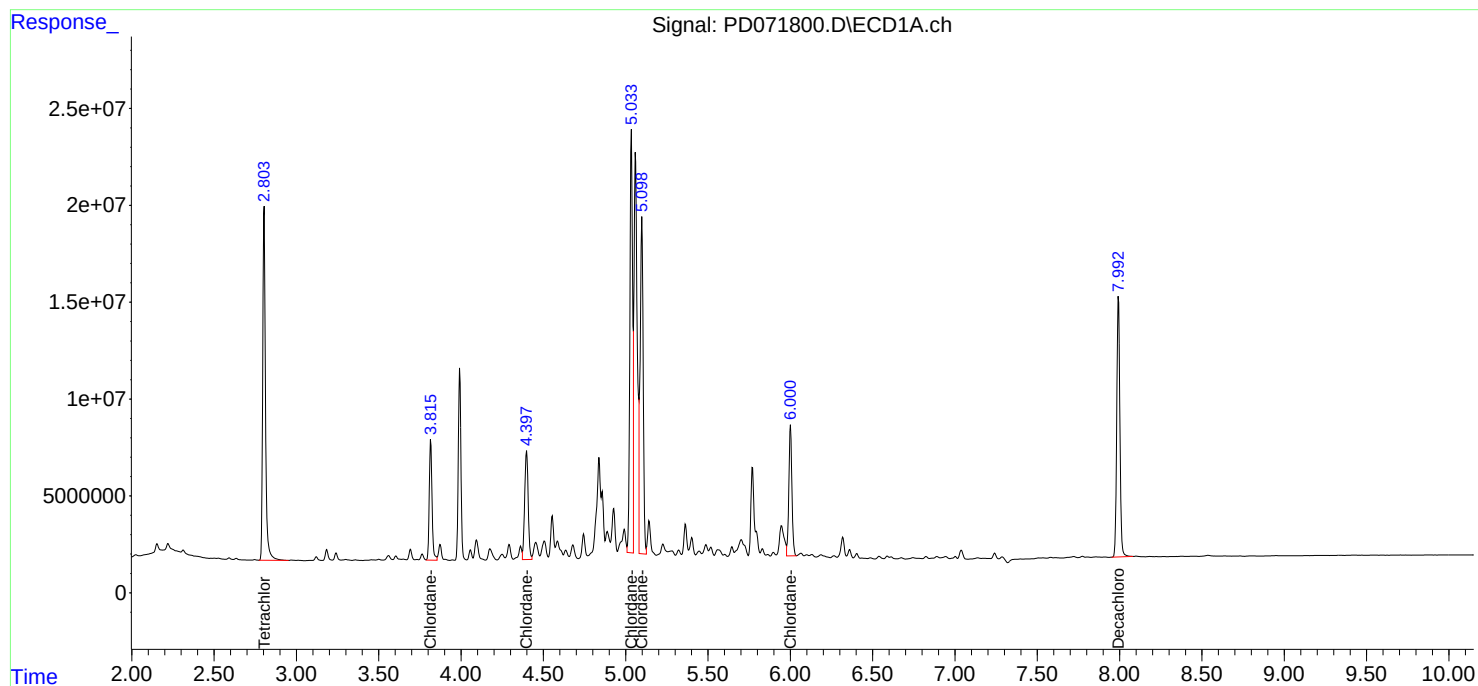


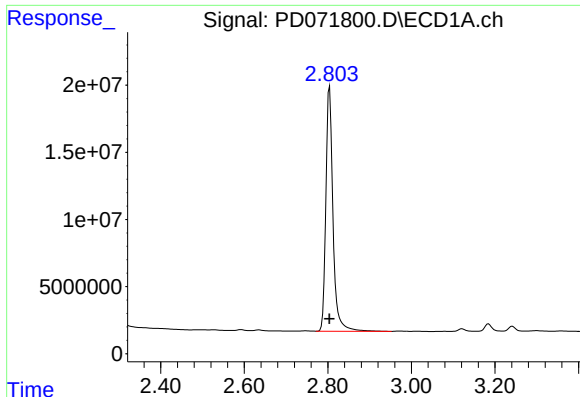

#1 Tetrachloro-m-xylene


R.T.: 2.804 min
Delta R.T.: 0.000 min
Response: 215147539
Conc: 72.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

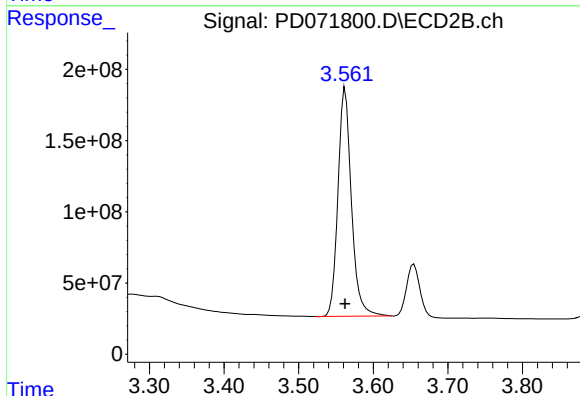


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 2011364686
Conc: 71.87 ng/ml

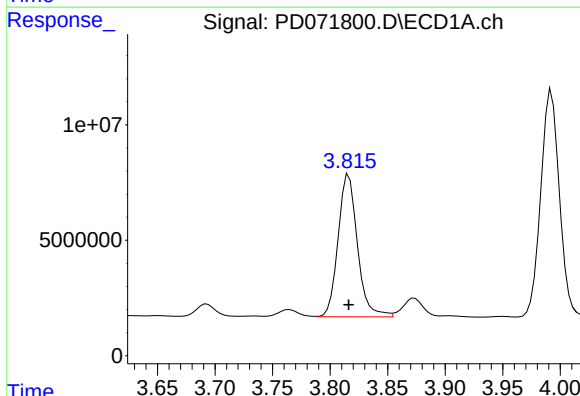


#23 Chlordane-1

R.T.: 3.816 min
Delta R.T.: 0.000 min
Response: 72198463
Conc: 720.01 ng/ml

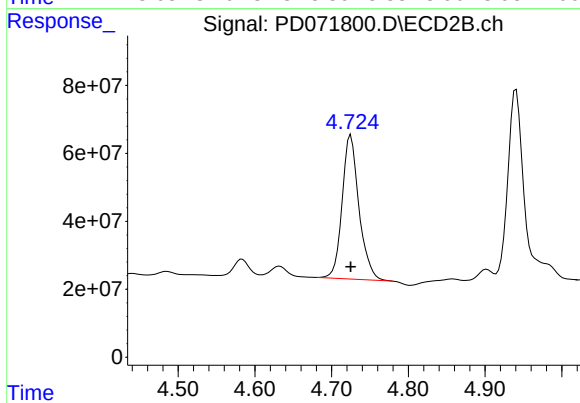

#23 Chlordane-1


R.T.: 4.725 min
Delta R.T.: 0.000 min
Response: 647894187
Conc: 717.87 ng/ml

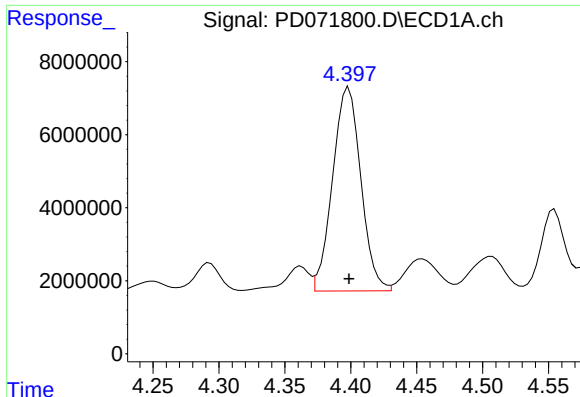

#24 Chlordane-2


R.T.: 4.399 min
Delta R.T.: 0.000 min
Response: 83216872
Conc: 720.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

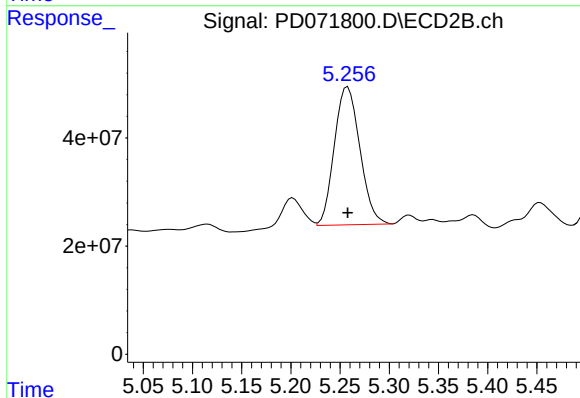


#24 Chlordane-2

R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 460804015
Conc: 718.70 ng/ml

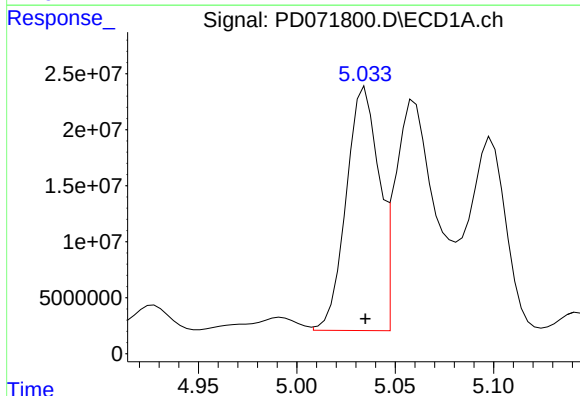


#25 Chlordane-3

R.T.: 5.035 min
Delta R.T.: 0.000 min
Response: 249777548
Conc: 716.67 ng/ml

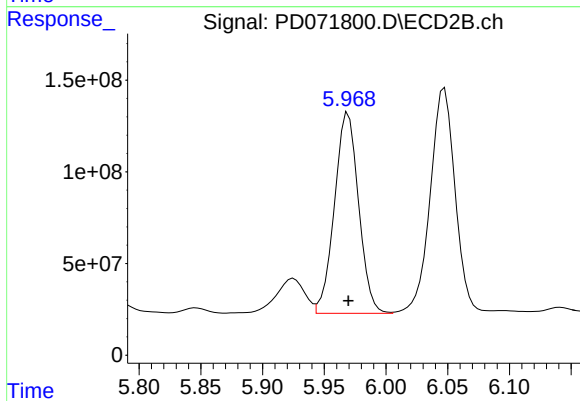

#25 Chlordane-3


R.T.: 5.969 min
Delta R.T.: 0.000 min
Response: 1491002478
Conc: 721.27 ng/ml

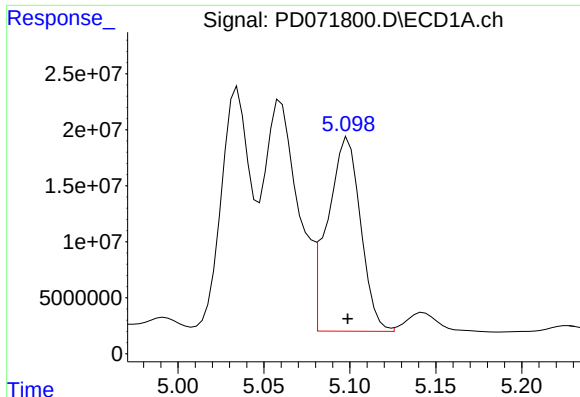

#26 Chlordane-4


R.T.: 5.099 min
Delta R.T.: 0.000 min
Response: 230995713
Conc: 720.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

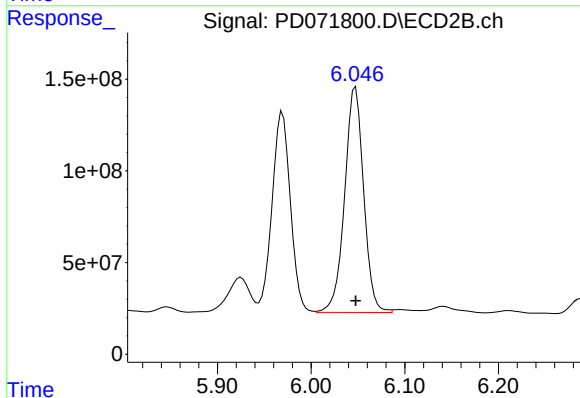


#26 Chlordane-4

R.T.: 6.047 min
Delta R.T.: 0.000 min
Response: 1737214182
Conc: 721.98 ng/ml

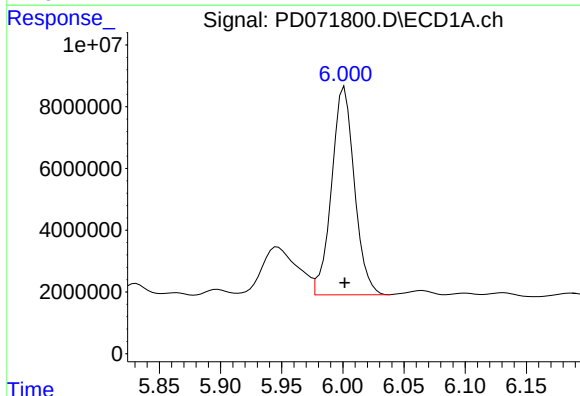


#27 Chlordane-5

R.T.: 6.001 min
Delta R.T.: 0.000 min
Response: 87571339
Conc: 720.89 ng/ml

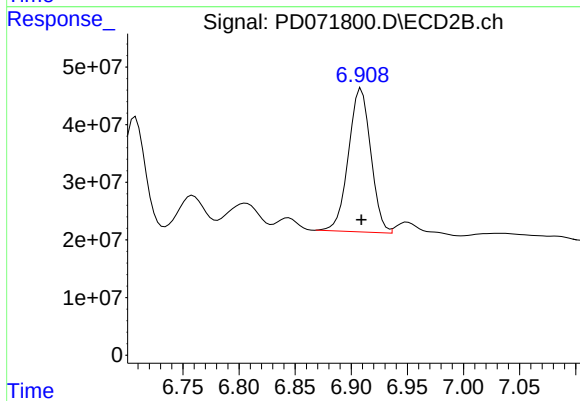

#27 Chlordane-5


R.T.: 6.909 min
Delta R.T.: 0.000 min
Response: 344427384
Conc: 718.84 ng/ml

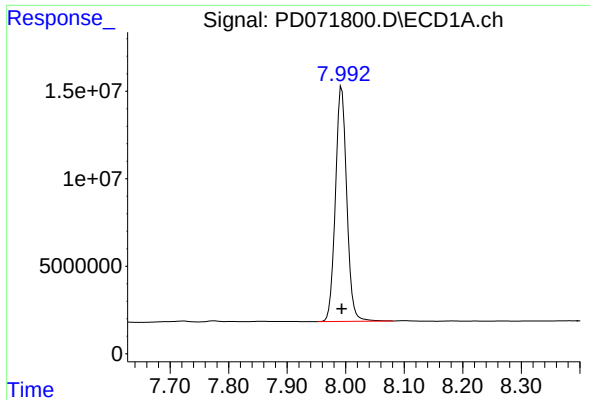

#28 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: 0.000 min
Response: 180335391
Conc: 72.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

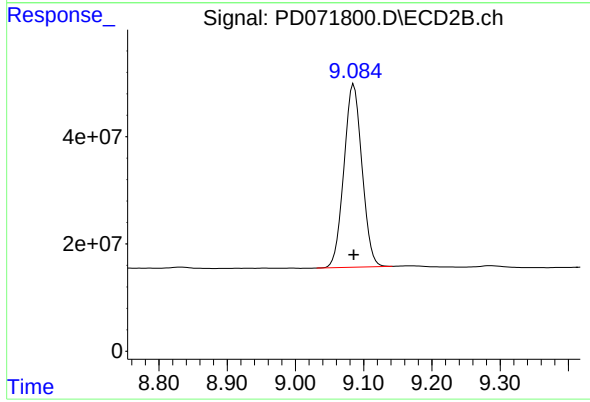

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 627906910
Conc: 72.18 ng/ml