

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091119\
 Data File : PD054465.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Sep 2019 14:13
 Operator : SG\AJ
 Sample : K4717-18
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AC1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 00:50:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090419CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 05 08:40:10 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.302	3.972	11663465	16376489	16.502	16.593
27)	SA Decachlor...	7.991	9.008	18617067	27318130	27.509	29.202


Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091119\
Data File : PD054465.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Sep 2019 14:13
Operator : SG\AJ
Sample : K4717-18
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 00:50:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090419CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 05 08:40:10 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

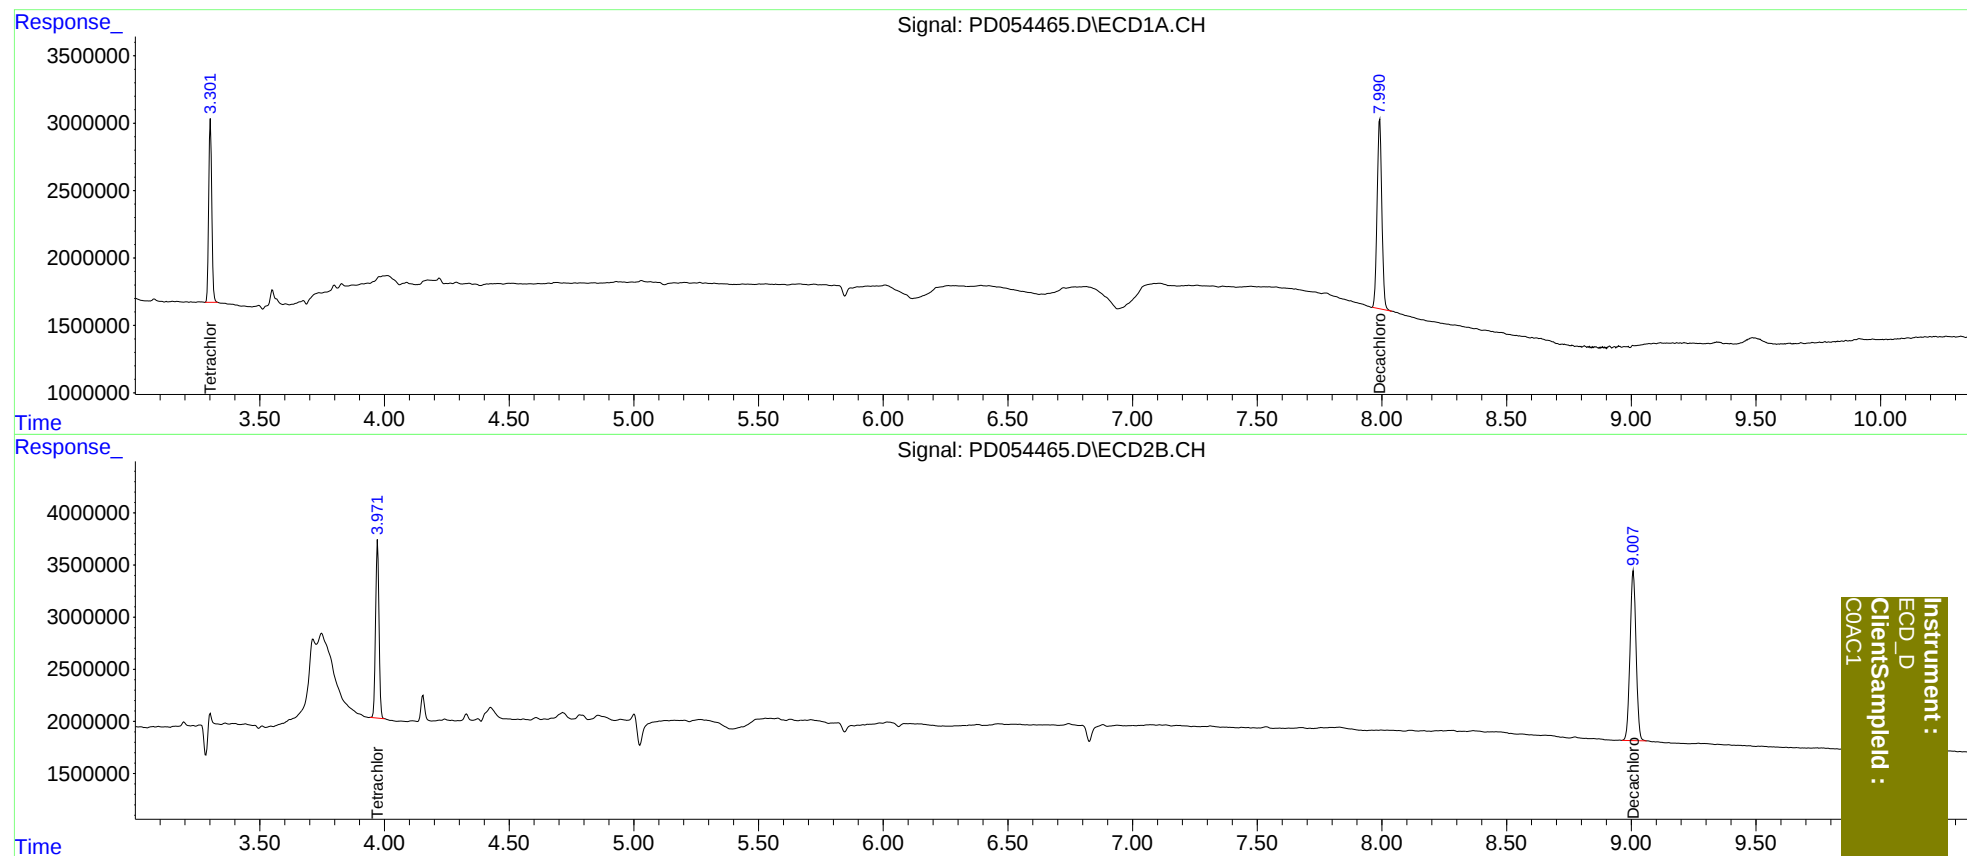


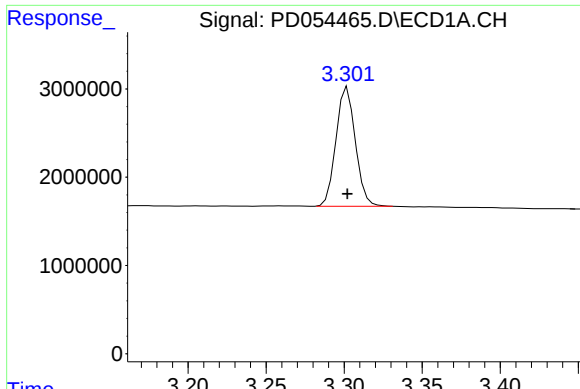

#1 Tetrachloro-m-xylene


R.T.: 3.302 min
Delta R.T.: 0.000 min
Response: 11663465
Conc: 16.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AC1

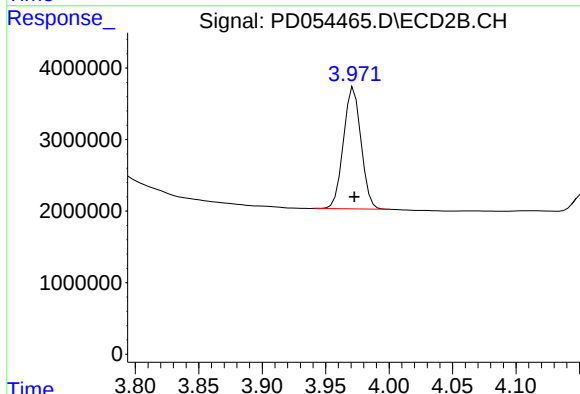


#1 Tetrachloro-m-xylene

R.T.: 3.972 min
Delta R.T.: 0.000 min
Response: 16376489
Conc: 16.59 ng/ml

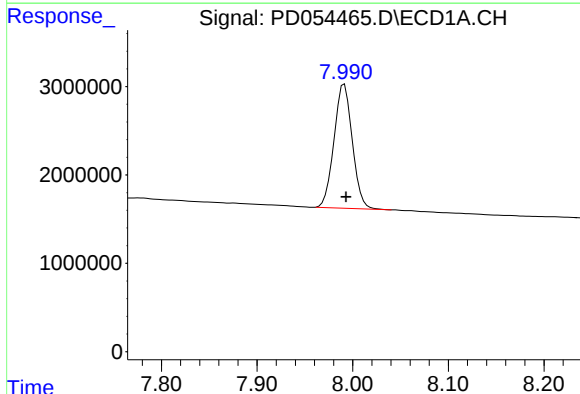

#27 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: -0.002 min
Response: 18617067
Conc: 27.51 ng/ml

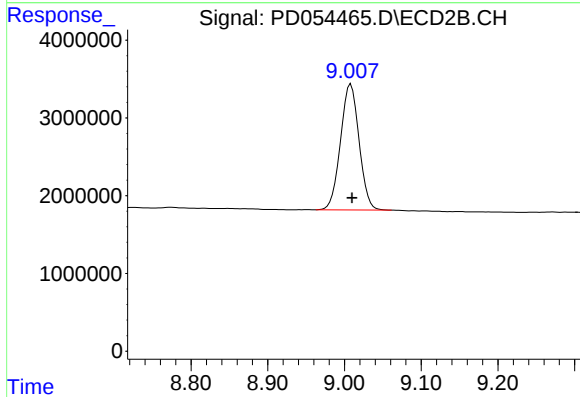

#27 Decachlorobiphenyl

R.T.: 9.008 min
Delta R.T.: -0.002 min
Response: 27318130
Conc: 29.20 ng/ml