

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091119\
 Data File : PD054475.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Sep 2019 17:13
 Operator : SG\AJ
 Sample : K4717-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AB4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 00:52:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090419CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 05 08:40:10 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.302	3.973	12364217	17523506	17.494	17.755
27)	SA Decachlor...	7.993	9.009	22660594	29429991	33.484	31.459
Target Compounds							
9)	A Endosulfan I	0.000	6.227f	0	1676505	N.D.	1.349
10)	B trans-Chl...	0.000	6.053	0	7344466	N.D.	5.318
13)	MA Dieldrin	5.529	6.471	2835671	4861103	3.036	3.606
15)	B Endosulfa...	0.000	6.862	0	1552342	N.D.	1.246
16)	A 4,4'-DDD	0.000	6.783	0	4800701	N.D.	4.505
17)	MA 4,4'-DDT	0.000	7.105	0	1850161	N.D.	1.781
19)	B Endosulfa...	0.000	7.212	0	4049767	N.D.	3.549
22)	Toxaphene-1	5.529	0.000	2835671	0	540.046	N.D. #
24)	Toxaphene-3	0.000	7.105	0	1850161	N.D.	169.354
25)	Toxaphene-4	0.000	7.105	0	1850161	N.D.	61.698
26)	Toxaphene-5	0.000	7.613	0	2447693	N.D.	142.173


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091119\
Data File : PD054475.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Sep 2019 17:13
Operator : SG\AJ
Sample : K4717-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 00:52:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090419CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 05 08:40:10 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

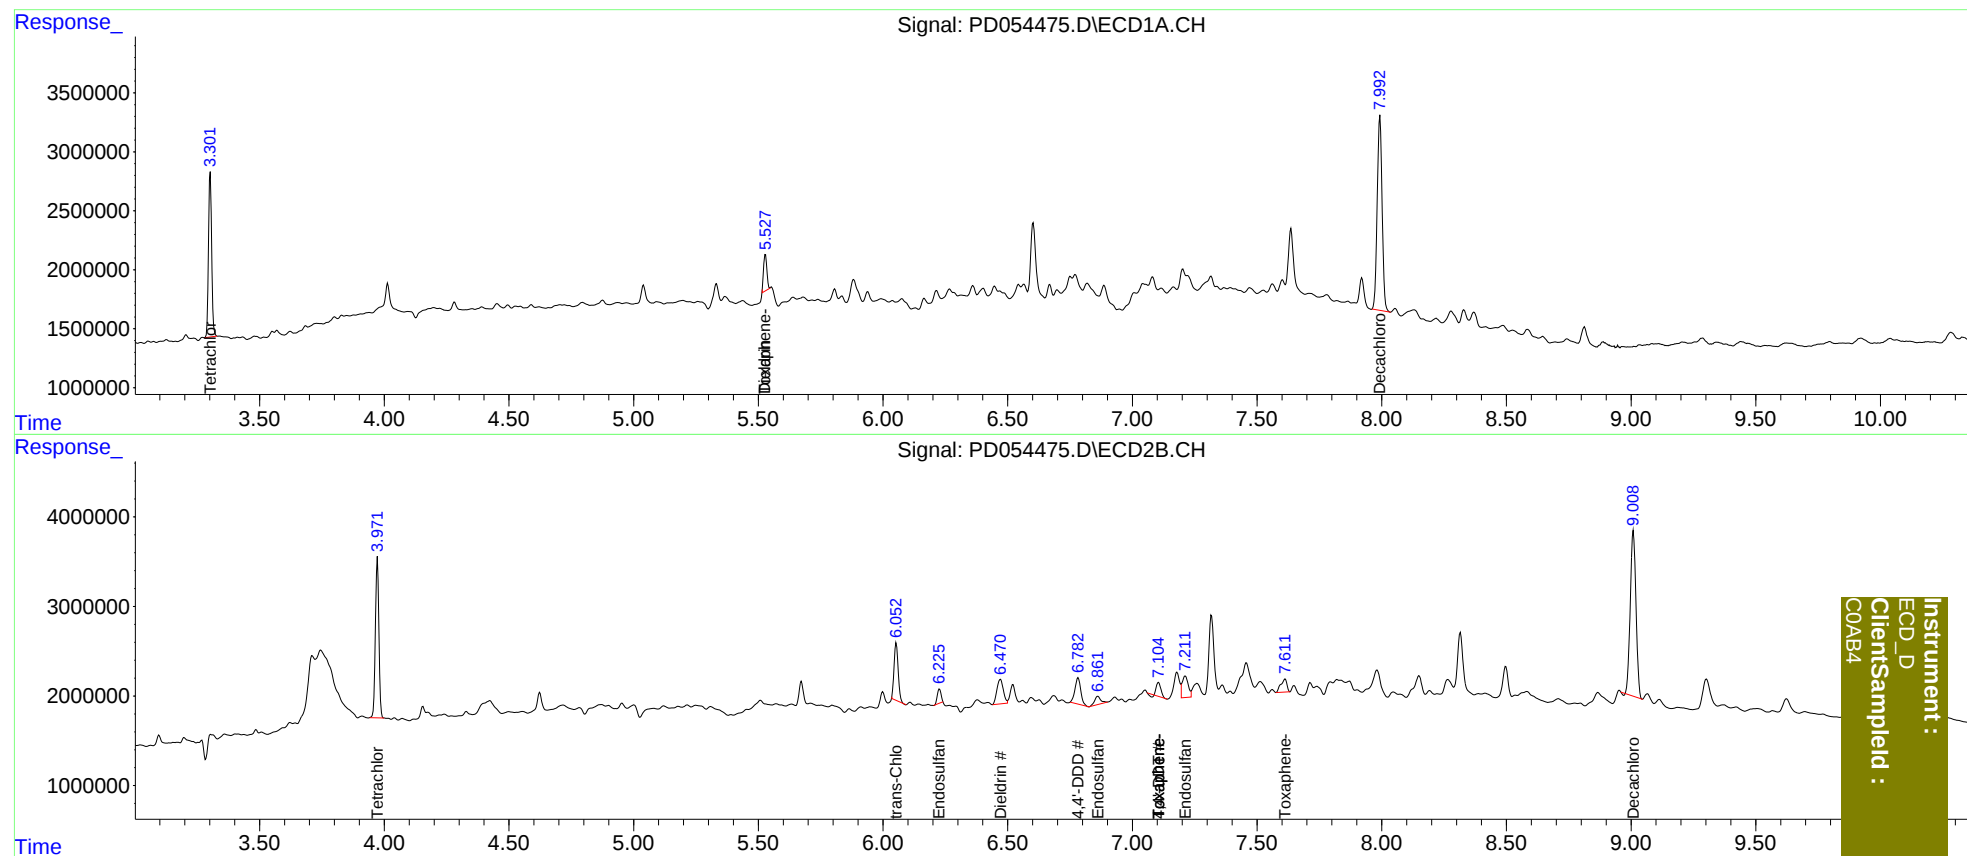


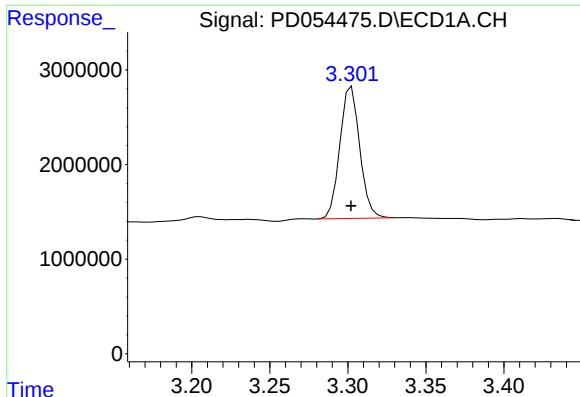

#1 Tetrachloro-m-xylene


R.T.: 3.302 min
Delta R.T.: 0.000 min
Response: 12364217
Conc: 17.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AB4

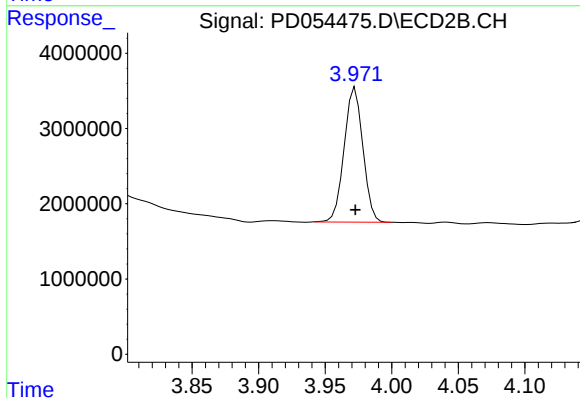


#1 Tetrachloro-m-xylene

R.T.: 3.973 min
Delta R.T.: 0.000 min
Response: 17523506
Conc: 17.76 ng/ml

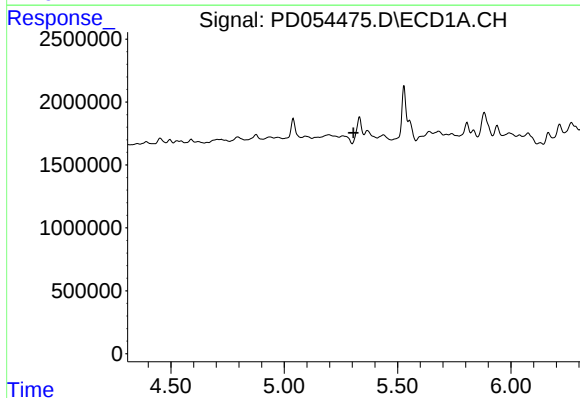


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.306 min
Response: 0
Conc: N.D.

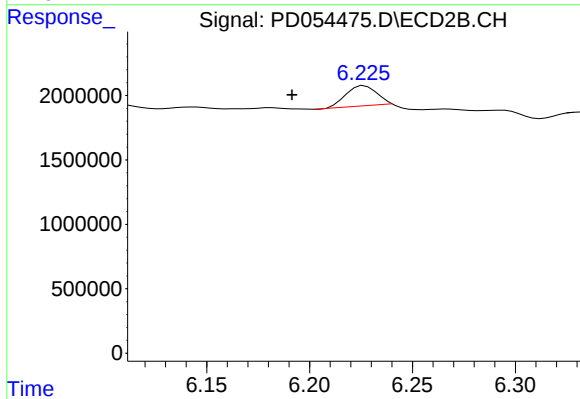

#9 Endosulfan I


R.T.: 6.227 min
Delta R.T.: 0.035 min
Response: 1676505
Conc: 1.35 ng/ml

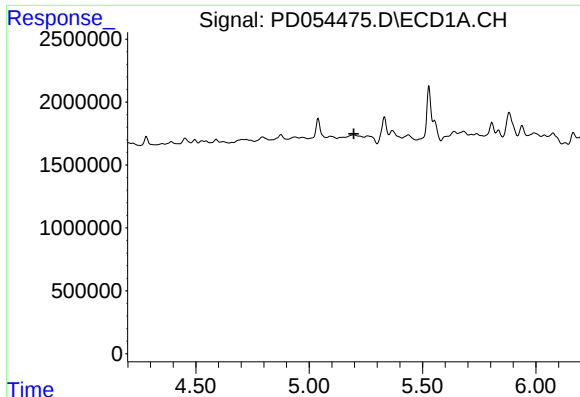

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.197 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0AB4

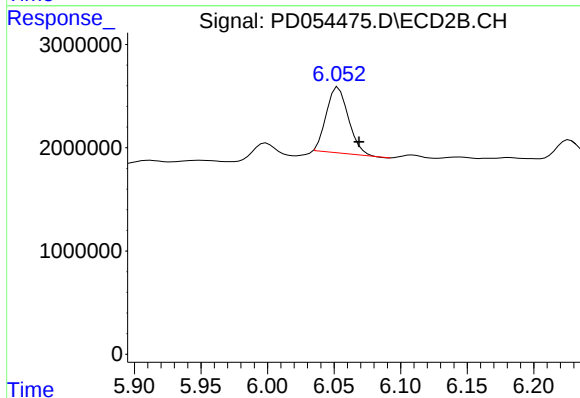


#10 trans-Chlordane

R.T.: 6.053 min
Delta R.T.: -0.016 min
Response: 7344466
Conc: 5.32 ng/ml

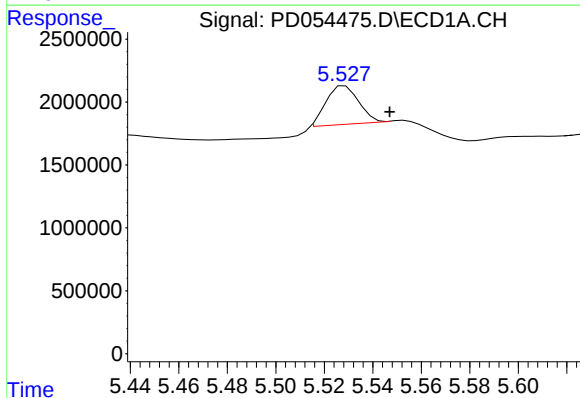


#13 Dieldrin

R.T.: 5.529 min
Delta R.T.: -0.018 min
Response: 2835671
Conc: 3.04 ng/ml

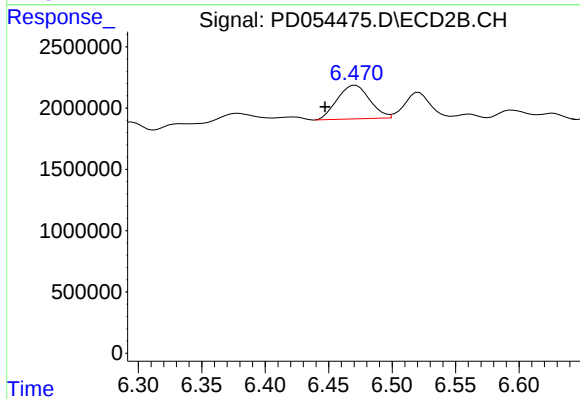

#13 Dieldrin


R.T.: 6.471 min
Delta R.T.: 0.024 min
Response: 4861103
Conc: 3.61 ng/ml

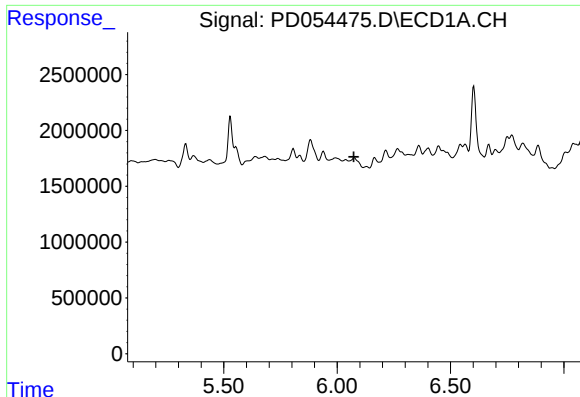

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.073 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0AB4

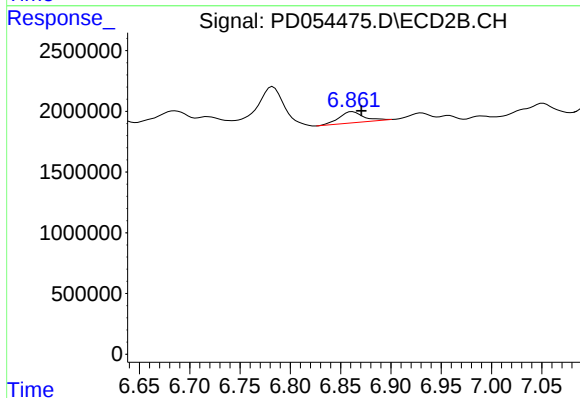


#15 Endosulfan II

R.T.: 6.862 min
Delta R.T.: -0.009 min
Response: 1552342
Conc: 1.25 ng/ml

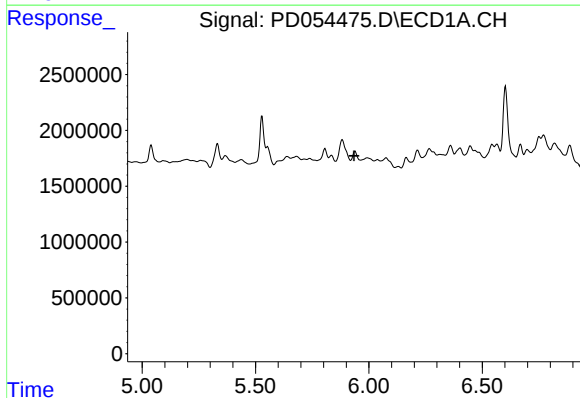


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.935 min
Response: 0
Conc: N.D.

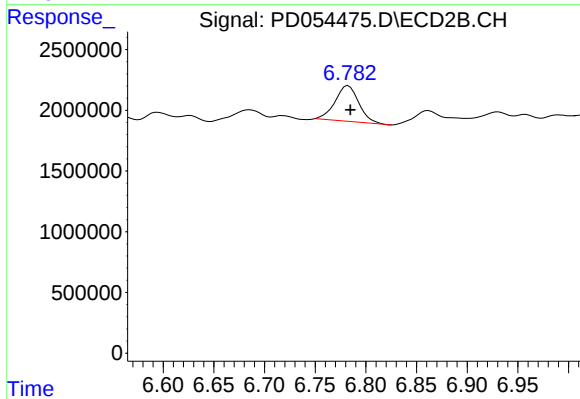

#16 4,4'-DDD


R.T.: 6.783 min
Delta R.T.: -0.002 min
Response: 4800701
Conc: 4.50 ng/ml

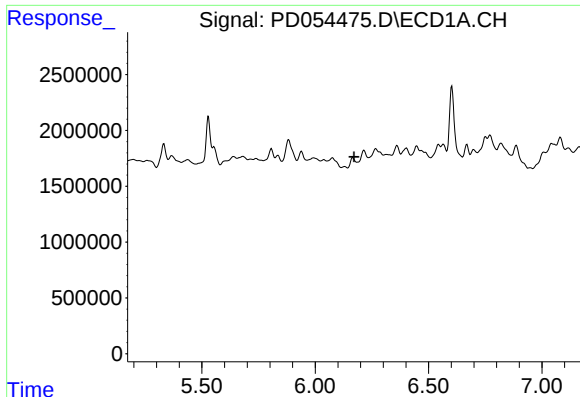

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0AB4

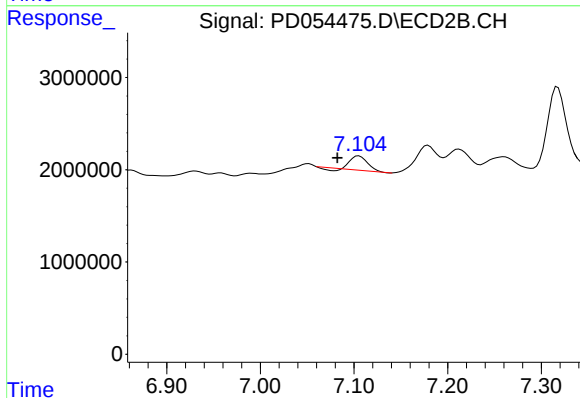


#17 4,4'-DDT

R.T.: 7.105 min
Delta R.T.: 0.023 min
Response: 1850161
Conc: 1.78 ng/ml

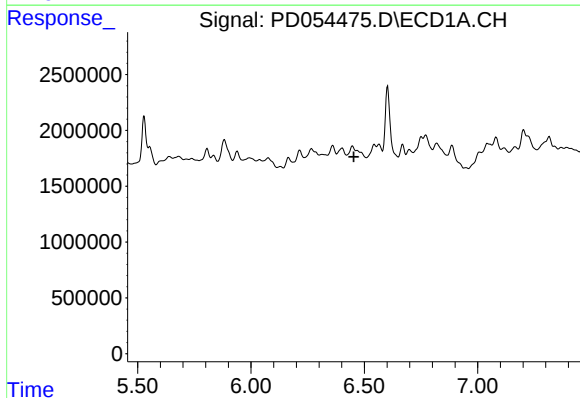


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.454 min
Response: 0
Conc: N.D.

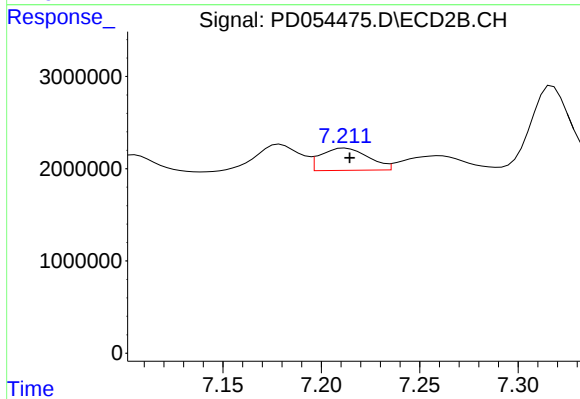

#19 Endosulfan Sulfate


R.T.: 7.212 min
Delta R.T.: -0.002 min
Response: 4049767
Conc: 3.55 ng/ml

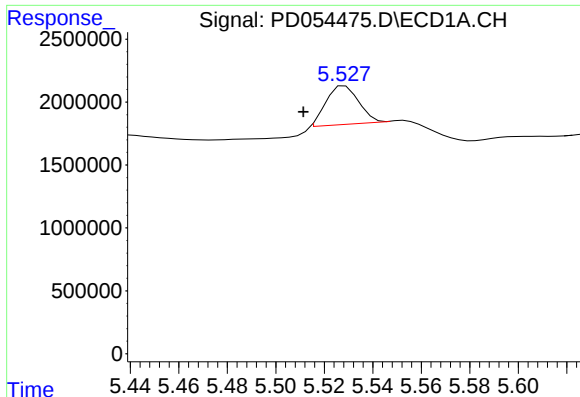

#22 Toxaphene-1


R.T.: 5.529 min
Delta R.T.: 0.017 min
Response: 2835671
Conc: 540.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AB4

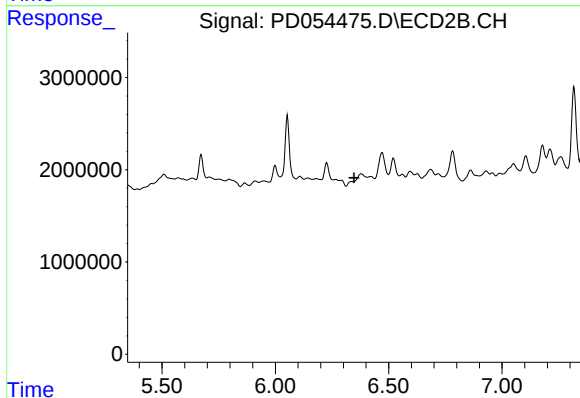


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T. : 6.348 min
Response: 0
Conc: N.D.

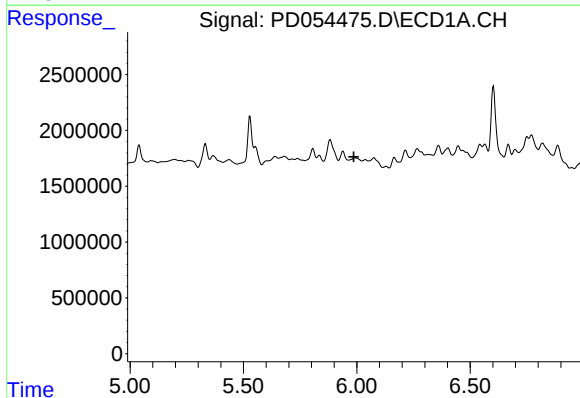


#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T. : 5.988 min
Response: 0
Conc: N.D.

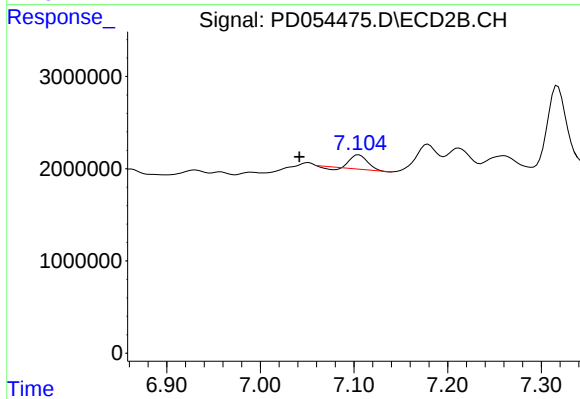

#24 Toxaphene-3


R.T.: 7.105 min
Delta R.T.: 0.063 min
Response: 1850161
Conc: 169.35 ng/ml

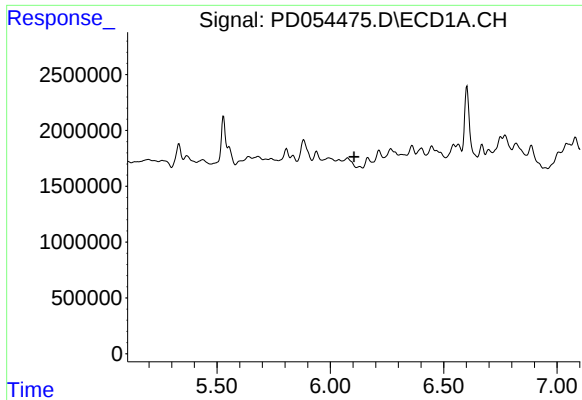

#25 Toxaphene-4


R.T.: 0.000 min
Exp R.T.: 6.105 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0AB4

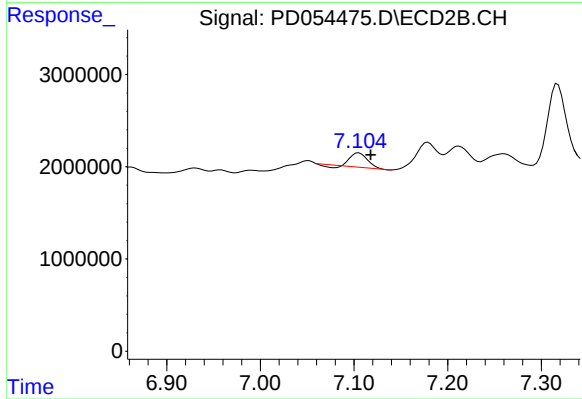


#25 Toxaphene-4

R.T.: 7.105 min
Delta R.T.: -0.013 min
Response: 1850161
Conc: 61.70 ng/ml

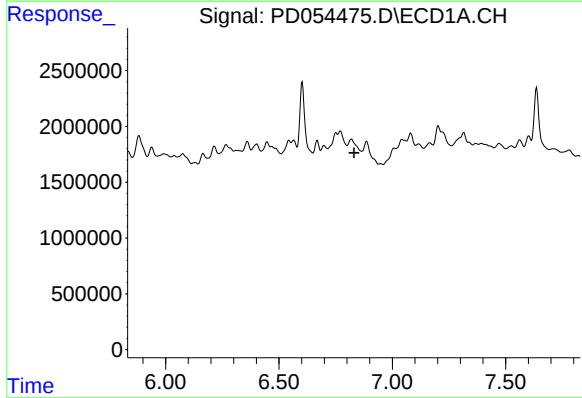


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T.: 6.832 min
Response: 0
Conc: N.D.

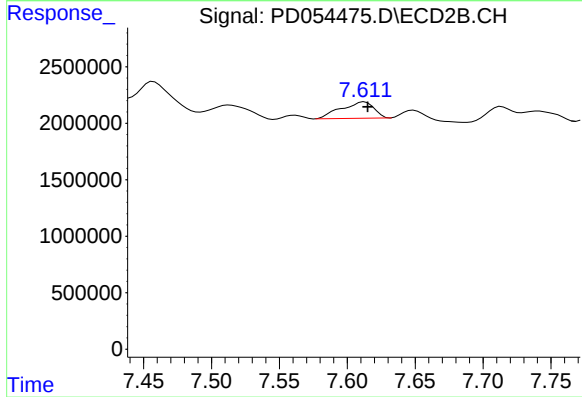

#26 Toxaphene-5


R.T.: 7.613 min
Delta R.T.: -0.002 min
Response: 2447693
Conc: 142.17 ng/ml

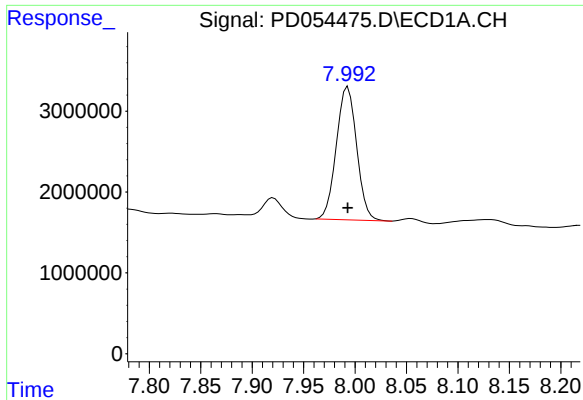

#27 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: 0.000 min
Response: 22660594
Conc: 33.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AB4

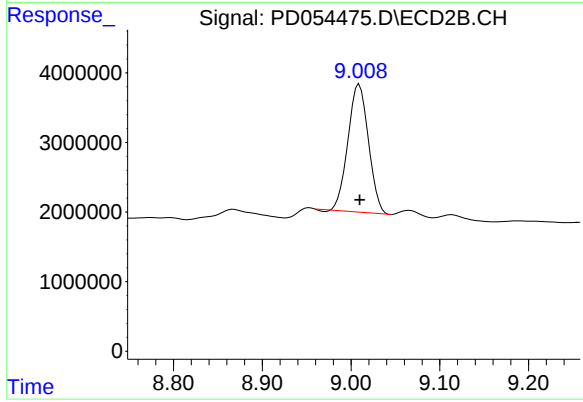

#27 Decachlorobiphenyl

R.T.: 9.009 min
Delta R.T.: 0.000 min
Response: 29429991
Conc: 31.46 ng/ml