

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091120\
 Data File : PD059172.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2020 10:11
 Operator : DD\AJ
 Sample : MDL-S-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-S-05

Manual Integrations
 APPROVED

Ankita
 9/14/2020 11:05:12 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 10:26:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090420CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 05 02:06:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.205	3.864	19456064	34916626	19.301	21.307
27)	SA Decachlor...	7.838	8.857	37664698	53696064	38.432	39.925
Target Compounds							
2)	A alpha-BHC	3.627	4.246	1393029	2386332	0.888	0.983
3)	MA gamma-BHC...	3.898	4.527	1430887	2072110	0.903	0.940
4)	MA Heptachlor	4.177	5.027	1155398	2051678	1.029	0.974
5)	MB Aldrin	4.411	5.326	1241797	2000808	0.954	0.970
6)	B beta-BHC	4.147	4.699	649354	877145	1.059	0.921
7)	B delta-BHC	4.337	4.910	1396369	2104383	0.960	1.048
8)	B Heptachlo...	4.843	5.710	1165843	2185909	1.021	1.089
9)	A Endosulfan I	5.169	6.063	1148869	1717935	1.076	1.011
10)	B trans-Chl...	5.063	5.943	1268977	1920760	1.062	1.032
11)	B cis-Chlor...	5.119	6.015	1260192	1897171	1.056	1.007
12)	B 4,4'-DDE	5.288	6.175	1052974	1679994	0.888	0.946
13)	MA Dieldrin	5.407	6.318	1084506	1759462	0.964	0.950
14)	MA Endrin	5.659	6.534	971408	1463064	1.048	0.908
15)	B Endosulfa...	5.930	6.744	1024890	1621204	1.000m	1.049
16)	A 4,4'-DDD	5.795	6.662	849446	1340285	1.067m	0.940
17)	MA 4,4'-DDT	6.028	6.959	790421	1005692	0.932	0.686 #
18)	B Endrin al...	6.099	6.867	611349	1576530	0.776	1.174 #
19)	B Endosulfa...	6.309	7.090	911209	1587516	0.942	1.005
20)	A Methoxychlor	6.576	7.418	263097	684196	0.738m	0.887m
21)	B Endrin ke...	6.789	7.555	1156920	1821564	1.078	1.069

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091120\
Data File : PD059172.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2020 10:11
Operator : DD\AJ
Sample : MDL-S-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 10:26:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090420CLP.M
Quant Title : GC Extractables
QLast Update : Sat Sep 05 02:06:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

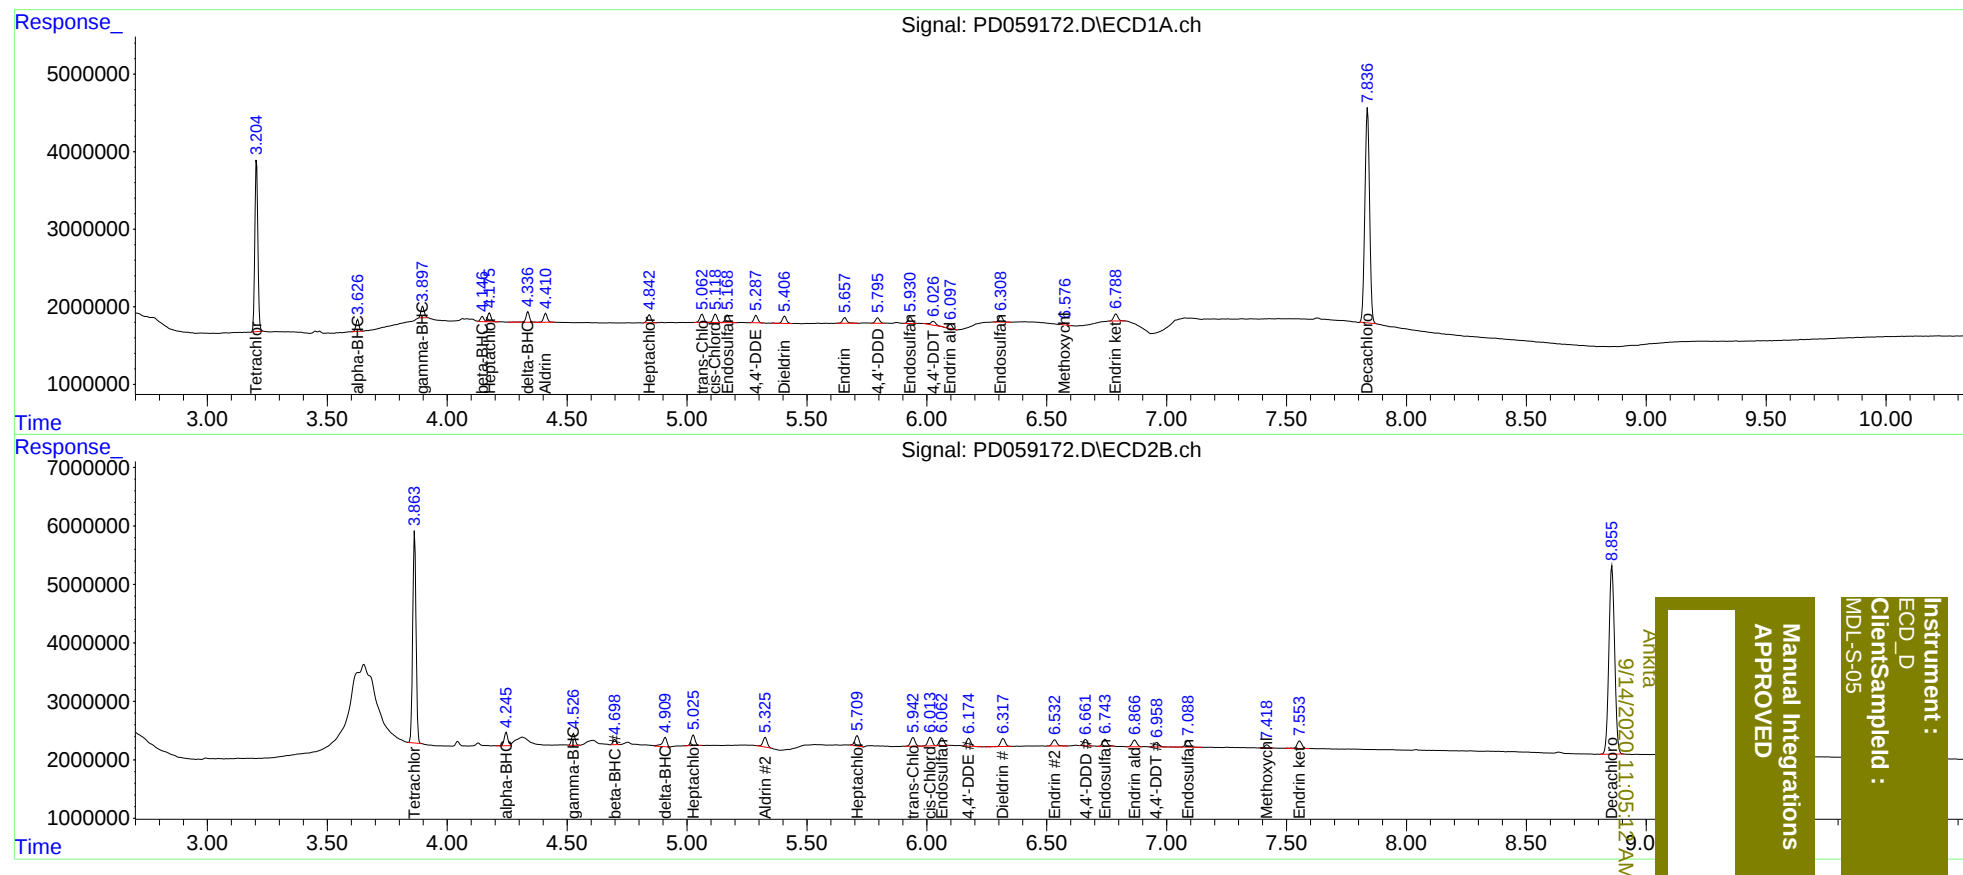

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sample :
MDL-S-05

9/14/2020 11:05:12 AM