

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091120\
 Data File : PD059188.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2020 14:09
 Operator : DD\AJ
 Sample : MDL-TOX-S-2
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-TOX-S-2

Manual Integrations
 APPROVED

Ankita
 9/14/2020 11:05:43 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 14:26:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090420CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 05 02:06:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.206	3.865	16771591	30004835	16.638	18.310
27)	SA Decachlor...	7.839	8.859	33052835	46571361	33.726	34.628
Target Compounds							
22)	Toxaphene-1	5.374	6.221	542031	804415	83.189m	88.053
23)	Toxaphene-2	5.847	6.508	470916	961425	93.135	84.014
24)	Toxaphene-3	5.964	6.912	1494804	1064904	84.890	79.667
25)	Toxaphene-4	6.208	6.990	1405202	3399173	83.101	81.651
26)	Toxaphene-5	6.683	7.485	1465402	2042003	73.082	101.008 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091120\
Data File : PD059188.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2020 14:09
Operator : DD\AJ
Sample : MDL-TOX-S-2
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 14:26:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090420CLP.M
Quant Title : GC Extractables
QLast Update : Sat Sep 05 02:06:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

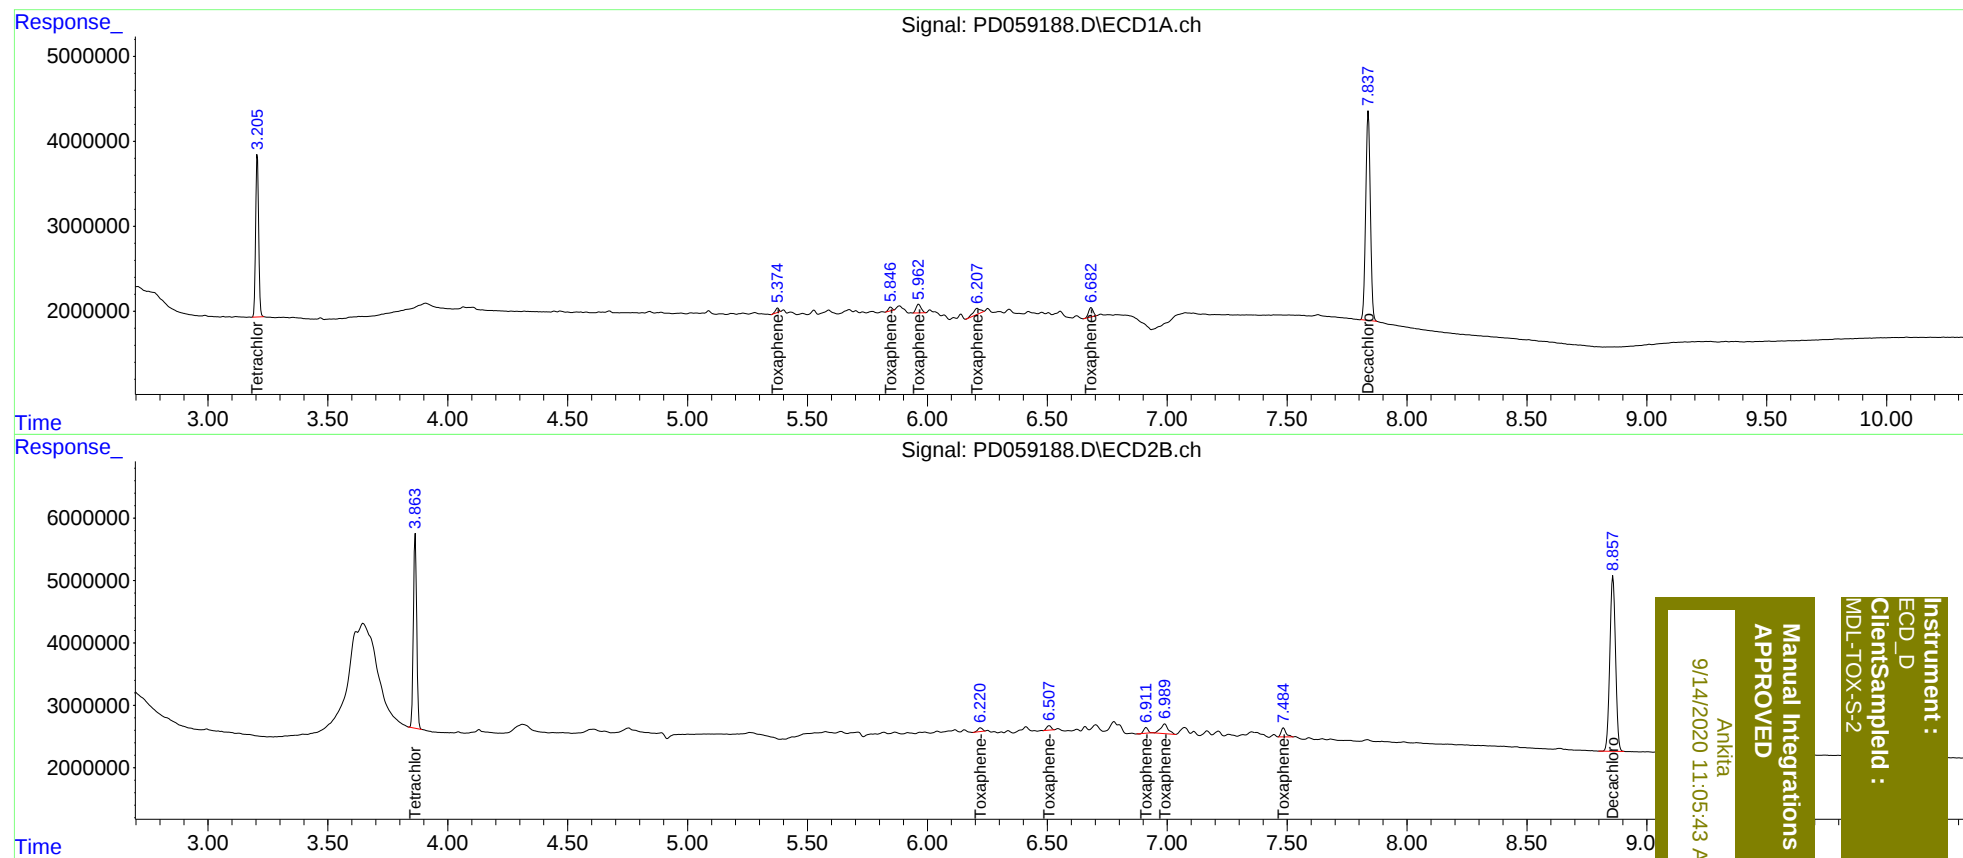

Manual Integrations
APPROVED

Ankita

9/14/2020 11:05:43 AM

Instrument :
ECD_D
ClientSampled :
MDL-TOX-S-2