

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091120\
 Data File : PD059170.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2020 09:43
 Operator : DD\AJ
 Sample : MDL-S-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-S-03

Manual Integrations
 APPROVED

Ankita
 9/14/2020 11:05:08 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 10:29:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090420CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 05 02:06:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.205	3.864	19714357	35572333	19.558	21.707
27)	SA Decachlor...	7.837	8.858	37793142	53881177	38.563	40.063
Target Compounds							
2)	A alpha-BHC	3.627	4.246	1380969	2503297	0.880	1.031
3)	MA gamma-BHC...	3.898	4.527	1567971	2106852	0.990	0.956
4)	MA Heptachlor	4.176	5.027	1170613	2085260	1.042	0.990
5)	MB Aldrin	4.410	5.326	1215977	2249048	0.934	1.090
6)	B beta-BHC	4.147	4.699	671701	918581	1.095	0.964
7)	B delta-BHC	4.337	4.910	1340812	2088040	0.922	1.040
8)	B Heptachlo...	4.843	5.710	1170090	2384974	1.024	1.188
9)	A Endosulfan I	5.169	6.063	1175704	2263226	1.101	1.332
10)	B trans-Chl...	5.063	5.943	1213460	2039734	1.016	1.096
11)	B cis-Chlor...	5.119	6.015	1272489	2262750	1.066	1.201
12)	B 4,4'-DDE	5.288	6.175	1090440	2141417	0.920	1.206 #
13)	MA Dieldrin	5.407	6.318	1091169	1846067	0.970	0.997
14)	MA Endrin	5.658	6.533	946947	1465460	1.022	0.909
15)	B Endosulfa...	5.932	6.744	1036138	1631269	1.011	1.055
16)	A 4,4'-DDD	5.796	6.662	945471	1264015	1.188	0.886 #
17)	MA 4,4'-DDT	6.028	6.959	675969	999577	0.797	0.681
18)	B Endrin al...	6.097	6.868	648128	1492218	0.823	1.111 #
19)	B Endosulfa...	6.309	7.090	930634	1679991	0.963	1.064
20)	A Methoxychlor	6.575	7.419	248588	661605	0.698m	0.858m
21)	B Endrin ke...	6.790	7.555	1137130	2055639	1.060	1.206

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091120\
Data File : PD059170.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2020 09:43
Operator : DD\AJ
Sample : MDL-S-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 10:29:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090420CLP.M
Quant Title : GC Extractables
QLast Update : Sat Sep 05 02:06:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

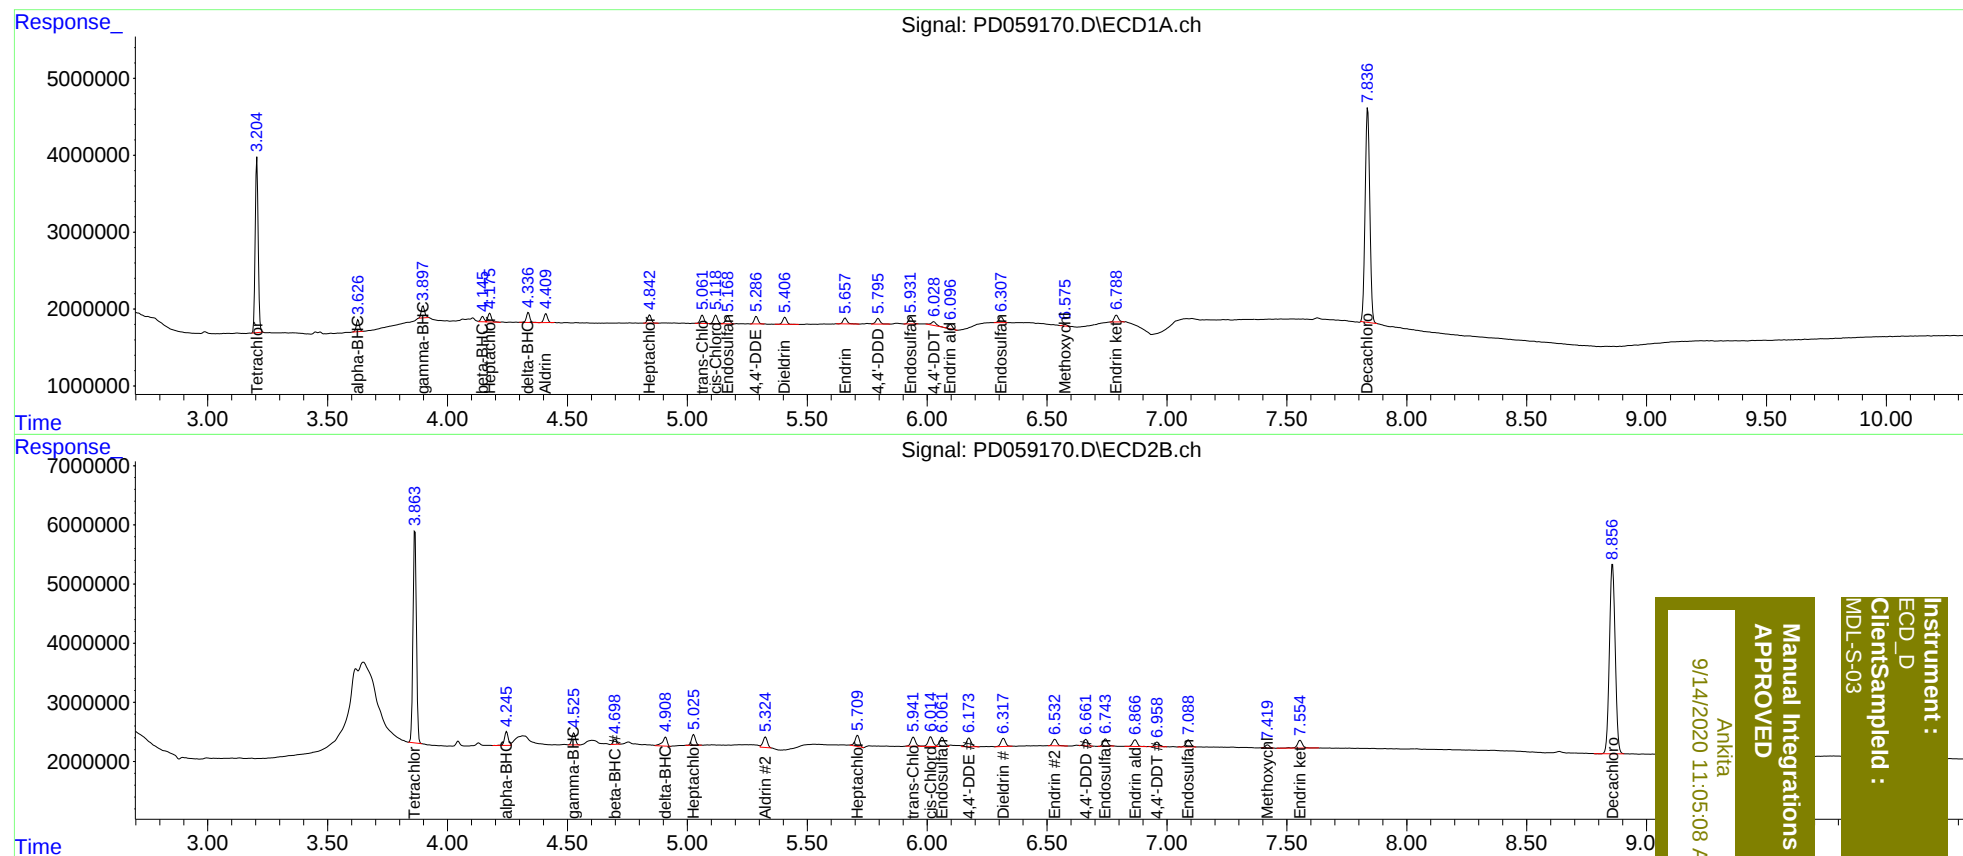

Manual Integrations
APPROVED

Ankita

9/14/2020 11:05:08 AM

Instrument :
ECD_D
Client Sample :
MDL-S-03