

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091120\
 Data File : PD059173.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2020 10:25
 Operator : DD\AJ
 Sample : MDL-S-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-S-06

Manual Integrations
 APPROVED

Ankita
 9/14/2020 11:05:14 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 10:37:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090420CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 05 02:06:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.206	3.865	13476964	23988952	13.370	14.639
27)	SA Decachlor...	7.837	8.858	26177211	37915795	26.711	28.192
Target Compounds							
2)	A alpha-BHC	3.628	4.247	917581	1651540	0.585	0.680
3)	MA gamma-BHC...	3.899	4.527	1052553	1371527	0.665	0.622
4)	MA Heptachlor	4.177	5.027	763000	1435233	0.679	0.681
5)	MB Aldrin	4.411	5.326	854835	1698477	0.657	0.823 #
6)	B beta-BHC	4.147	4.700	456525	617532	0.744	0.648
7)	B delta-BHC	4.337	4.909	918805	1418855	0.632	0.707
8)	B Heptachlo...	4.844	5.710	779852	1680670	0.683	0.837
9)	A Endosulfan I	5.170	6.063	781172	1639588	0.732	0.965 #
10)	B trans-Chl...	5.063	5.943	831116	1436352	0.696	0.772
11)	B cis-Chlor...	5.119	6.015	809638	1696837	0.678	0.901 #
12)	B 4,4'-DDE	5.289	6.175	751338	1469943	0.634	0.828 #
13)	MA Dieldrin	5.407	6.319	762336	1238325	0.677	0.669
14)	MA Endrin	5.657	6.534	580390	941420	0.626m	0.584
15)	B Endosulfa...	5.932	6.743	653001	1210383	0.637	0.783
16)	A 4,4'-DDD	5.796	6.661	523730	895797	0.658	0.628m
17)	MA 4,4'-DDT	6.028	6.957	324532	706388	0.383m	0.482m#
18)	B Endrin al...	6.098	6.866	451380	1064150	0.573m	0.792 #
19)	B Endosulfa...	6.309	7.089	649363	1113107	0.672	0.705
20)	A Methoxychlor	6.578	7.417	218168	554561	0.612m	0.719m
21)	B Endrin ke...	6.789	7.555	821930	1332584	0.766	0.782

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091120\
Data File : PD059173.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2020 10:25
Operator : DD\AJ
Sample : MDL-S-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 10:37:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090420CLP.M
Quant Title : GC Extractables
QLast Update : Sat Sep 05 02:06:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

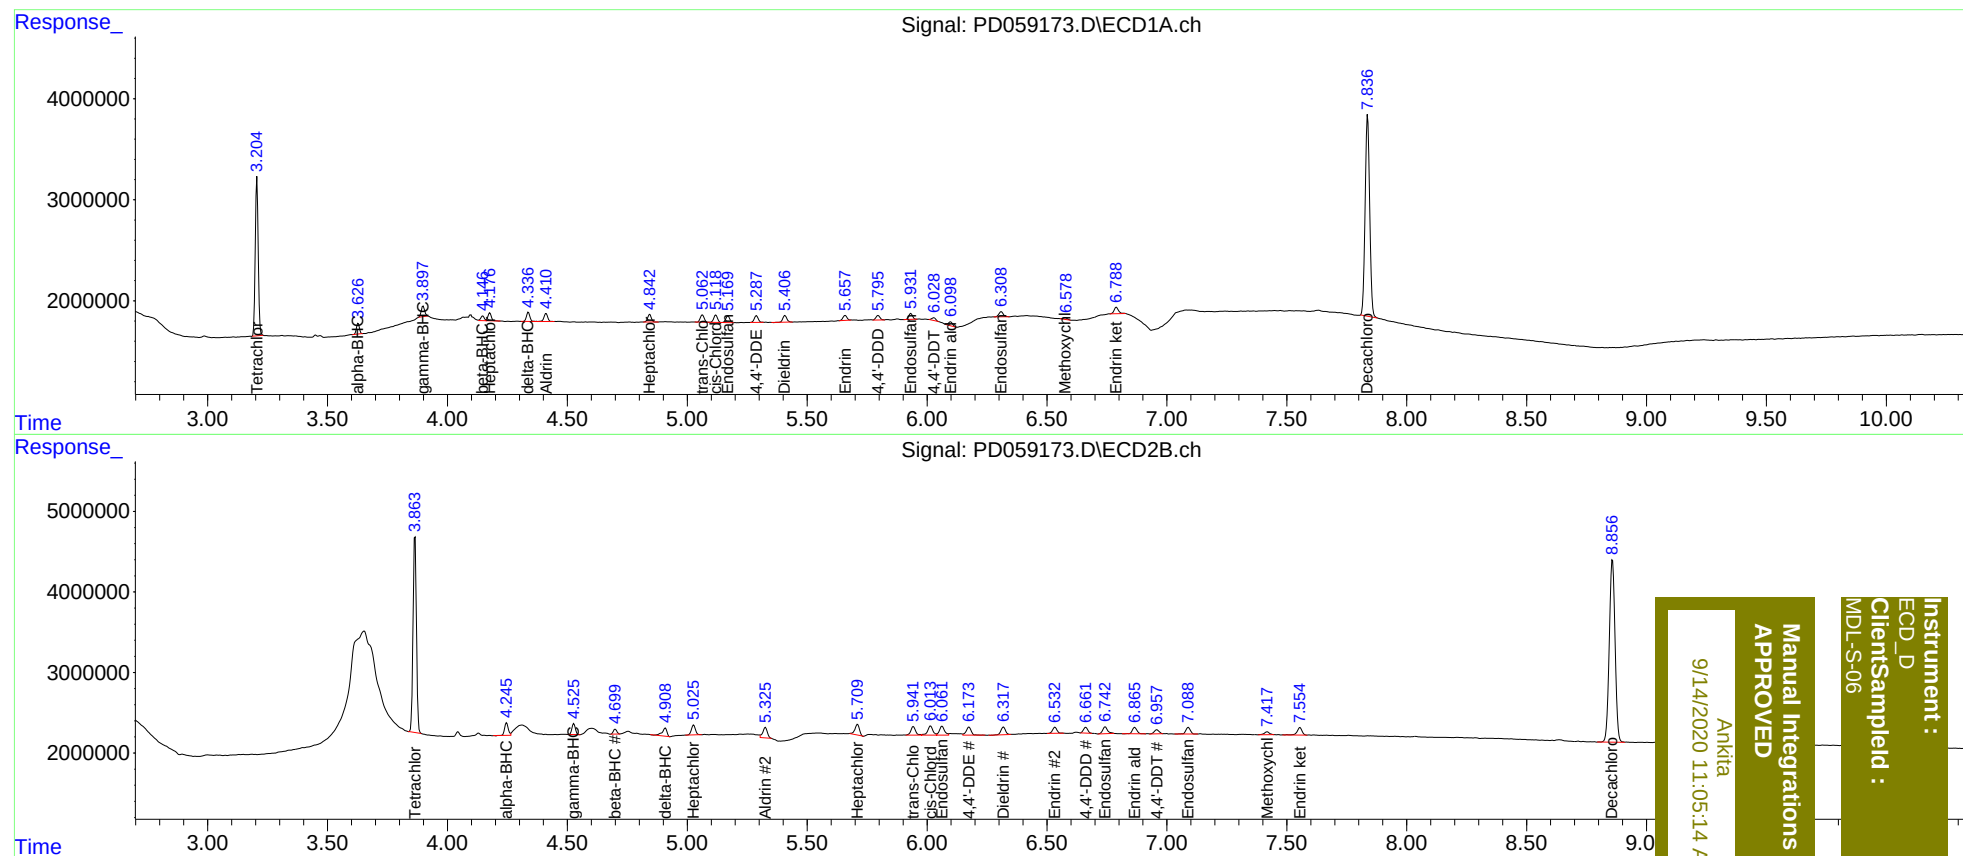

Manual Integrations
APPROVED

Ankita
9/14/2020 11:05:14 AM

Instrument :
ECD_D
Client Sampled :
MDL-S-06