

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091120\
 Data File : PD059174.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2020 10:39
 Operator : DD\AJ
 Sample : MDL-S-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-S-07

Manual Integrations
 APPROVED

Ankita
 9/14/2020 11:05:16 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 10:55:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090420CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 05 02:06:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.206	3.865	14974910	26778978	14.856	16.341
2)	SA Decachlor...	7.837	8.857	29025494	41404009	29.617	30.785
Target Compounds							
2)	A alpha-BHC	3.627	4.246	1100192	1867201	0.701	0.769
3)	MA gamma-BHC...	3.898	4.527	1107248	1576126	0.699	0.715
4)	MA Heptachlor	4.176	5.027	933180	1538996	0.831	0.731
5)	MB Aldrin	4.411	5.326	972424	1950111	0.747	0.945 #
6)	B beta-BHC	4.147	4.700	580579	673311	0.947	0.707 #
7)	B delta-BHC	4.337	4.909	1061948	1798751	0.730	0.896
8)	B Heptachlo...	4.844	5.711	898346	1823138	0.786	0.908
9)	A Endosulfan I	5.170	6.063	853452	1501492	0.800	0.884
10)	B trans-Chl...	5.063	5.943	922506	1508220	0.772	0.810
11)	B cis-Chlor...	5.119	6.015	961640	1477951	0.806	0.784
12)	B 4,4'-DDE	5.288	6.175	842472	1385866	0.710	0.781
13)	MA Dieldrin	5.408	6.318	893506	1397462	0.794	0.755
14)	MA Endrin	5.658	6.533	812744	1134729	0.877	0.704
15)	B Endosulfa...	5.932	6.742	785930	1342459	0.767	0.868m
16)	A 4,4'-DDD	5.796	6.660	645705	1011004	0.811	0.709m
17)	MA 4,4'-DDT	6.027	6.958	367690	748496	0.434m	0.510
18)	B Endrin al...	6.098	6.867	429965	1149794	0.546	0.856 #
19)	B Endosulfa...	6.309	7.089	701702	1289246	0.726	0.817
20)	A Methoxychlor	6.577	7.417	217989	571305	0.612m	0.740m
21)	B Endrin ke...	6.789	7.555	955149	1380614	0.890	0.810

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091120\
Data File : PD059174.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2020 10:39
Operator : DD\AJ
Sample : MDL-S-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 10:55:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090420CLP.M
Quant Title : GC Extractables
QLast Update : Sat Sep 05 02:06:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

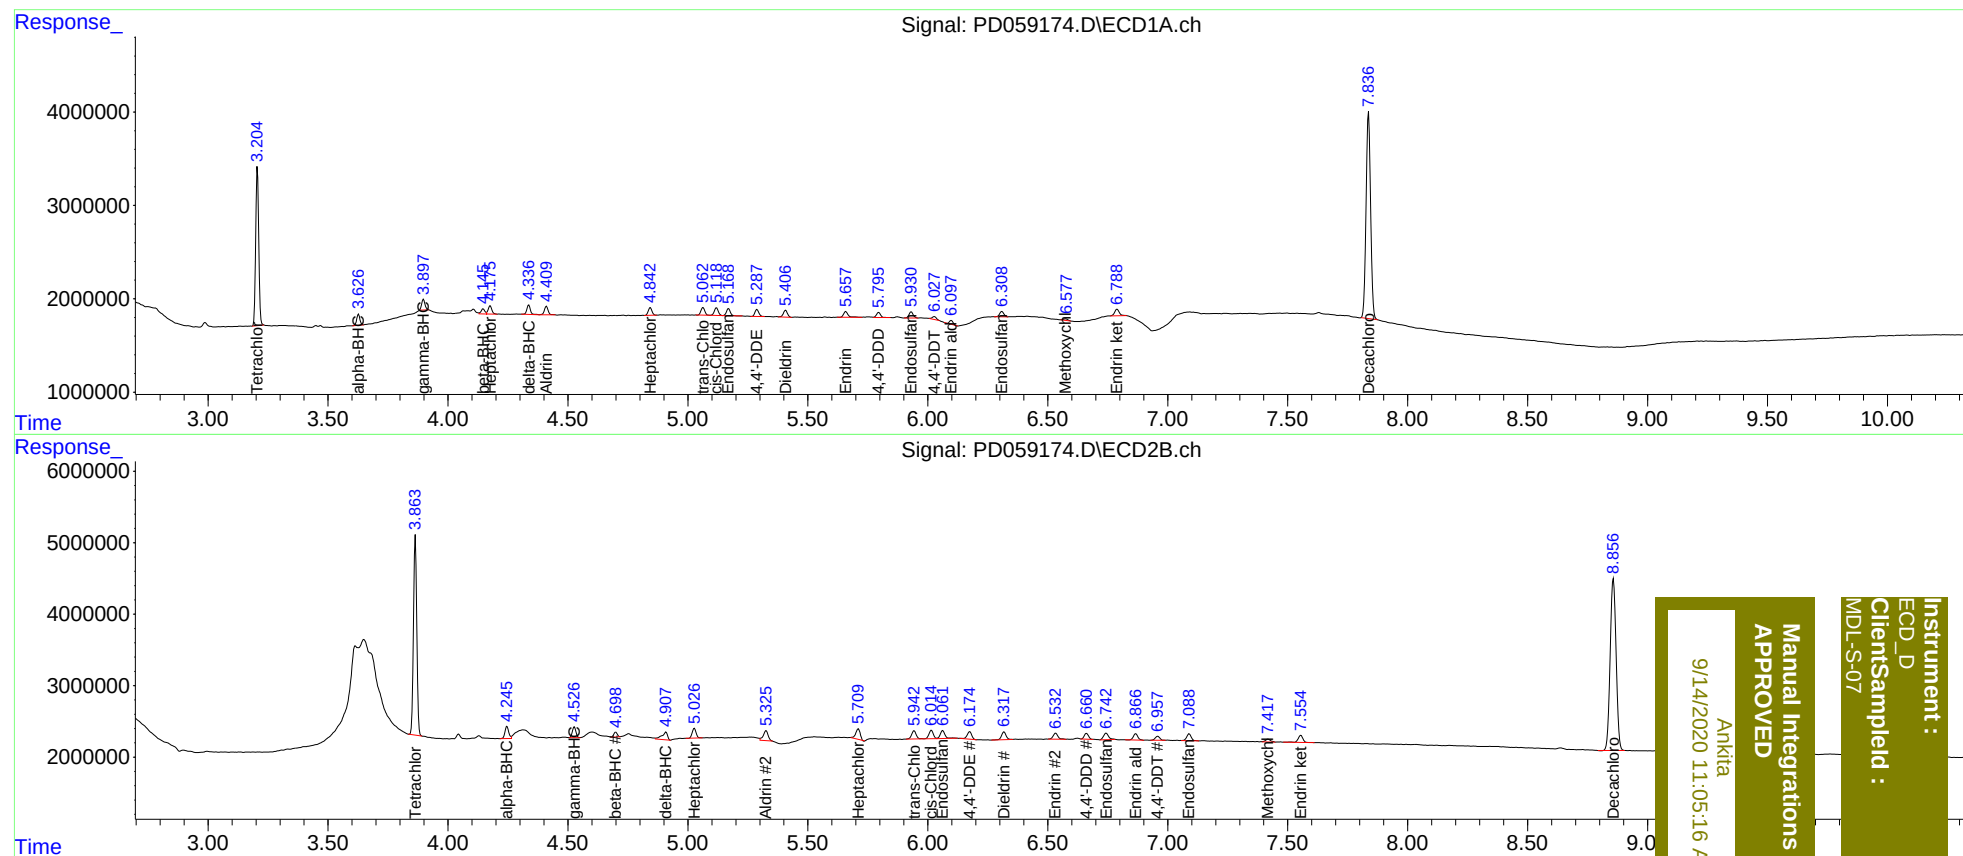

Manual Integrations
APPROVED

Ankita
9/14/2020 11:05:16 AM

Instrument :
ECD_D
Client Sample :
MDL-S-07