

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091123\
 Data File : PD077827.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2023 10:32
 Operator : AR\AJ
 Sample : TOXAPH501
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 11:29:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091123CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 11 11:20:25 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.760	241.8E6	152.2E6	79.894	80.040
27)	SA Decachlor...	9.084	7.900	557.3E6	322.6E6	157.856	160.043
Target Compounds							
22)	Toxaphene-1	6.248	5.313	217.8E6	96734550	8002.757	8061.534
23)	Toxaphene-2	6.453	5.672	275.1E6	110.9E6	8039.923	8088.314
24)	Toxaphene-3	6.652	5.955	191.6E6	123.4E6	8181.229	7983.907
25)	Toxaphene-4	7.163	6.588	624.5E6	391.3E6	8103.893	8280.467
26)	Toxaphene-5	7.586	6.714	454.1E6	514.0E6	8228.687	8211.324

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091123\
Data File : PD077827.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2023 10:32
Operator : AR\AJ
Sample : TOXAPH501
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 11:29:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091123CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Mon Sep 11 11:20:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

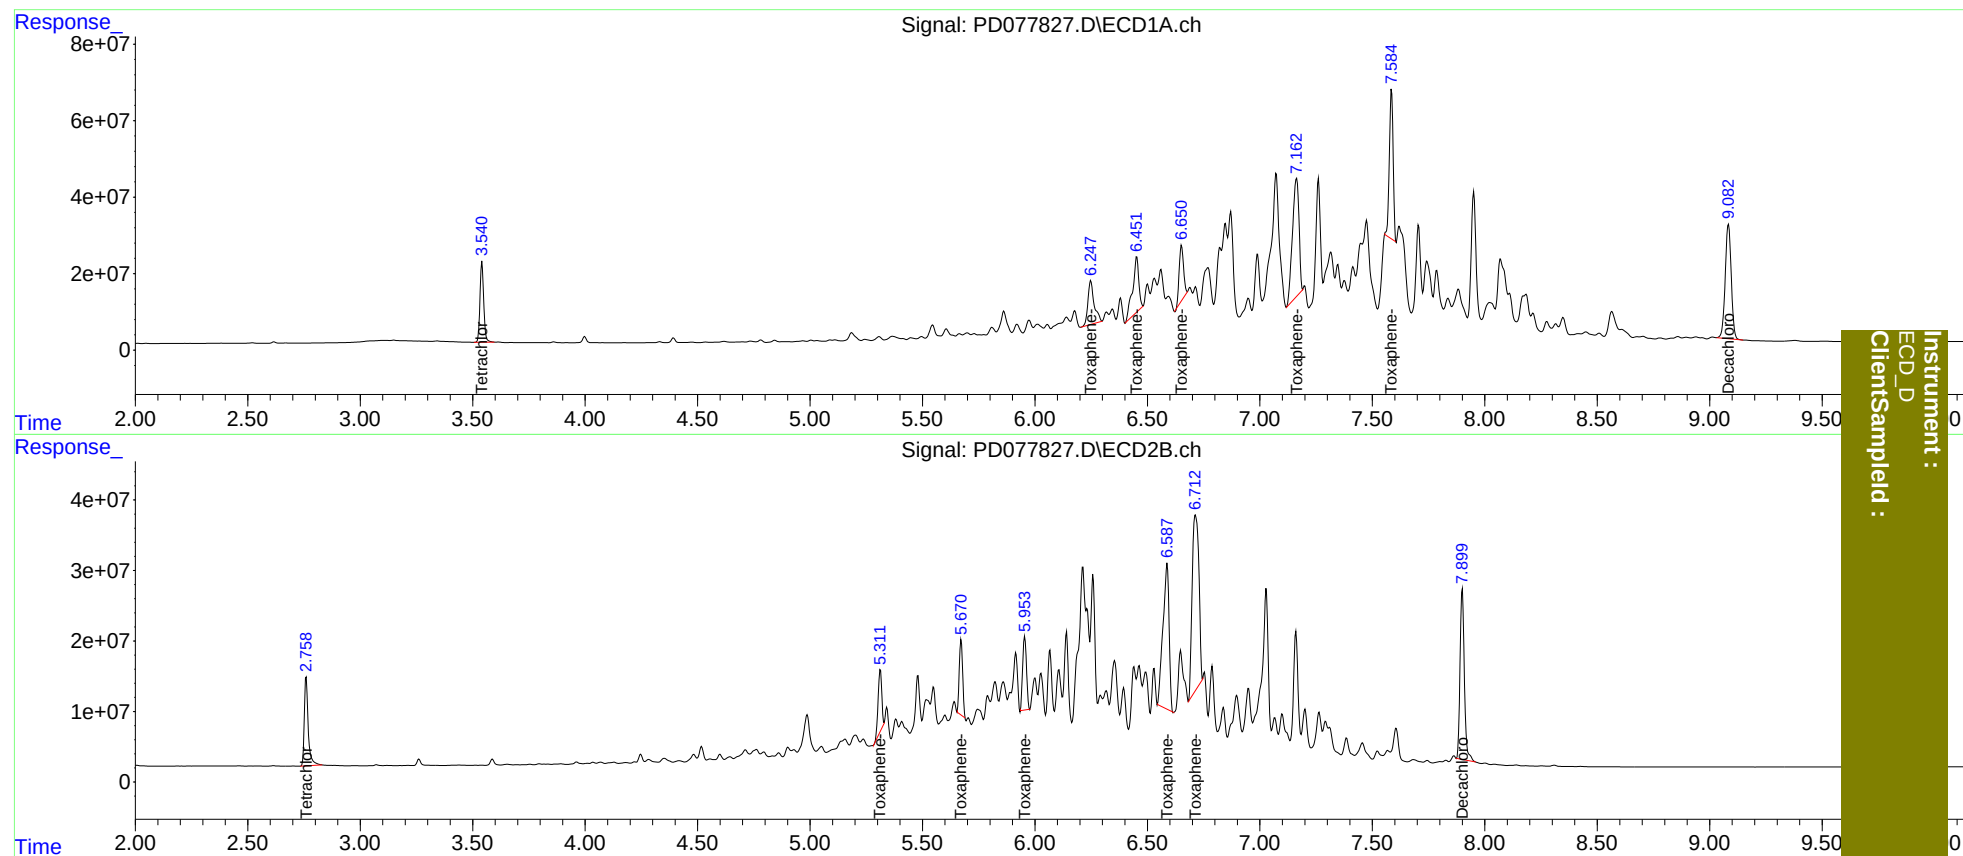

Instrument :
ECD_D
ClientSampled :
0