

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091123\
 Data File : PD077855.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2023 17:32
 Operator : AR\AJ
 Sample : PIBLK266
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 22:12:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091123CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 11 14:09:05 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.760	55375787	34121030	21.737	21.565
27)	SA Decachlor...	9.082	7.899	134.2E6	72605089	43.018	42.093
Target Compounds							
2)	A alpha-BHC	3.948f	3.250	372338	49308	<MDL	<MDL #
3)	MA gamma-BHC...	0.000	3.603	0	200844	N.D.	<MDL
4)	MA Heptachlor	4.911	3.893f	157288	119283	<MDL	<MDL #
5)	MB Aldrin	0.000	4.217	0	237485	N.D.	<MDL
6)	B beta-BHC	0.000	3.893	0	119283	N.D.	0.115
7)	B delta-BHC	4.766	0.000	3395347	0	0.816	N.D. #
8)	B Heptachlo...	5.688	0.000	4732202	0	1.229	N.D. #
10)	B trans-Chl...	5.982	0.000	325271	0	<MDL	N.D. #
11)	B cis-Chlor...	5.982f	0.000	325271	0	<MDL	N.D. #
14)	MA Endrin	6.517f	5.640	148079	207831	<MDL	0.108 #
21)	B Endrin ke...	7.689	0.000	175346	0	<MDL	N.D. #
23)	Toxaphene-2	6.488f	5.640	356586	207831	10.691	16.003 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091123\
Data File : PD077855.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2023 17:32
Operator : AR\AJ
Sample : PIBLK266
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 22:12:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091123CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Mon Sep 11 14:09:05 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

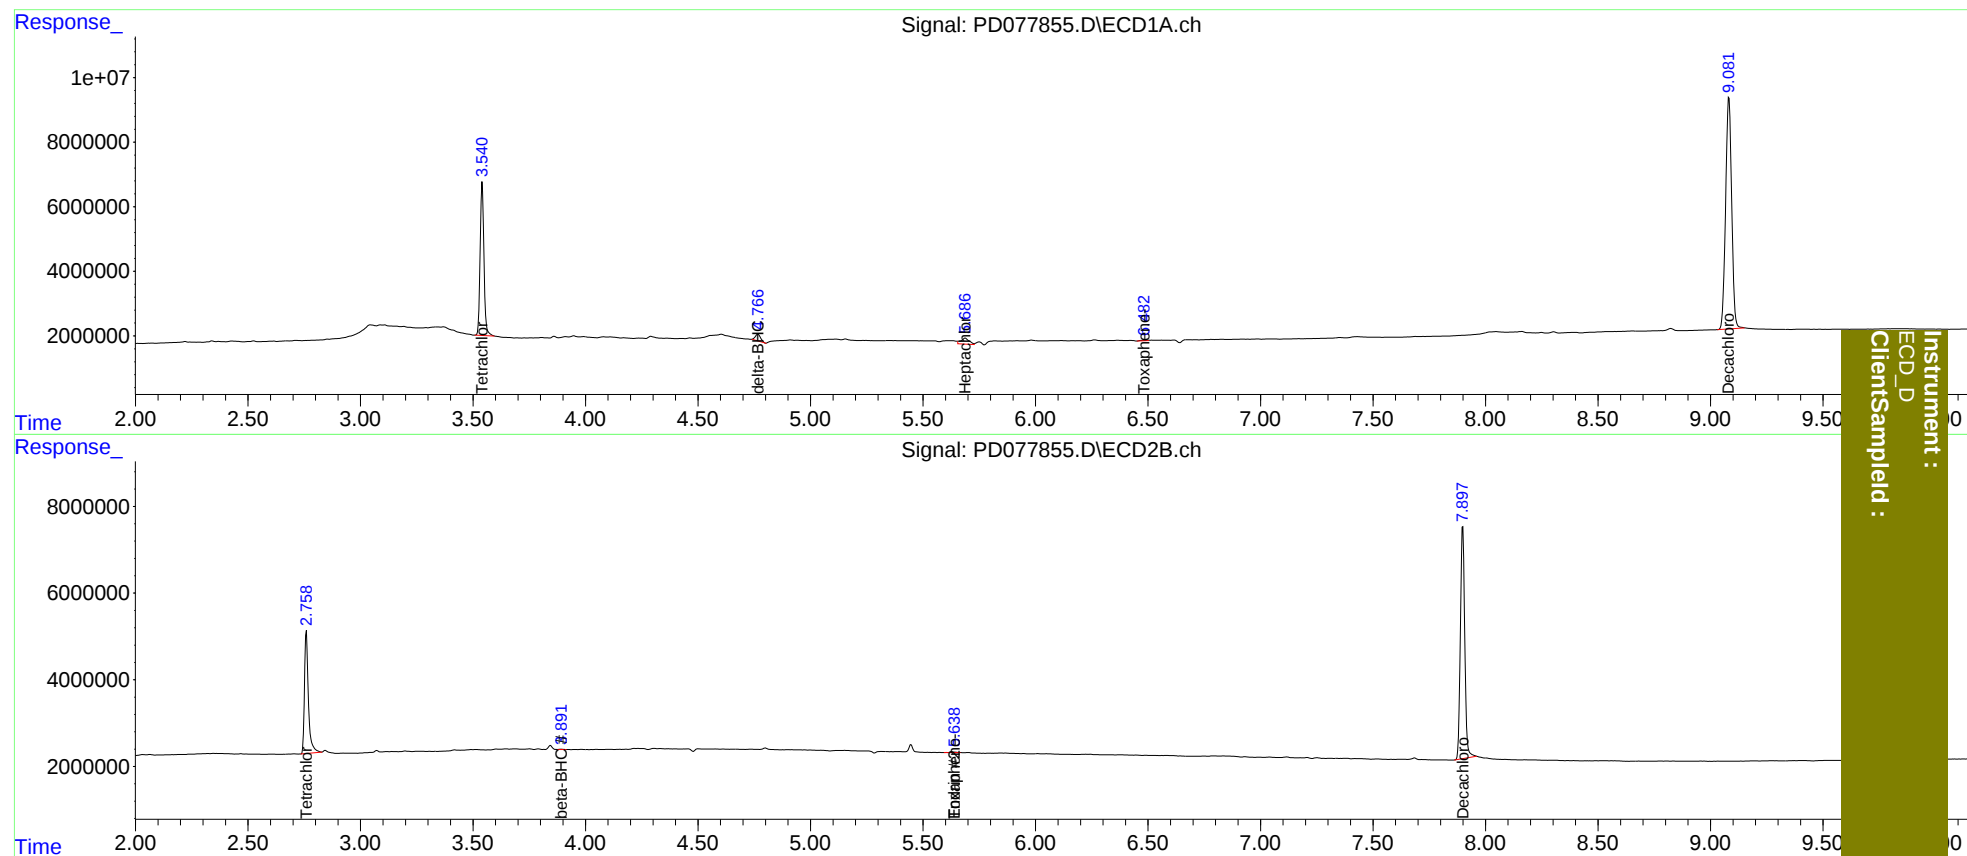


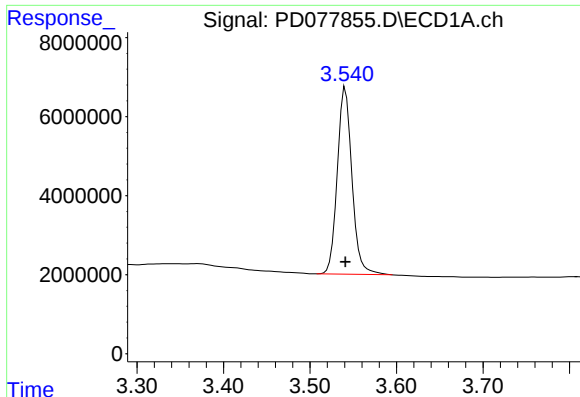

#1 Tetrachloro-m-xylene


R.T.: 3.541 min
Delta R.T.: 0.000 min
Response: 55375787
Conc: 21.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

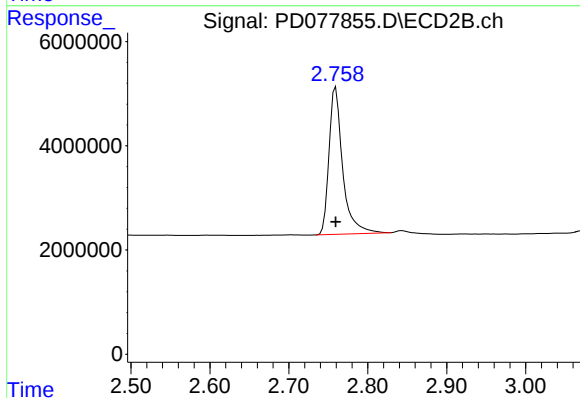


#1 Tetrachloro-m-xylene

R.T.: 2.760 min
Delta R.T.: 0.000 min
Response: 34121030
Conc: 21.56 ng/ml

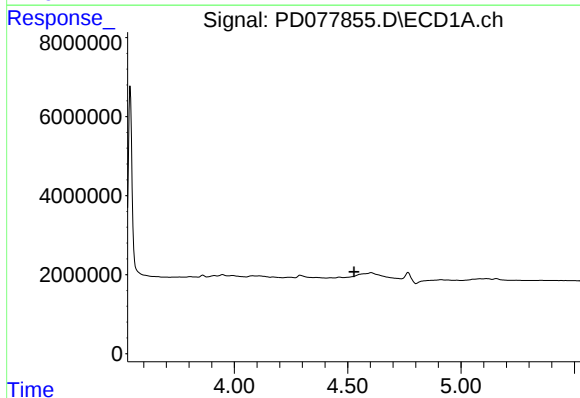


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.529 min
Response: 0
Conc: N.D.

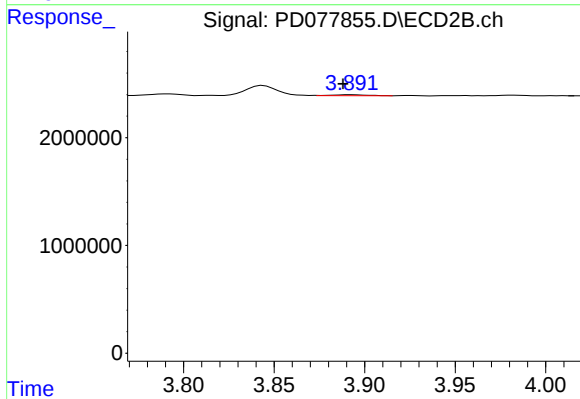

#6 beta-BHC


R.T.: 3.893 min
Delta R.T.: 0.005 min
Response: 119283
Conc: 0.11 ng/ml

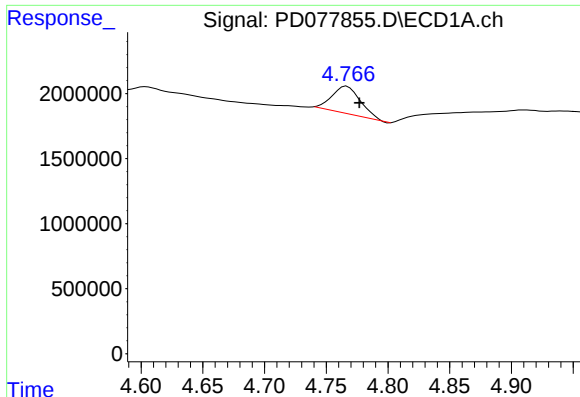

#7 delta-BHC


R.T.: 4.766 min
Delta R.T.: -0.010 min
Response: 3395347
Conc: 0.82 ng/ml

Instrument :
ECD_D
ClientSampleId :

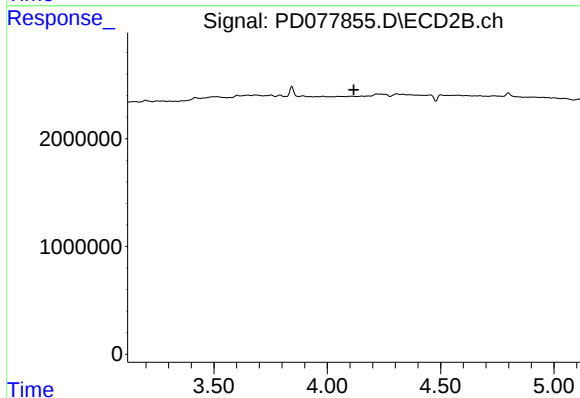


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.117 min
Response: 0
Conc: N.D.

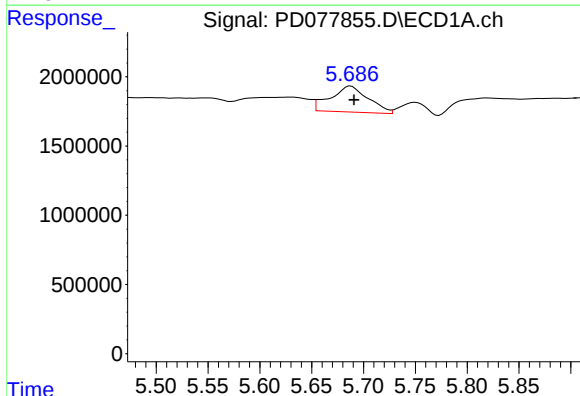


#8 Heptachlor epoxide

R.T.: 5.688 min
Delta R.T.: -0.003 min
Response: 4732202
Conc: 1.23 ng/ml

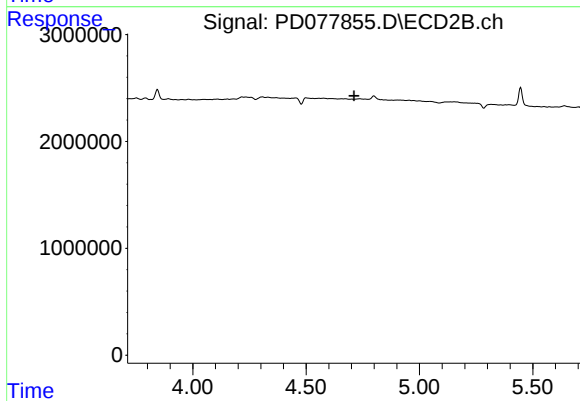

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.712 min
Response: 0
Conc: N.D.

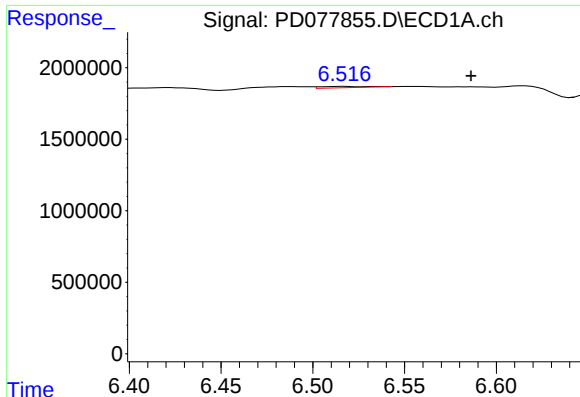

#14 Endrin


R.T.: 6.517 min
Delta R.T.: -0.069 min
Response: 148079
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

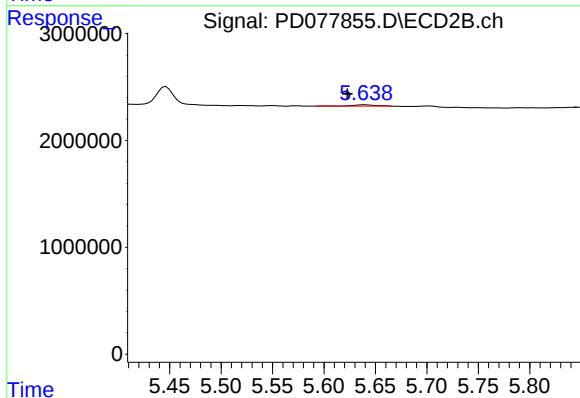


#14 Endrin

R.T.: 5.640 min
Delta R.T.: 0.017 min
Response: 207831
Conc: 0.11 ng/ml

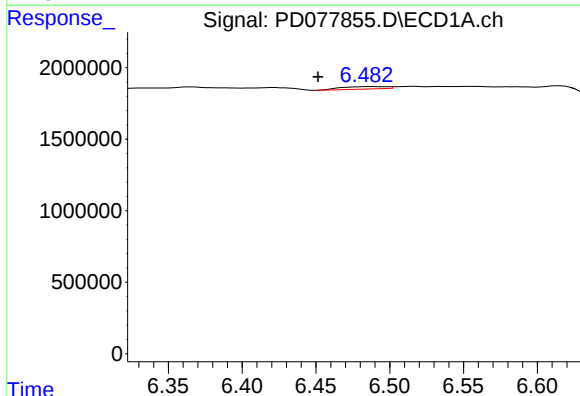


#23 Toxaphene-2

R.T.: 6.488 min
Delta R.T.: 0.036 min
Response: 356586
Conc: 10.69 ng/ml

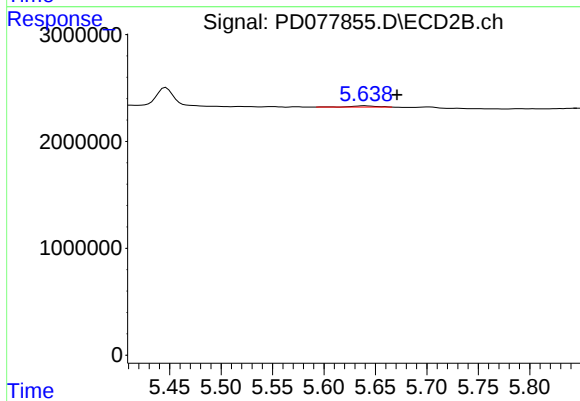

#23 Toxaphene-2

R.T.: 5.640 min
Delta R.T.: -0.031 min
Response: 207831
Conc: 16.00 ng/ml

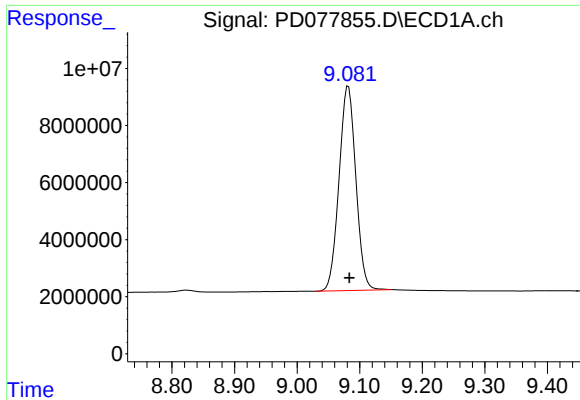

#27 Decachlorobiphenyl


R.T.: 9.082 min

Delta R.T.: -0.002 min

Response: 134210843

Conc: 43.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

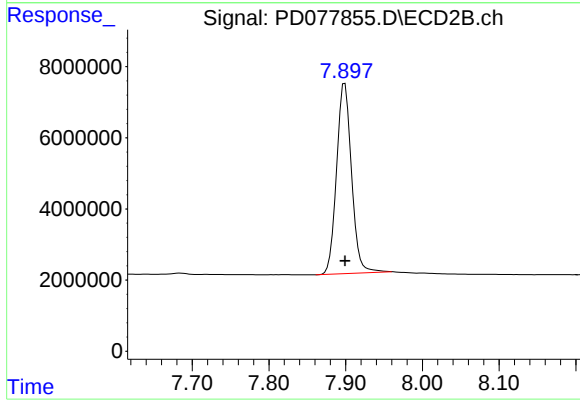

#27 Decachlorobiphenyl

R.T.: 7.899 min

Delta R.T.: 0.000 min

Response: 72605089

Conc: 42.09 ng/ml