

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091124\
 Data File : PD085000.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2024 15:16
 Operator : AR\AJ
 Sample : P3878-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDC45

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 02:14:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
27)	SA Decachlor...	9.035	8.106	20219200	53141981	15.481	15.283
Target Compounds							
2)	A alpha-BHC	4.024f	0.000	1640929	0	0.965	N.D. #
4)	MA Heptachlor	0.000	4.091	0	126.4E6	N.D.	29.698
6)	B beta-BHC	0.000	4.091f	0	126.4E6	N.D.	58.317
7)	B delta-BHC	4.764	0.000	47629739	0	29.042	N.D. #
15)	B Endosulfa...	6.819f	0.000	1129349	0	0.856	N.D. #
21)	B Endrin ke...	0.000	7.060f	0	9883395	N.D.	2.245


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091124\
Data File : PD085000.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2024 15:16
Operator : AR\AJ
Sample : P3878-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 02:14:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

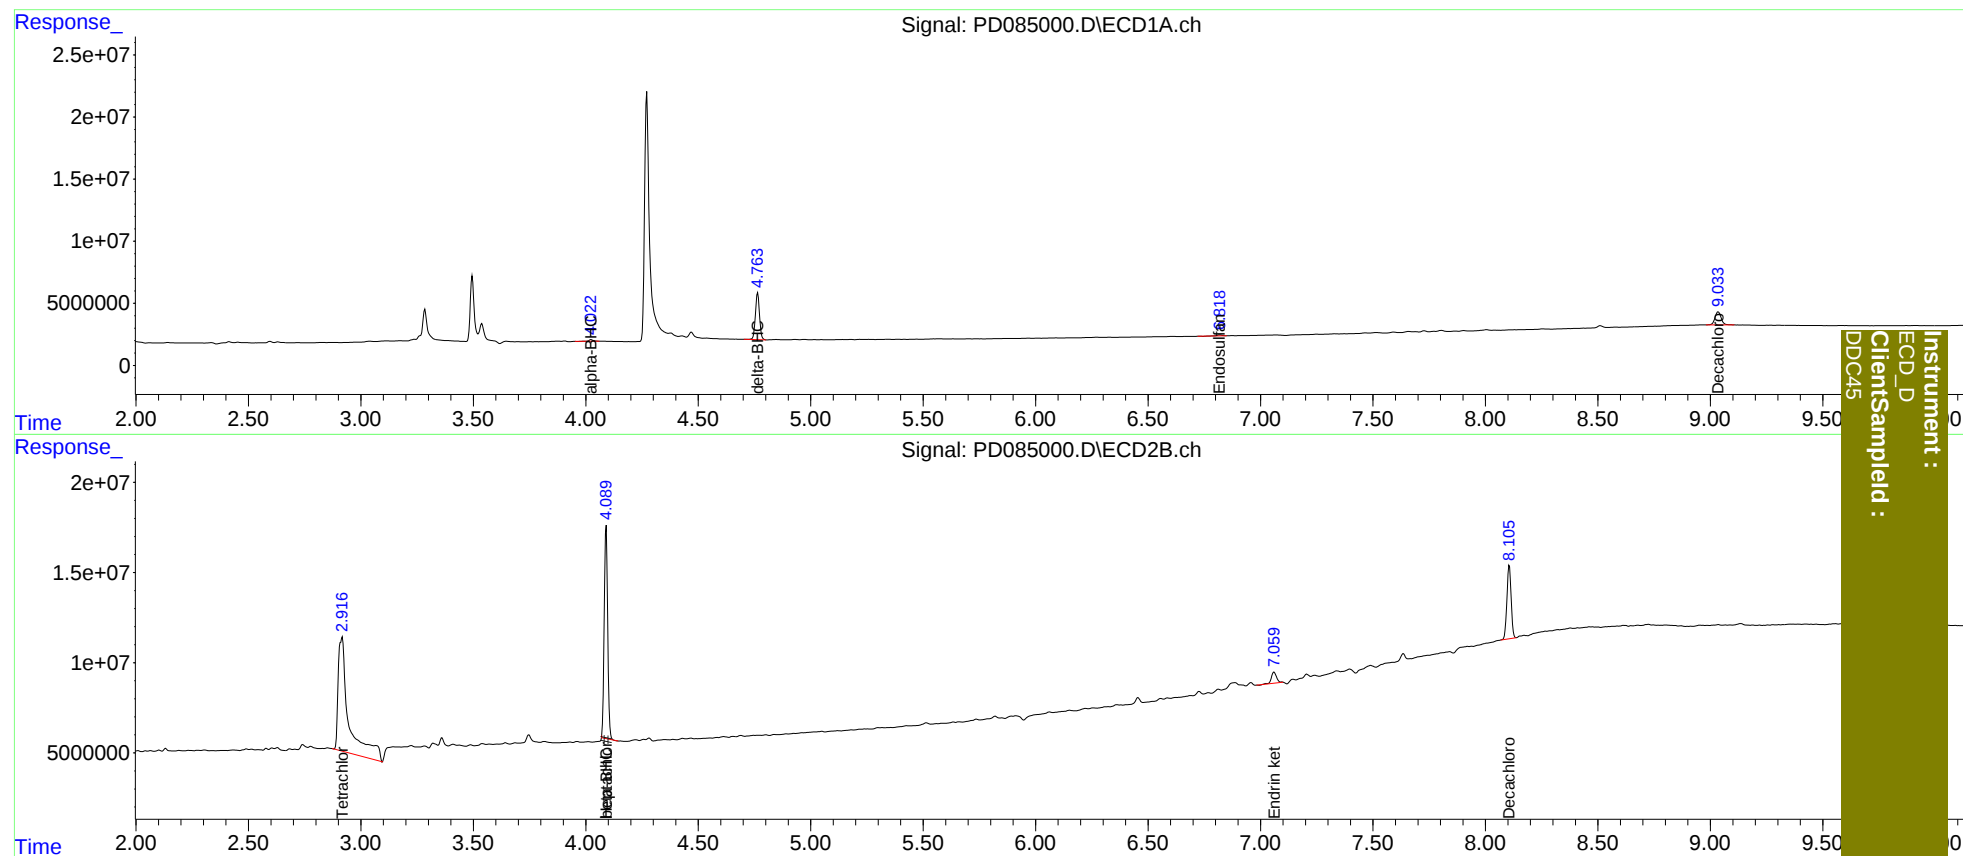


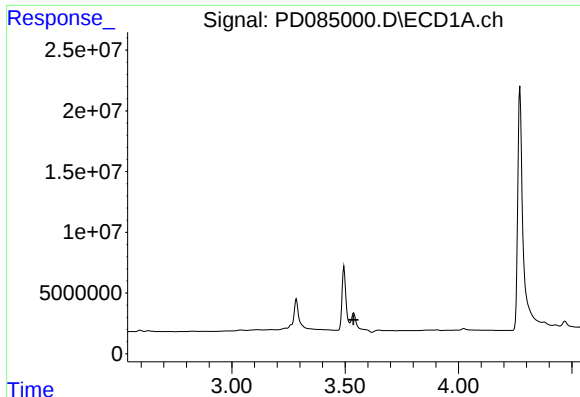

#1 Tetrachloro-m-xylene


R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: -71538270
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DDC45

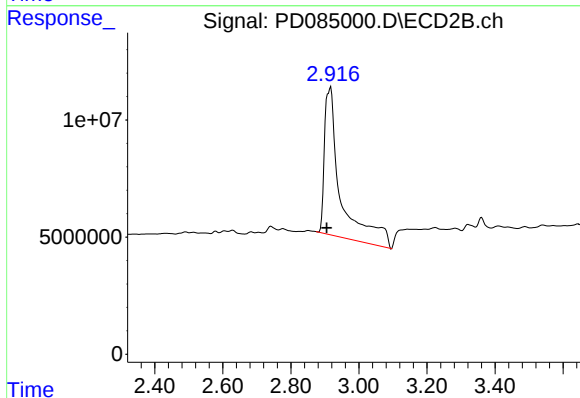


#1 Tetrachloro-m-xylene

R.T.: 2.917 min
Delta R.T.: 0.011 min
Response: 208243504
Conc: 58.85 ng/ml

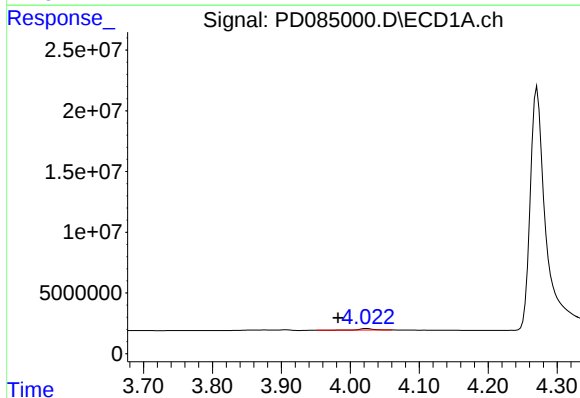


#2 alpha-BHC

R.T.: 4.024 min
Delta R.T.: 0.041 min
Response: 1640929
Conc: 0.97 ng/ml

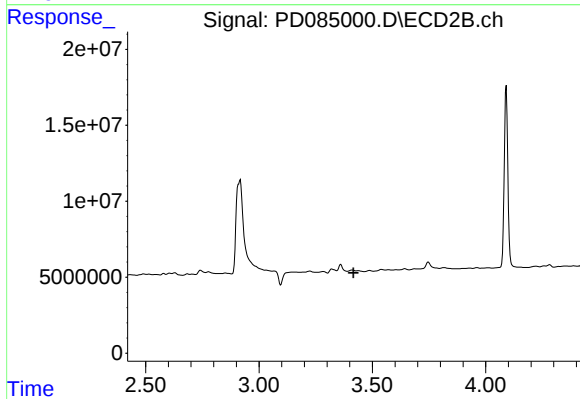

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 3.417 min
Response: 0
Conc: N.D.

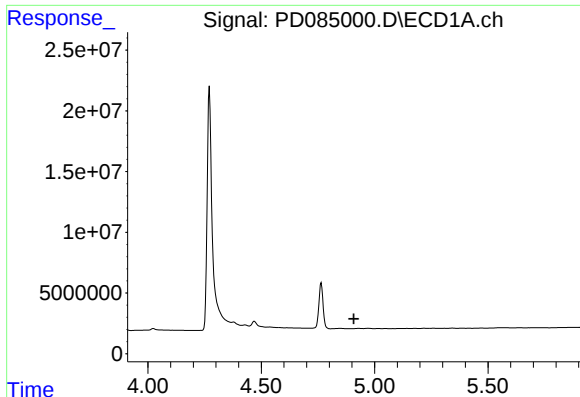

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DDC45

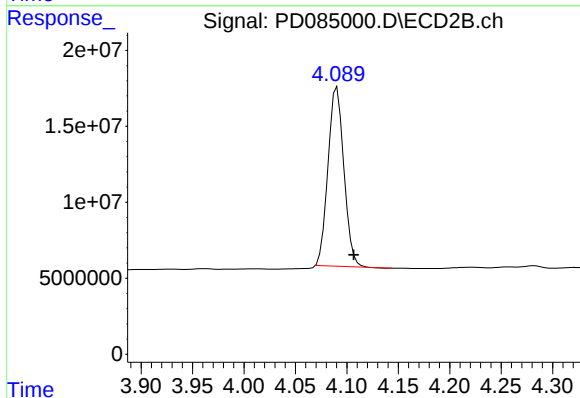


#4 Heptachlor

R.T.: 4.091 min
Delta R.T.: -0.016 min
Response: 126427717
Conc: 29.70 ng/ml

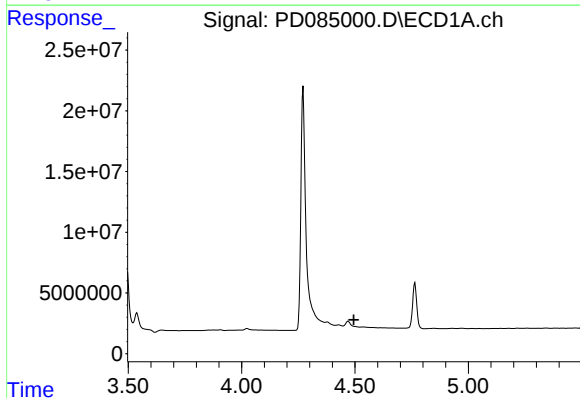


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.495 min
Response: 0
Conc: N.D.

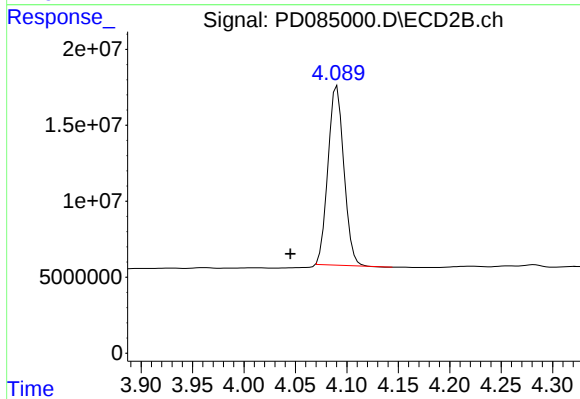

#6 beta-BHC


R.T.: 4.091 min
Delta R.T.: 0.045 min
Response: 126427717
Conc: 58.32 ng/ml

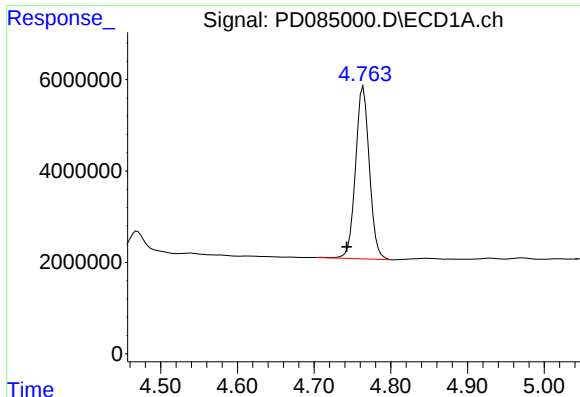

#7 delta-BHC


R.T.: 4.764 min
Delta R.T.: 0.022 min
Response: 47629739
Conc: 29.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
DDC45

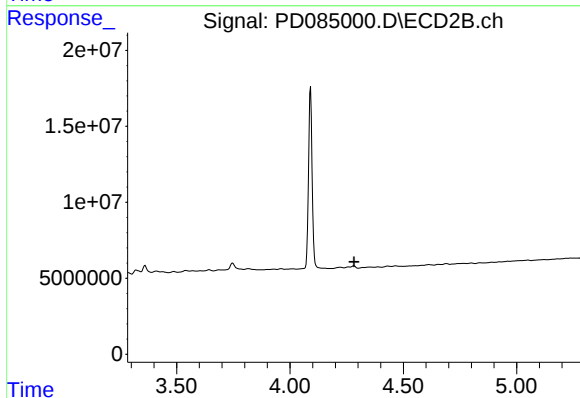


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.283 min
Response: 0
Conc: N.D.

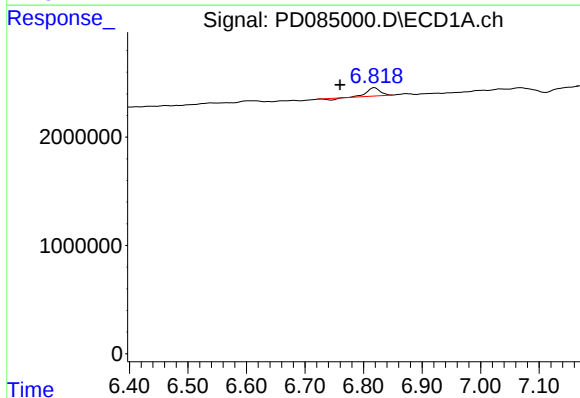


#15 Endosulfan II

R.T.: 6.819 min
Delta R.T.: 0.059 min
Response: 1129349
Conc: 0.86 ng/ml

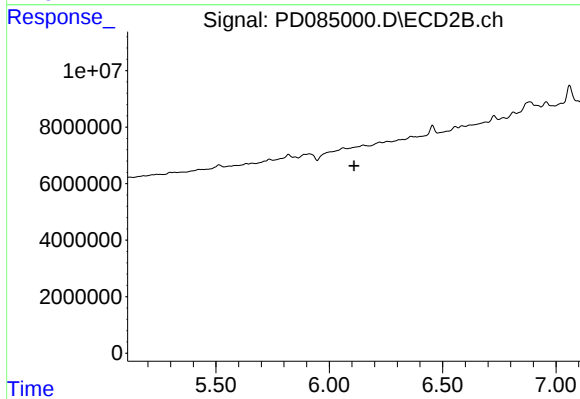

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.110 min
Response: 0
Conc: N.D.

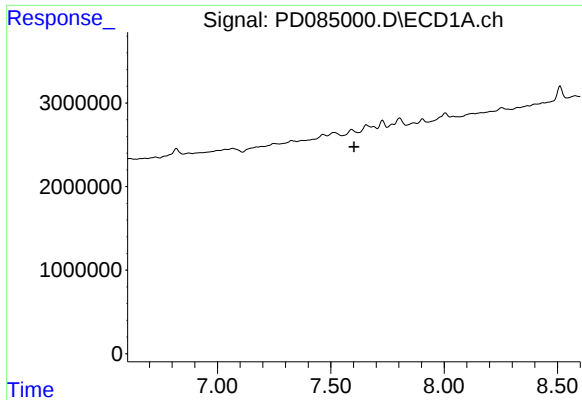

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.603 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DDC45

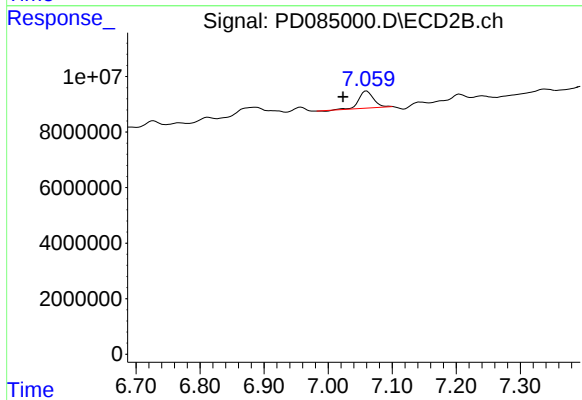


#21 Endrin ketone

R.T.: 7.060 min
Delta R.T.: 0.037 min
Response: 9883395
Conc: 2.24 ng/ml

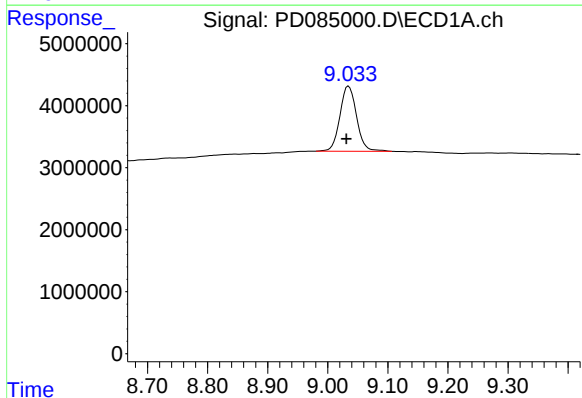

#27 Decachlorobiphenyl

R.T.: 9.035 min
Delta R.T.: 0.003 min
Response: 20219200
Conc: 15.48 ng/ml

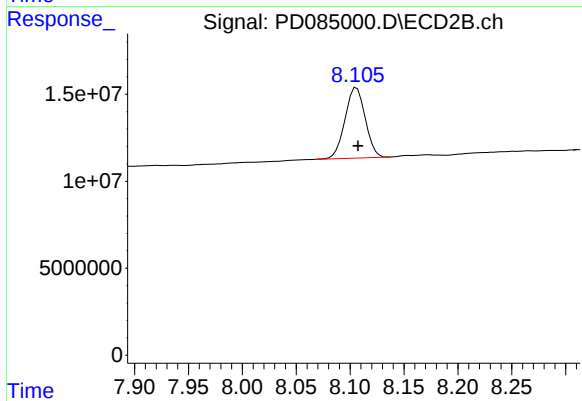

#27 Decachlorobiphenyl

R.T.: 8.106 min
Delta R.T.: -0.001 min
Response: 53141981
Conc: 15.28 ng/ml