

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091124\
 Data File : PD085005.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2024 16:23
 Operator : AR\AJ
 Sample : PIBLK111
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK269

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 02:15:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.539	2.906	11909221	93218318	11.775	26.342 #
27) SA Decachlor...	9.036	8.107	35386060	77929321	27.094	22.412
Target Compounds						
2) A alpha-BHC	3.944f	0.000	383181	0	0.225	N.D. #
14) MA Endrin	6.605f	0.000	3534092	0	3.132	N.D. #
20) A Methoxychlor	7.479	0.000	9435827	0	18.114	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091124\
Data File : PD085005.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2024 16:23
Operator : AR\AJ
Sample : PIBLK111
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 02:15:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

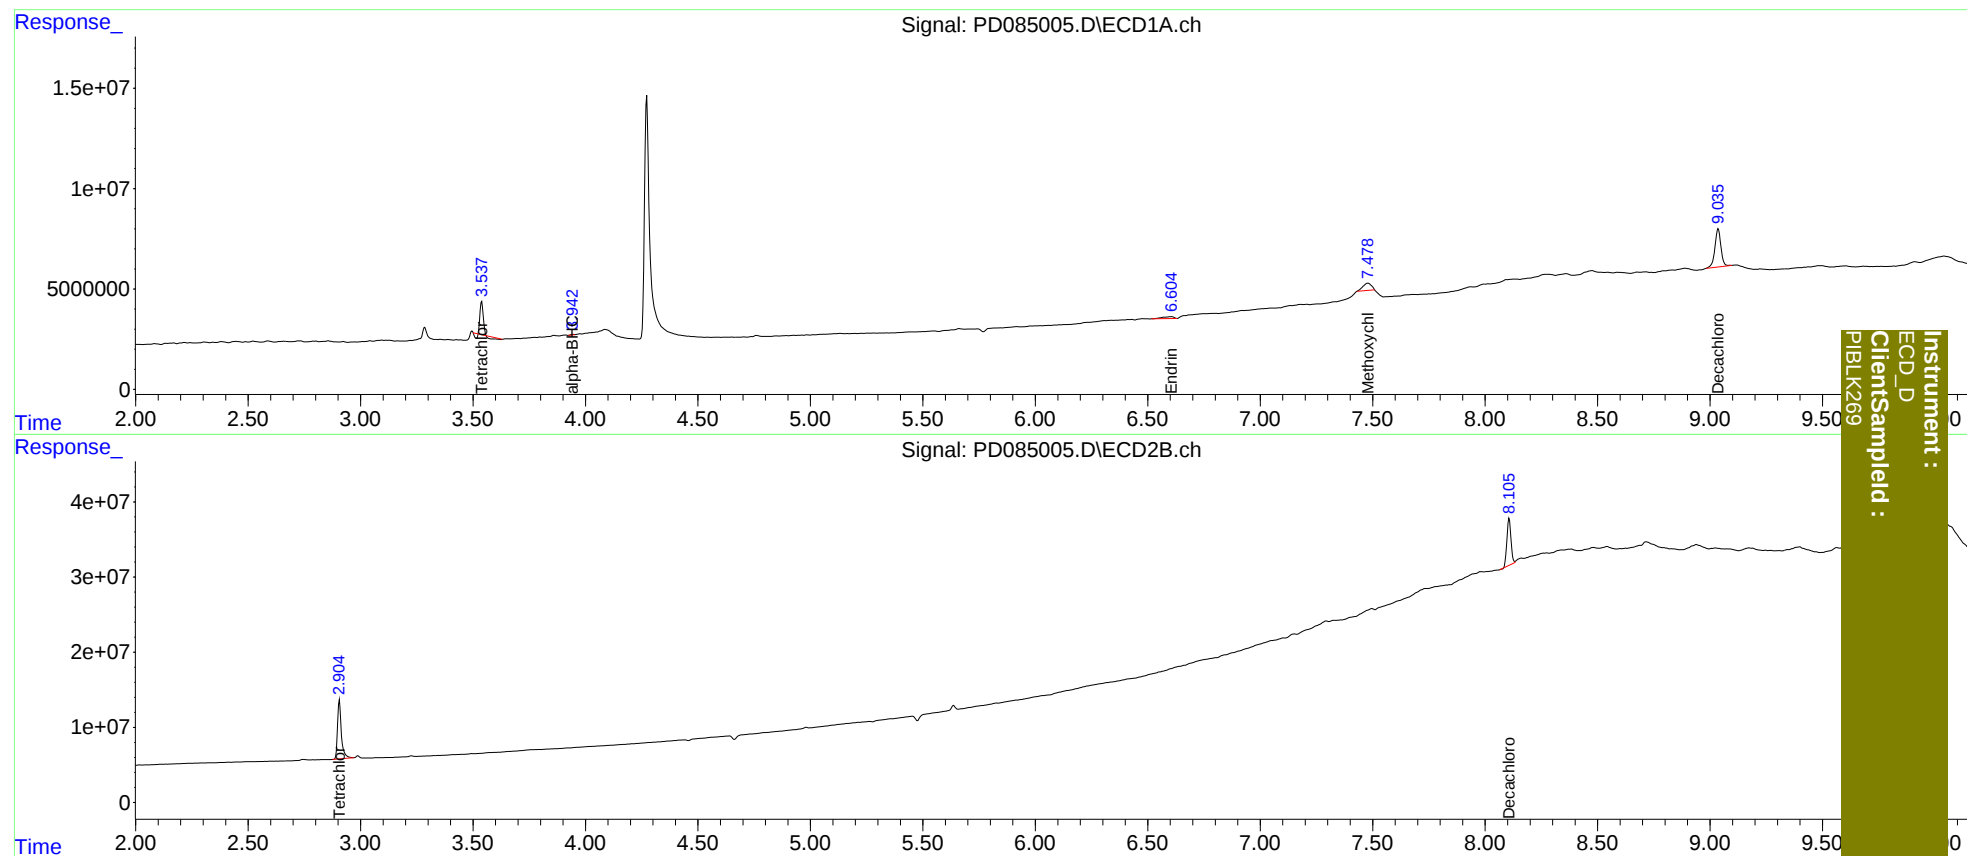


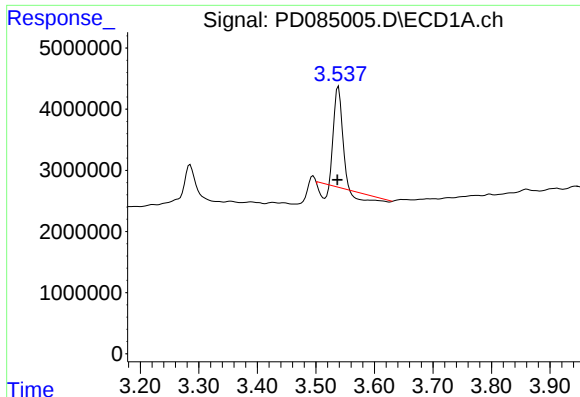

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: 0.002 min
Response: 11909221
Conc: 11.77 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK269

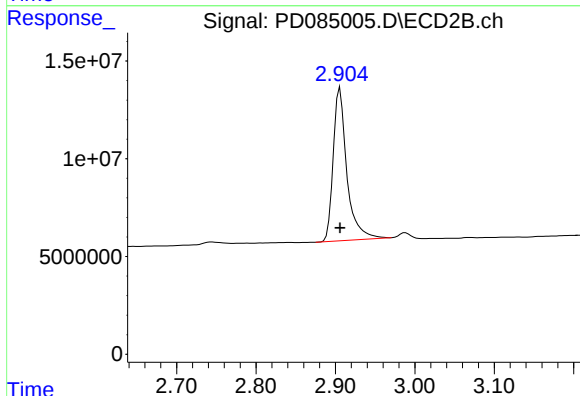


#1 Tetrachloro-m-xylene

R.T.: 2.906 min
Delta R.T.: 0.000 min
Response: 93218318
Conc: 26.34 ng/ml

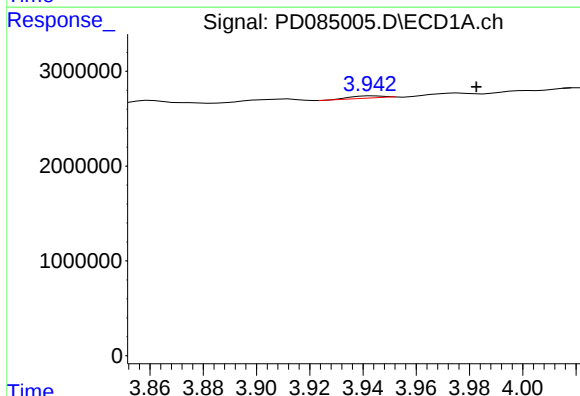


#2 alpha-BHC

R.T.: 3.944 min
Delta R.T.: -0.038 min
Response: 383181
Conc: 0.23 ng/ml

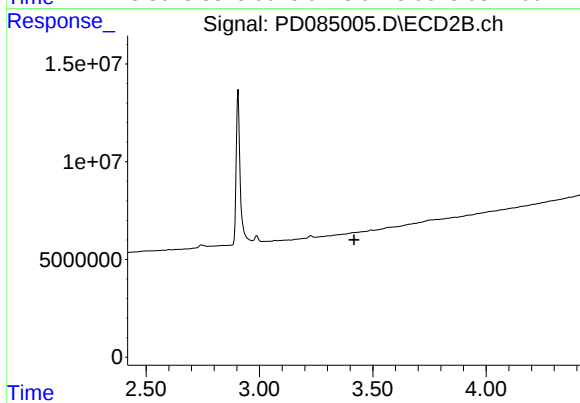

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 3.417 min
Response: 0
Conc: N.D.

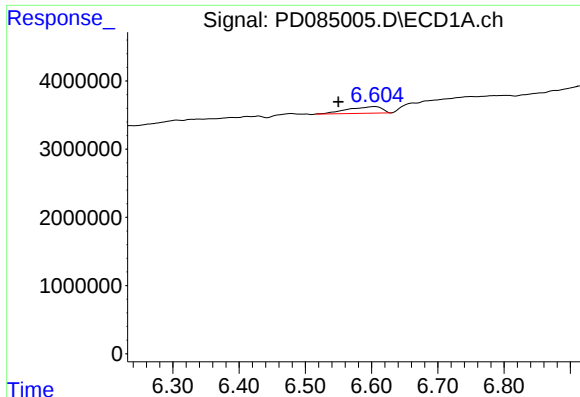

#14 Endrin


R.T.: 6.605 min
Delta R.T.: 0.055 min
Response: 3534092
Conc: 3.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK269

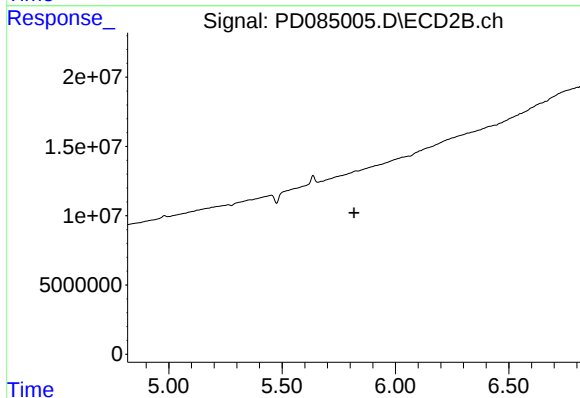


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.817 min
Response: 0
Conc: N.D.

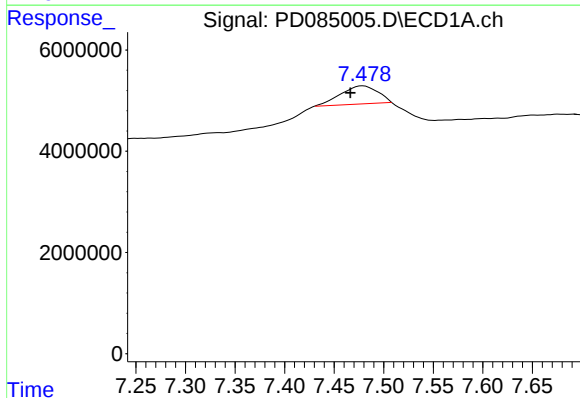


#20 Methoxychlor

R.T.: 7.479 min
Delta R.T.: 0.013 min
Response: 9435827
Conc: 18.11 ng/ml

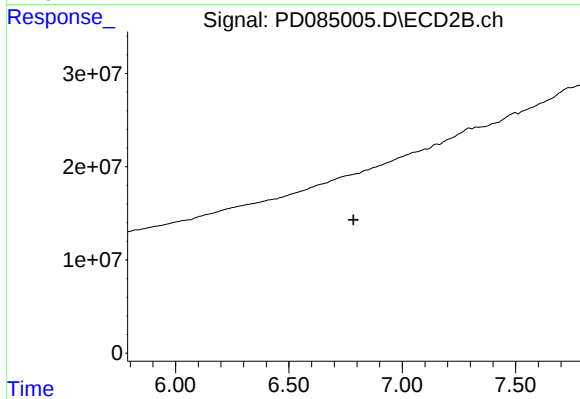

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.785 min
Response: 0
Conc: N.D.

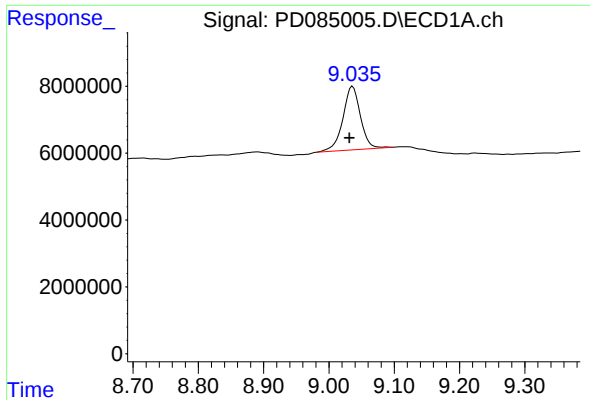

#27 Decachlorobiphenyl

R.T.: 9.036 min
Delta R.T.: 0.005 min
Response: 35386060
Conc: 27.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK269

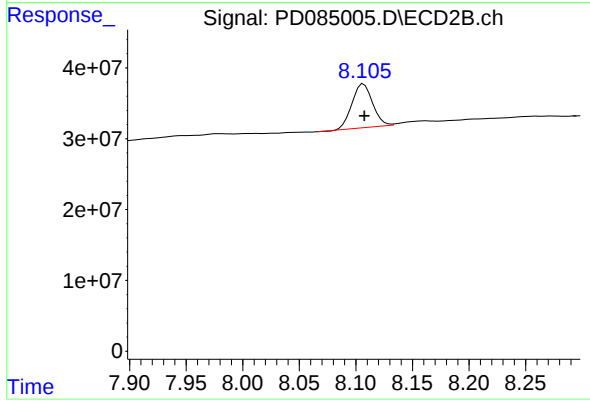

#27 Decachlorobiphenyl

R.T.: 8.107 min
Delta R.T.: 0.000 min
Response: 77929321
Conc: 22.41 ng/ml