

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091124\
 Data File : PD085017.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2024 20:14
 Operator : AR\AJ
 Sample : PIBLK112
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK270

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 02:18:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.905	19325547	90267168	19.108	25.508 #
27)	SA Decachlor...	9.034	8.106	33128286	76651130	25.366	22.044
Target Compounds							
20)	A Methoxychlor	7.485	0.000	2690565	0	5.165	N.D. #
21)	B Endrin ke...	0.000	7.090f	0	11425016	N.D.	2.595


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091124\
Data File : PD085017.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2024 20:14
Operator : AR\AJ
Sample : PIBLK112
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 02:18:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

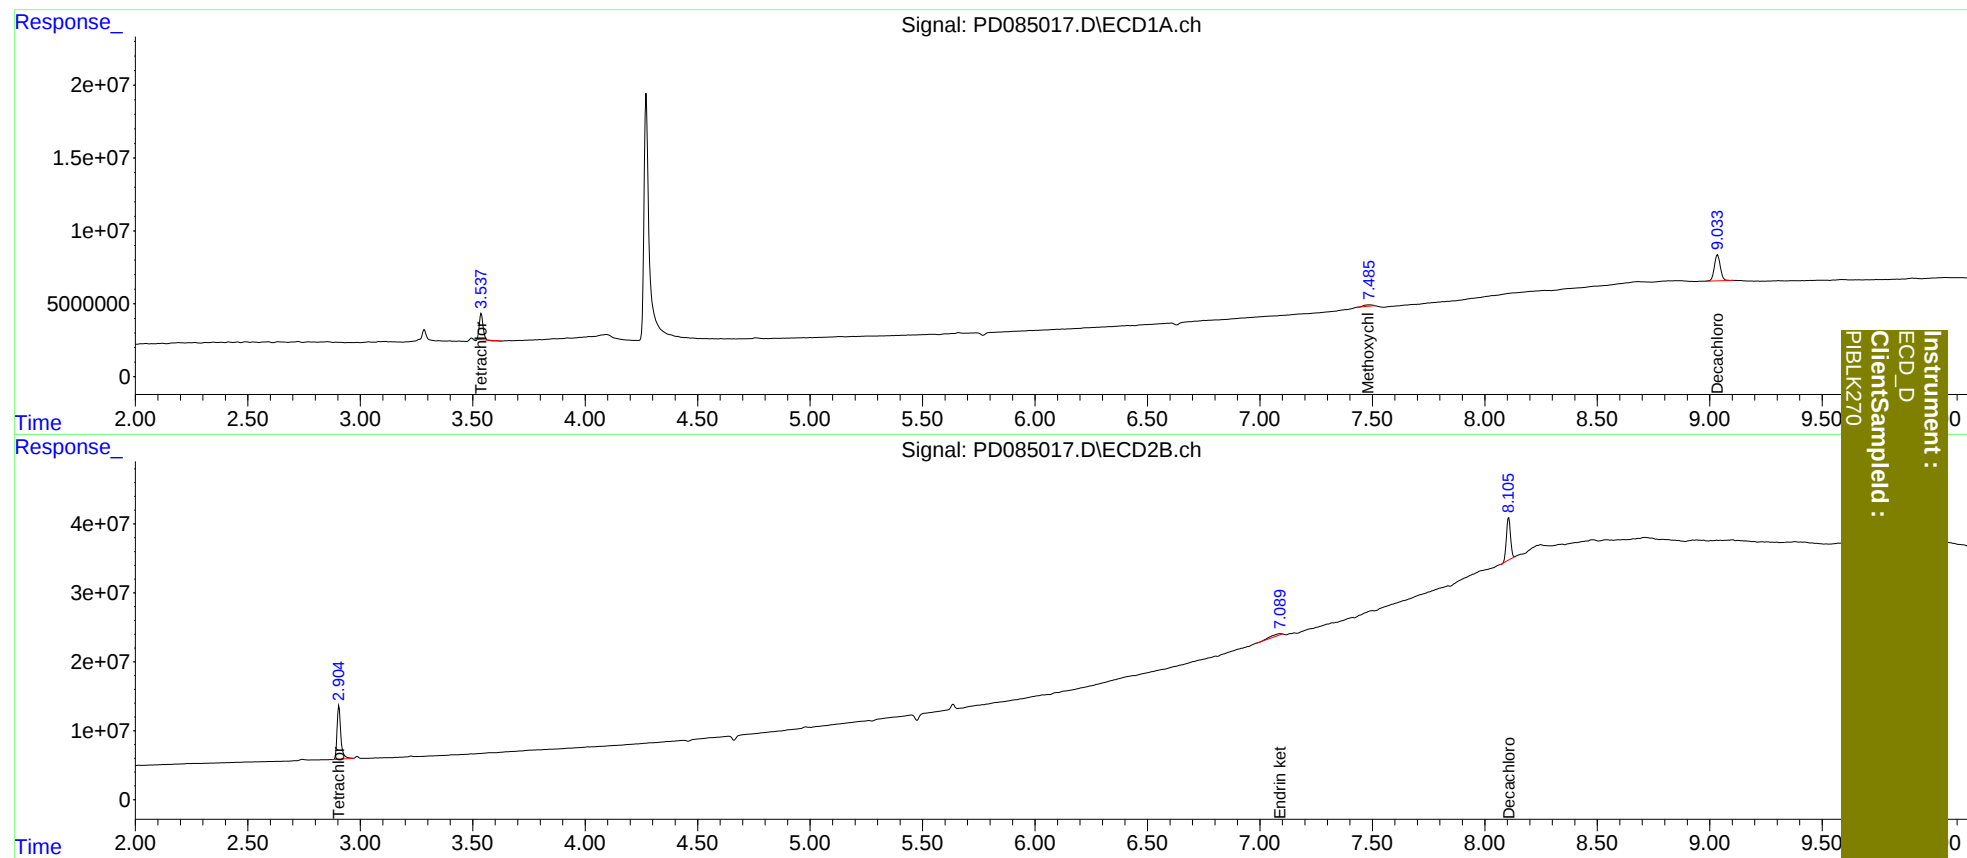


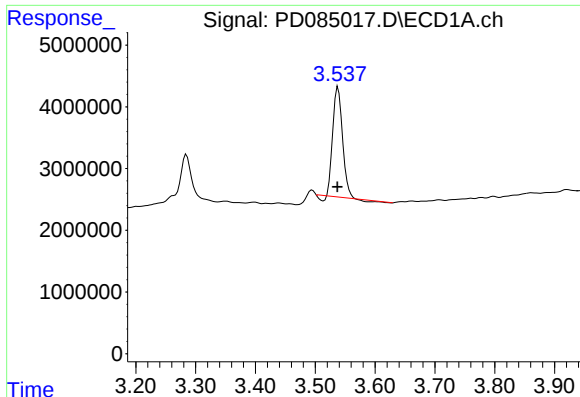

#1 Tetrachloro-m-xylene


R.T.: 3.538 min
Delta R.T.: 0.001 min
Response: 19325547
Conc: 19.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK270

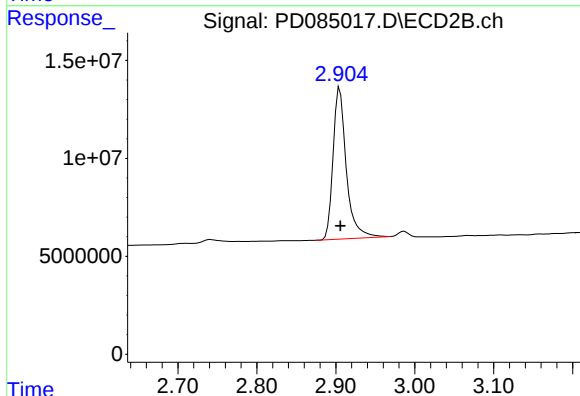


#1 Tetrachloro-m-xylene

R.T.: 2.905 min
Delta R.T.: 0.000 min
Response: 90267168
Conc: 25.51 ng/ml

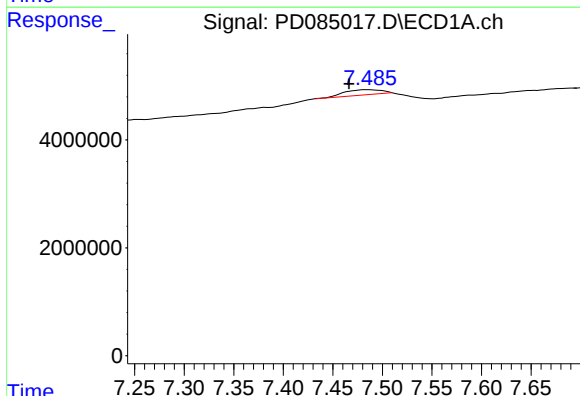


#20 Methoxychlor

R.T.: 7.485 min
Delta R.T.: 0.018 min
Response: 2690565
Conc: 5.17 ng/ml

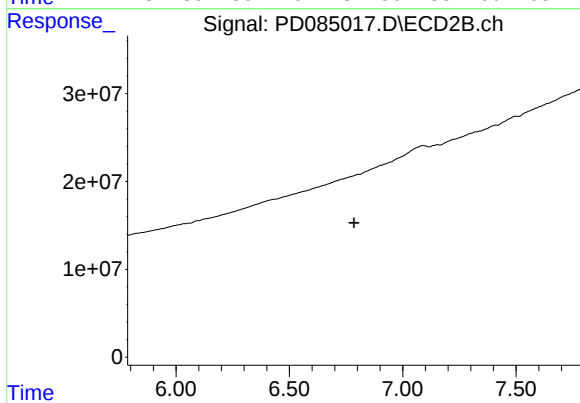

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.785 min
Response: 0
Conc: N.D.

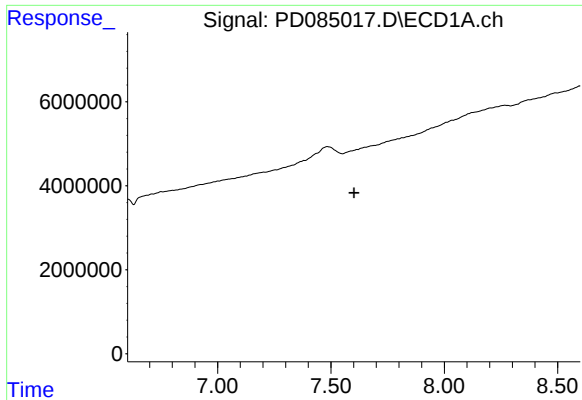

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.603 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK270

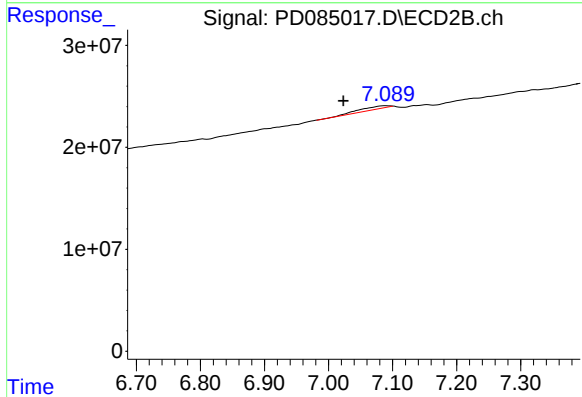


#21 Endrin ketone

R.T.: 7.090 min
Delta R.T.: 0.067 min
Response: 11425016
Conc: 2.59 ng/ml

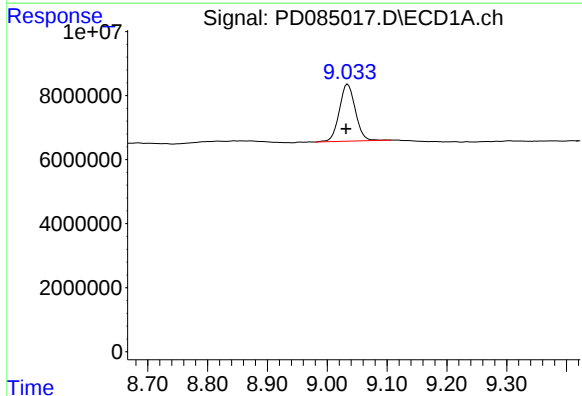

#27 Decachlorobiphenyl

R.T.: 9.034 min
Delta R.T.: 0.003 min
Response: 33128286
Conc: 25.37 ng/ml

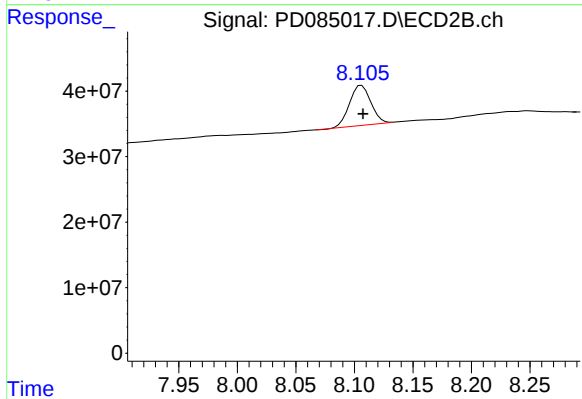

#27 Decachlorobiphenyl

R.T.: 8.106 min
Delta R.T.: -0.001 min
Response: 76651130
Conc: 22.04 ng/ml