

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091124\
 Data File : PD085024.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2024 22:14
 Operator : AR\AJ
 Sample : P3878-21MS
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :

ECD_D

ClientSampleId :

DDCC3MS

Manual Integrations**APPROVED**

Reviewed By :Abdul Mirza 09/12/2024

Supervised By :Ankita Jodhani 09/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 02:20:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.527	2.918	39200165	2676.9E6	38.758m	756.428m#
2)	SA Decachlor...	9.036	8.107	11352052	25475060	8.692	7.326
Target Compounds							
2)	A alpha-BHC	3.984	3.416	181.9E6	425.2E6	106.991	83.852
3)	MA gamma-BHC...	4.260f	3.751	47726.0E6	419.7E6	29499.529m	86.608 #
4)	MA Heptachlor	4.911	4.100	79260869	207.7E6	51.515	48.795m
5)	MB Aldrin	5.252	4.390	83808956	155.2E6	52.402	34.945 #
6)	B beta-BHC	4.494	4.044	44769863	98808115	61.635m	45.577 #
7)	B delta-BHC	4.742	4.281	237.9E6	528.0E6	145.054m	106.373m#
8)	B Heptachlo...	5.671	4.896	77550731	220.8E6	51.996	52.127
9)	A Endosulfan I	6.052	5.272	77539659	193.1E6	56.360m	50.364m
10)	B trans-Chl...	5.924	5.149	80124886	219.7E6	56.811	53.424m
11)	B cis-Chlor...	6.005	5.214	80104767	205.5E6	54.178m	48.991m
12)	B 4,4'-DDE	6.175	5.401	143.7E6	398.9E6	115.157	101.686
13)	MA Dieldrin	6.326	5.540	157.1E6	417.8E6	106.525	97.261
14)	MA Endrin	6.551	5.816	146.2E6	417.0E6	129.609m	112.629m
15)	B Endosulfa...	6.761	6.109	123.2E6	331.7E6	93.295m	89.462
16)	A 4,4'-DDD	6.681	5.958	111.5E6	394.5E6	112.899m	116.261
17)	MA 4,4'-DDT	6.997	6.211	106.7E6	351.4E6	119.165m	109.862m
18)	B Endrin al...	6.891	6.288	124.1E6	265.8E6	137.373m	93.078 #
19)	B Endosulfa...	7.125	6.513	145.2E6	330.1E6	126.070	92.418 #
20)	A Methoxychlor	7.469	6.785	511.3E6	820.9E6	981.478m	496.250 #
21)	B Endrin ke...	7.605	7.024	140.4E6	397.2E6	114.796	90.197

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091124\
Data File : PD085024.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2024 22:14
Operator : AR\AJ
Sample : P3878-21MS
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 02:20:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

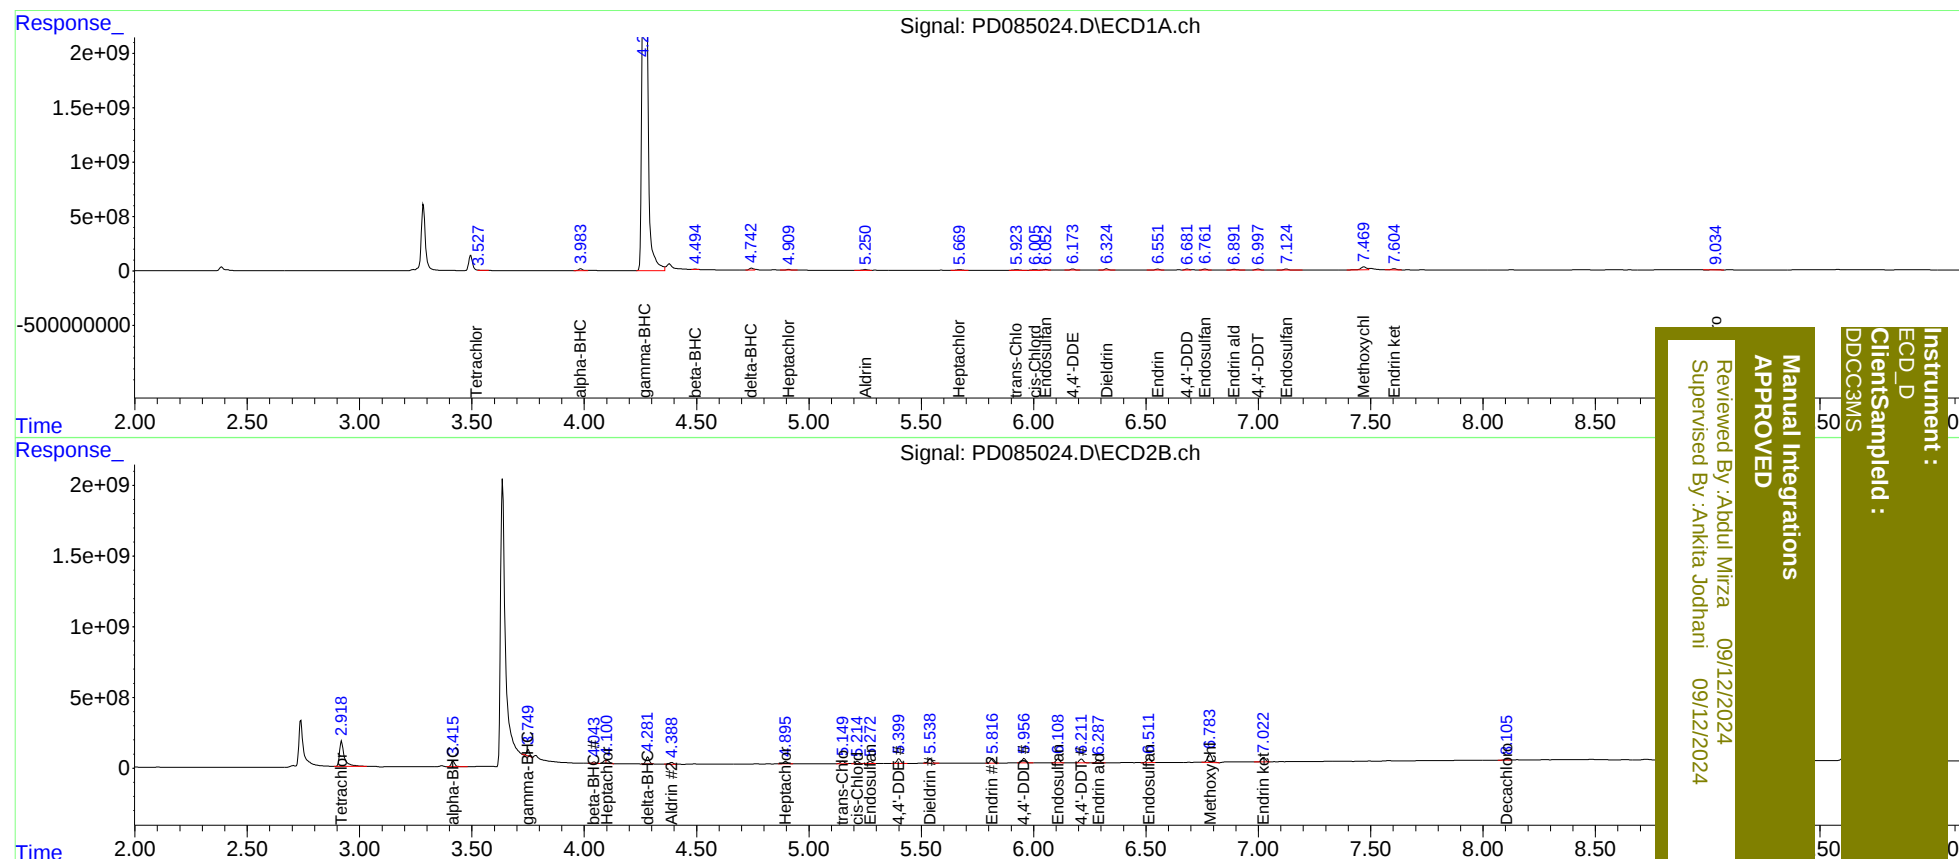

Reviewed By: Abdul Mirza 09/12/2024
Supervised By: Ankita Jodhani 09/12/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
DDCCMS