

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091125\
 Data File : PD090255.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2025 18:25
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 06:26:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX081825.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 19 05:29:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.877	128.2E6	1134.5E6	42.995	50.818
7)	SA Decachlor...	9.069	8.065	201.1E6	1363.8E6	46.425	51.387
Target Compounds							
2)	Toxaphene-1	6.240	5.470	18586467	115.0E6	429.226	502.210
3)	Toxaphene-2	6.440	5.641	24502938	78745971	440.983	513.248
4)	Toxaphene-3	7.146	6.750	45850805	386.7E6	434.864	532.911
5)	Toxaphene-4	7.561	7.192	60717934	259.2E6	450.326	522.569
6)	Toxaphene-5	7.926	7.323	34664258	194.2E6	450.764	541.119

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091125\
Data File : PD090255.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2025 18:25
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 06:26:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX081825.M
Quant Title : GC Extractables
QLast Update : Tue Aug 19 05:29:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x0.25µm

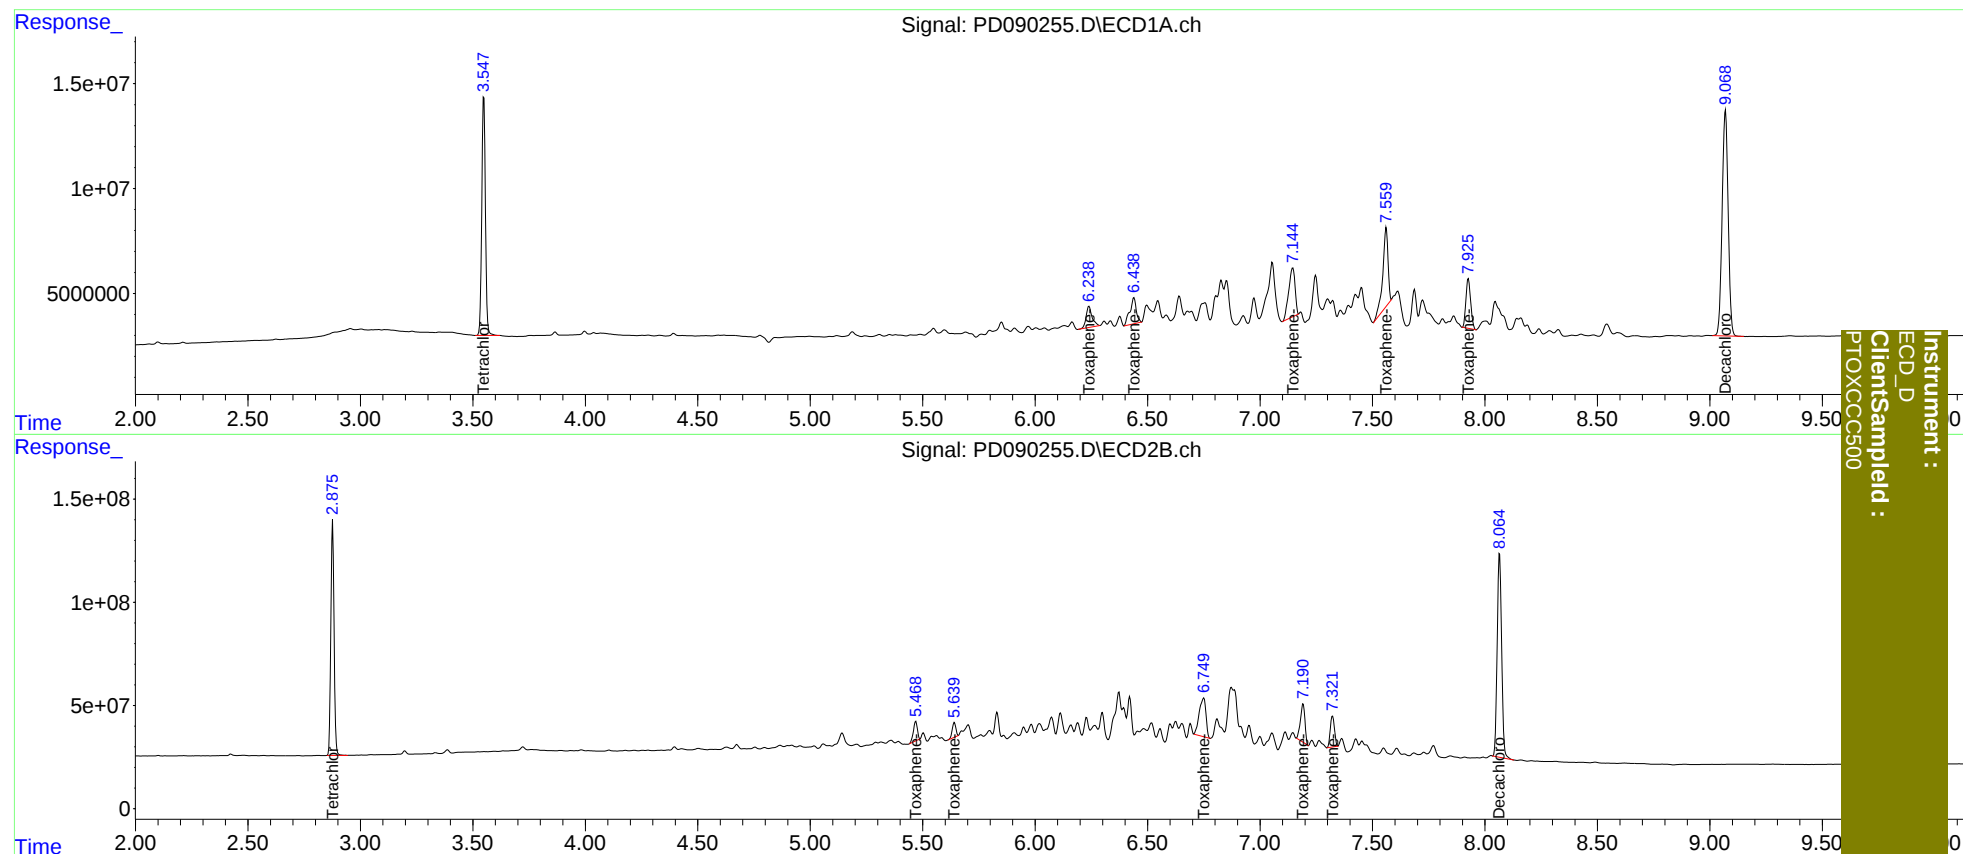

Instrument :
ECD_D
ClientSampled :
PTOXCCC500