

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091219\
 Data File : PD054498.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Sep 2019 13:09
 Operator : SG\AJ
 Sample : K4718-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AC4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 01:26:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090419CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 05 08:40:10 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.302	3.973	14196812	20302631	20.087	20.571
2)	SA Decachlor...	7.992	9.011	27168921	37211916	40.146	39.777
Target Compounds							
15)	B Endosulfa...	0.000	6.882	0	6485476	N.D.	5.204

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091219\
Data File : PD054498.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Sep 2019 13:09
Operator : SG\AJ
Sample : K4718-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 01:26:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090419CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 05 08:40:10 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

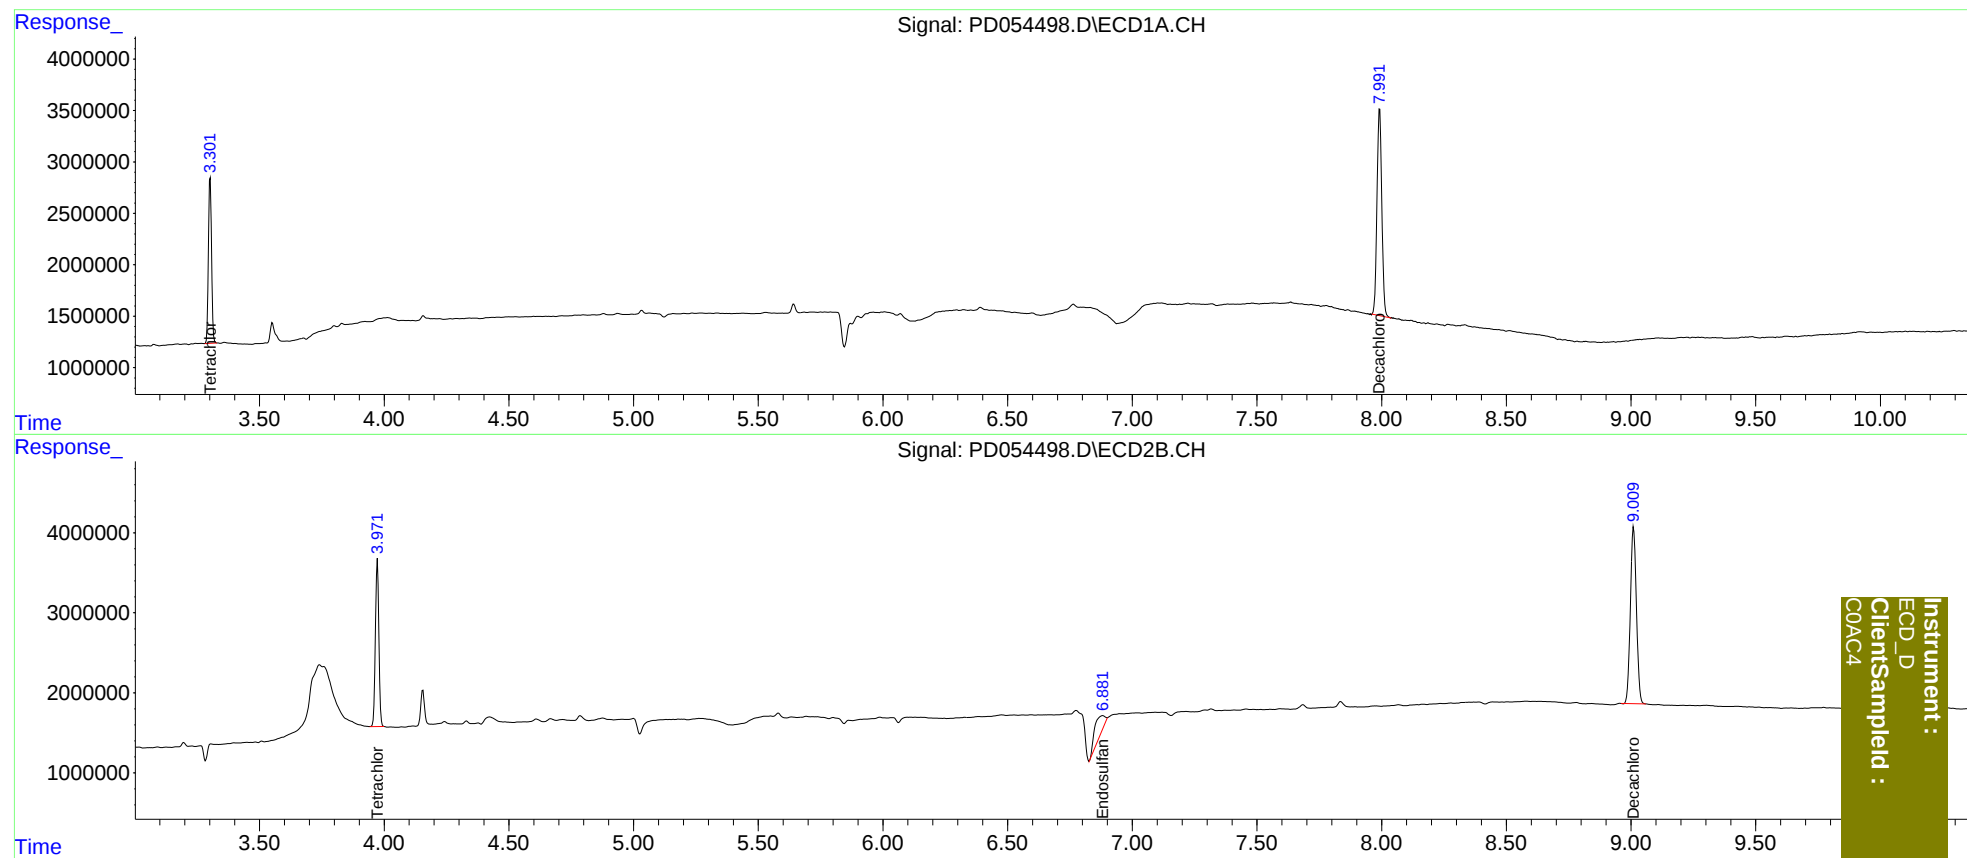


Instrument :
ECD_D
ClientSampleId :
C0AC4

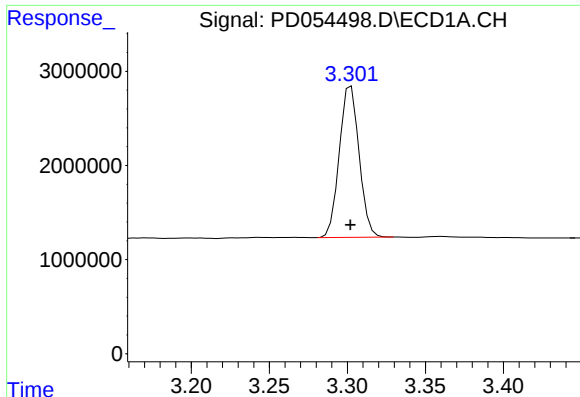

#1 Tetrachloro-m-xylene


R.T.: 3.302 min
Delta R.T.: 0.000 min
Response: 14196812
Conc: 20.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AC4

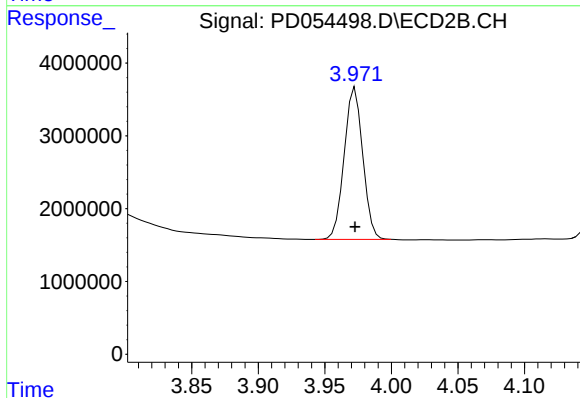


#1 Tetrachloro-m-xylene

R.T.: 3.973 min
Delta R.T.: 0.000 min
Response: 20302631
Conc: 20.57 ng/ml

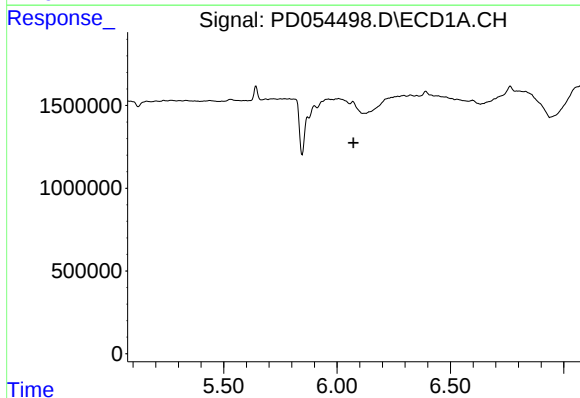


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.073 min
Response: 0
Conc: N.D.

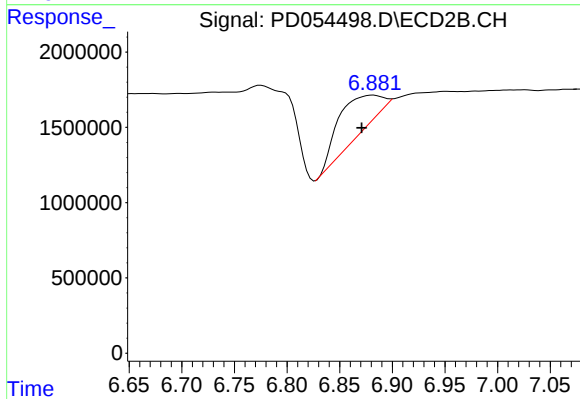

#15 Endosulfan II


R.T.: 6.882 min
Delta R.T.: 0.011 min
Response: 6485476
Conc: 5.20 ng/ml

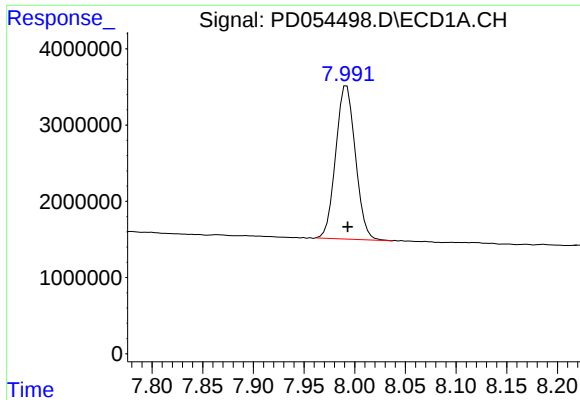

#27 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: 0.000 min
Response: 27168921
Conc: 40.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AC4

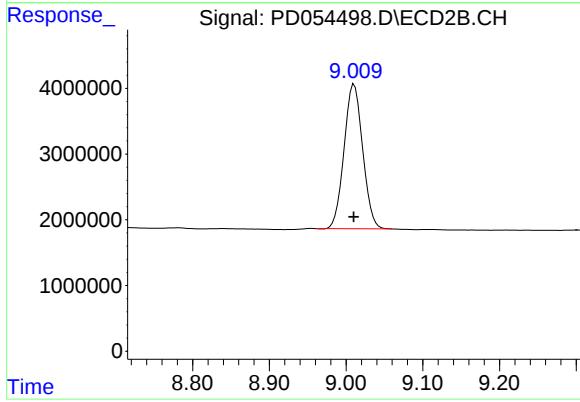

#27 Decachlorobiphenyl

R.T.: 9.011 min
Delta R.T.: 0.000 min
Response: 37211916
Conc: 39.78 ng/ml