

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091219\
 Data File : PD054499.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Sep 2019 13:23
 Operator : SG\AJ
 Sample : K4718-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AC6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 01:26:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090419CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 05 08:40:10 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.302	3.973	11210363	15584117	15.861	15.790
2) SA Decachlor...	7.992	9.009	18371782	22243270	27.147	23.777
Target Compounds						
9) A Endosulfan I	0.000	6.227f	0	881240	N.D.	0.709
10) B trans-Chl...	0.000	6.054	0	3395809	N.D.	2.459


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091219\
Data File : PD054499.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Sep 2019 13:23
Operator : SG\AJ
Sample : K4718-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 01:26:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090419CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 05 08:40:10 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

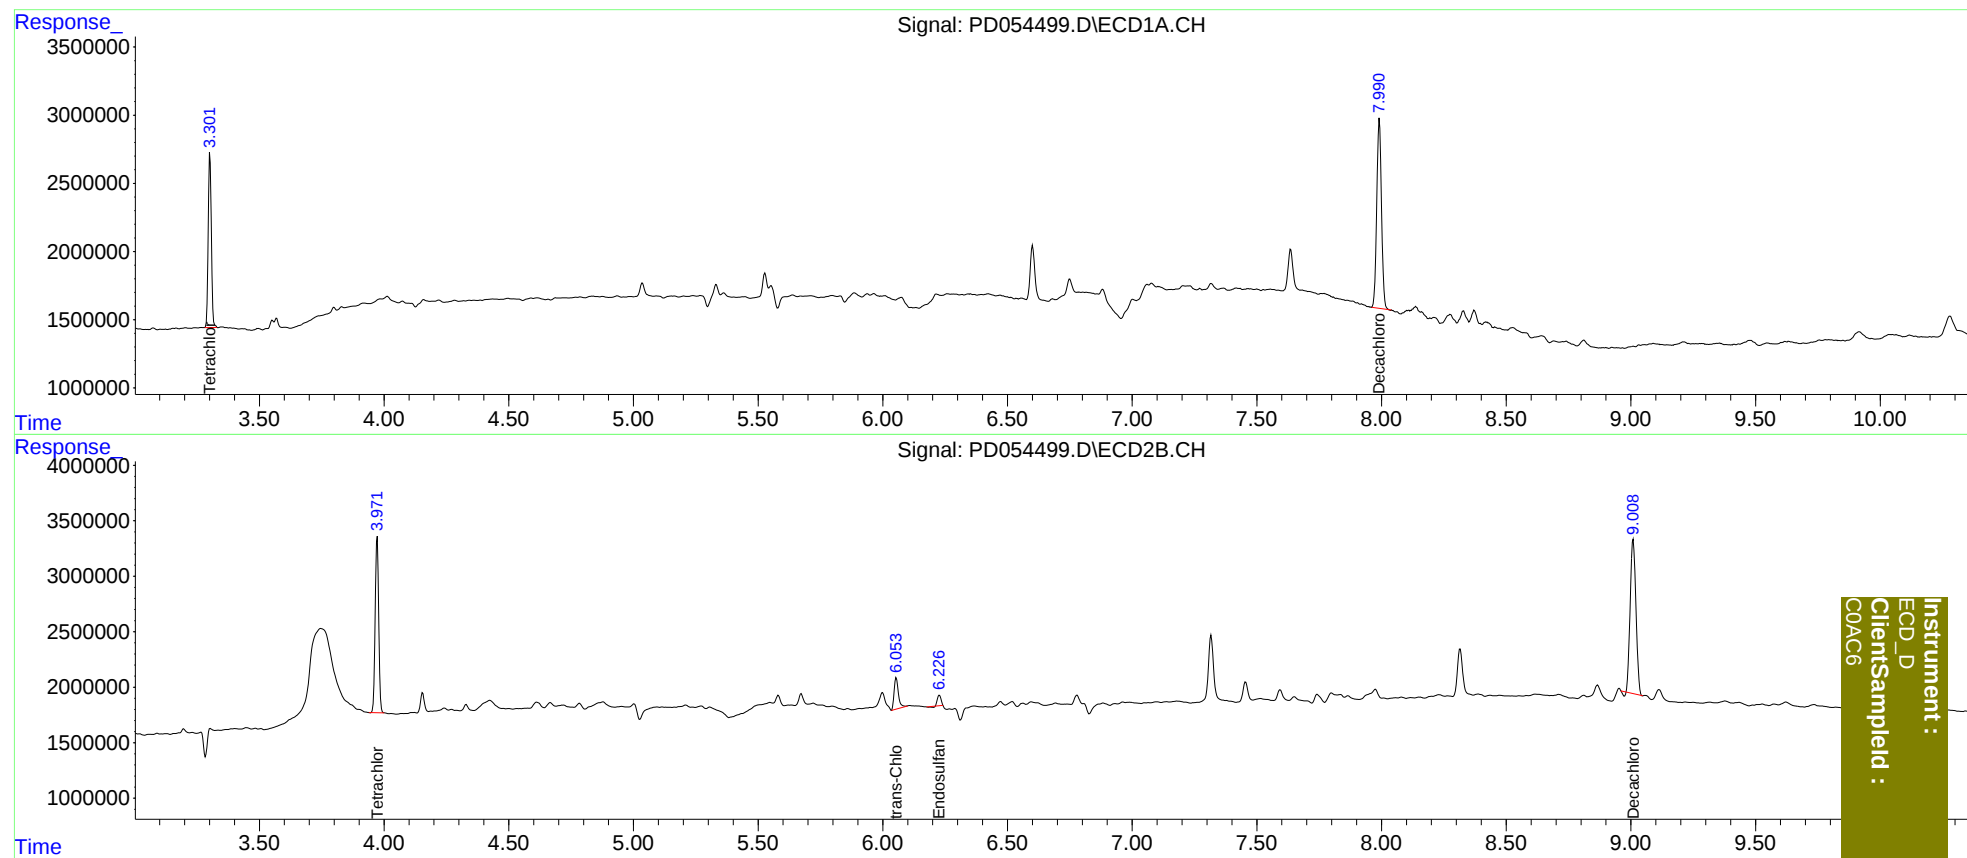


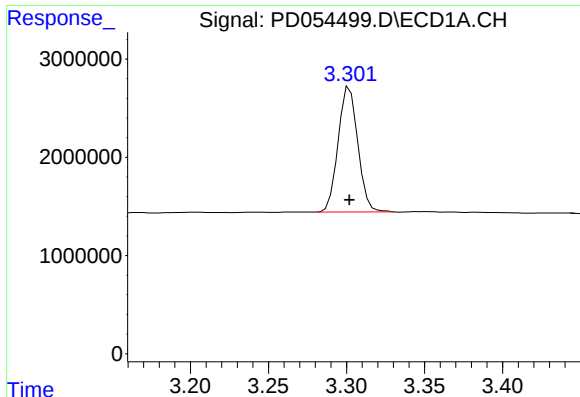

#1 Tetrachloro-m-xylene


R.T.: 3.302 min
Delta R.T.: 0.000 min
Response: 11210363
Conc: 15.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AC6

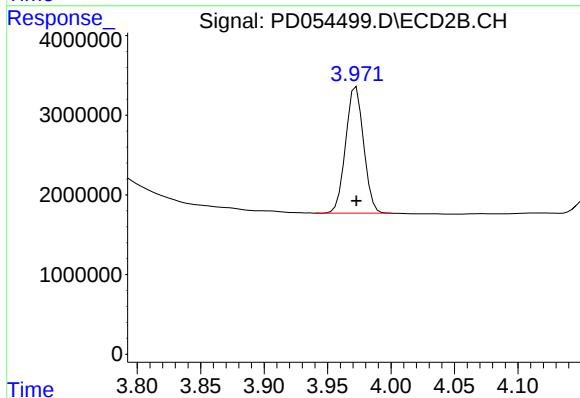


#1 Tetrachloro-m-xylene

R.T.: 3.973 min
Delta R.T.: 0.000 min
Response: 15584117
Conc: 15.79 ng/ml

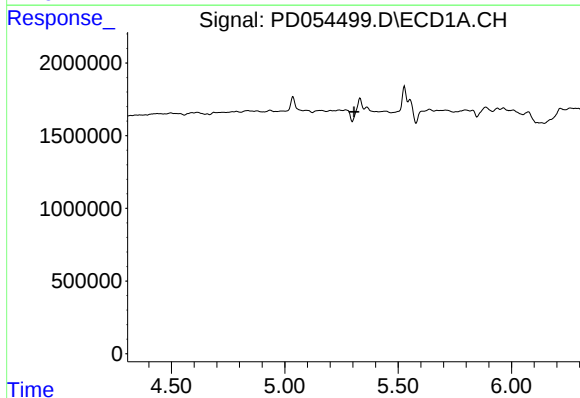


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.306 min
Response: 0
Conc: N.D.

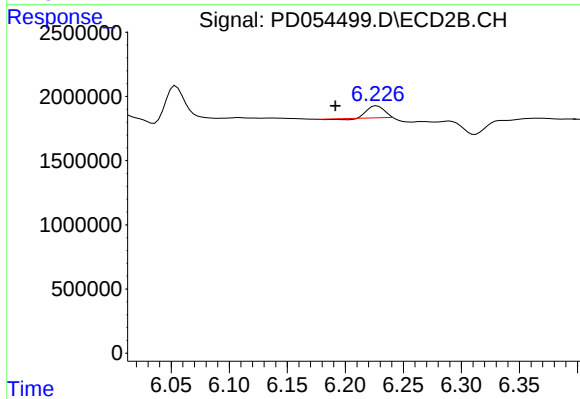

#9 Endosulfan I


R.T.: 6.227 min
Delta R.T.: 0.036 min
Response: 881240
Conc: 0.71 ng/ml

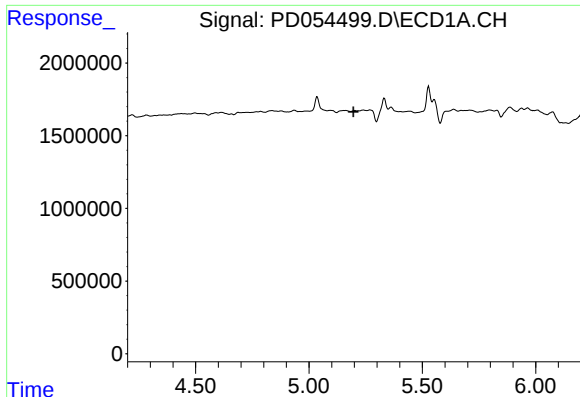

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.197 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0AC6

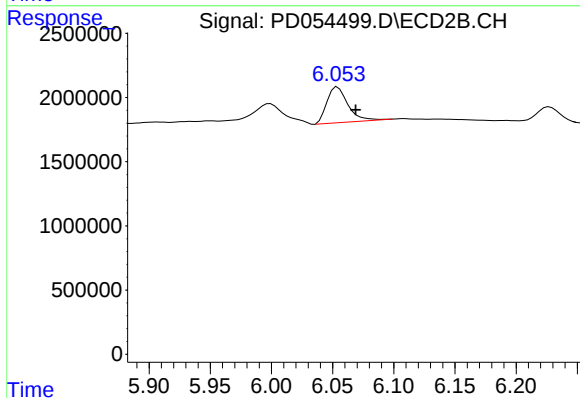


#10 trans-Chlordane

R.T.: 6.054 min
Delta R.T.: -0.015 min
Response: 3395809
Conc: 2.46 ng/ml

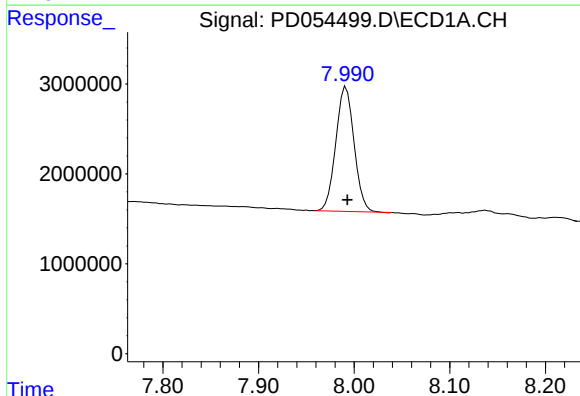

#27 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: -0.002 min
Response: 18371782
Conc: 27.15 ng/ml

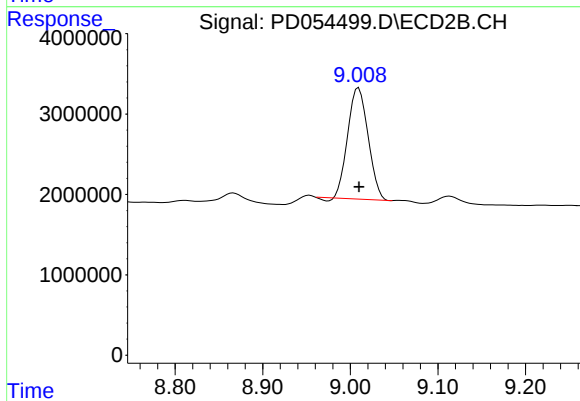

#27 Decachlorobiphenyl

R.T.: 9.009 min
Delta R.T.: 0.000 min
Response: 22243270
Conc: 23.78 ng/ml