Quantitation Report (Not Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091219\
Data File : PD054504.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Sep 2019 14:33
Operator : SG\AJ
Sample : K4718-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument : ECD_D
ClientSampleId : C0AE0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 01:30:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090419CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 05 08:40:10 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
	System Monitoring Compounds						
1)	SA Tetrachlo...	3.301	3.973	11534659	16140957	16.320	16.355
27)	SA Decachlor...	7.991	9.009	18673643	24742773	27.593	26.449
	Target Compounds						
15)	B Endosulfa...	0.000	6.883	0	3875589	N.D.	3.110

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091219\
Data File : PD054504.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Sep 2019 14:33
Operator : SG\AJ
Sample : K4718-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 01:30:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090419CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 05 08:40:10 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

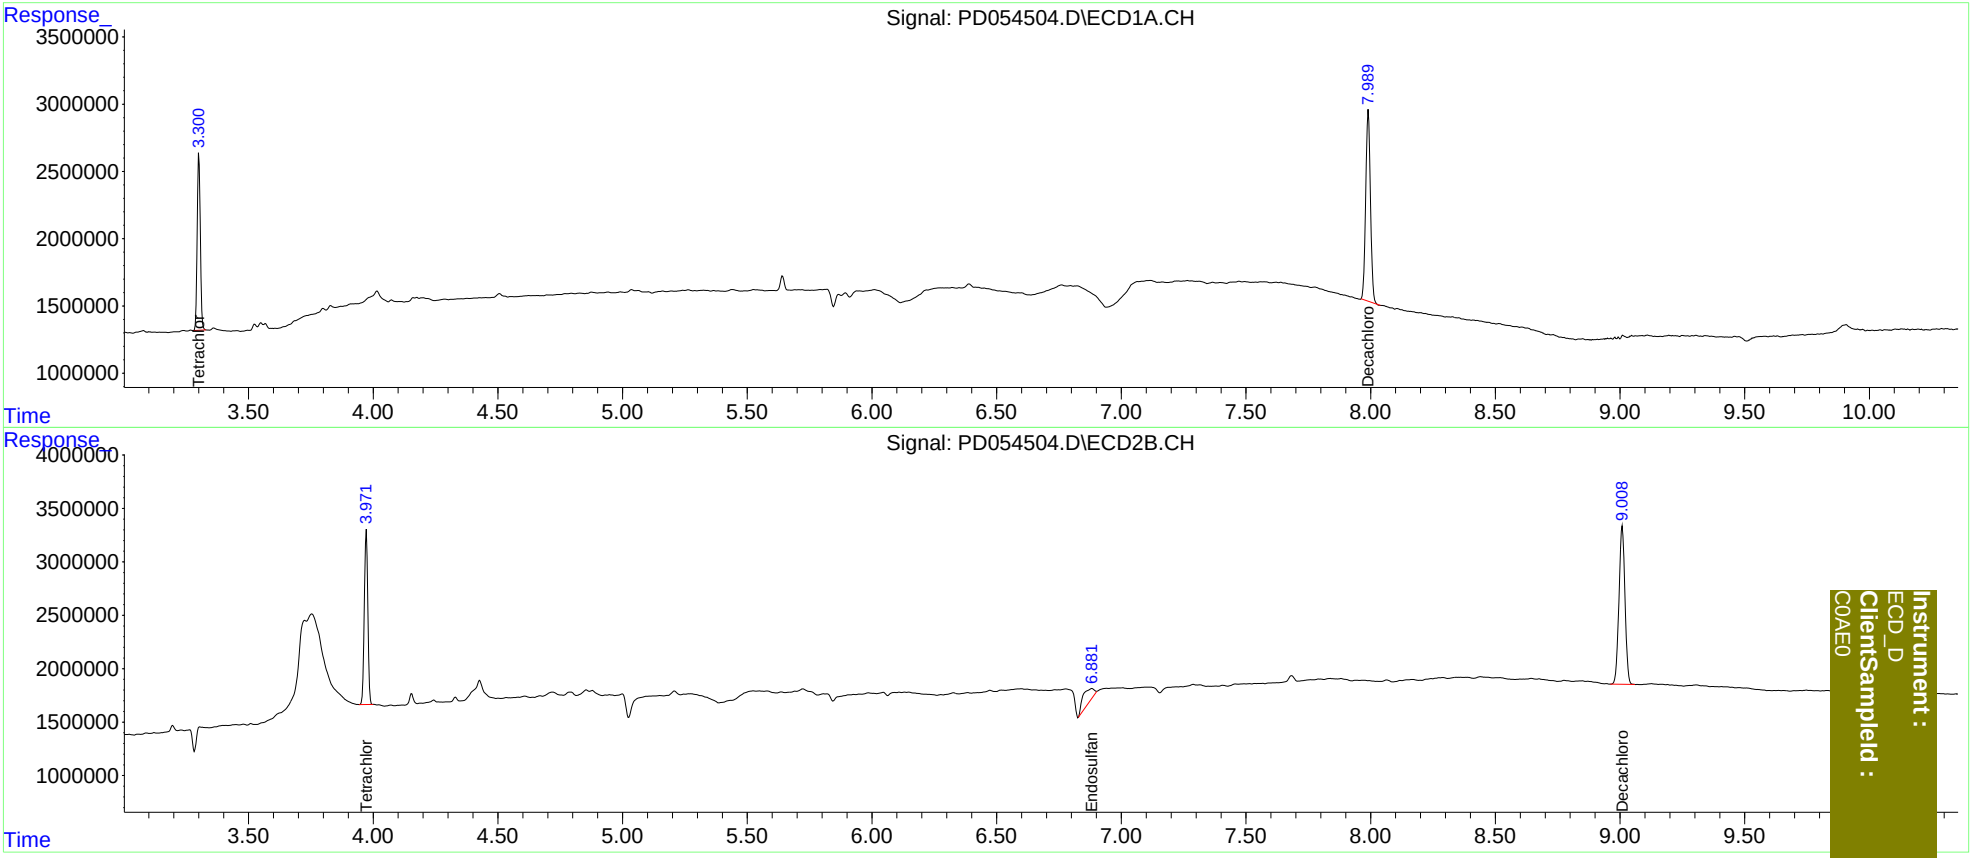

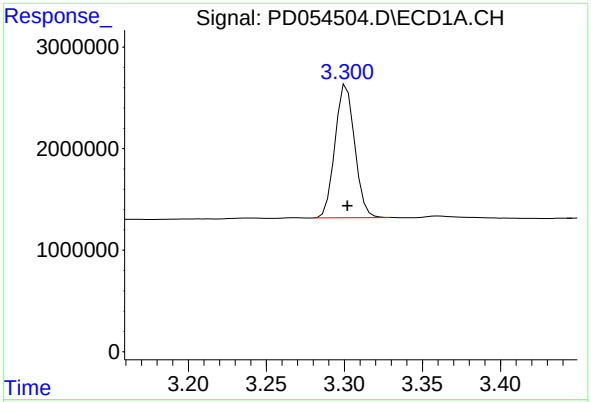

#1 Tetrachloro-m-xylene

R.T.: 3.301 min
Delta R.T.: 0.000 min
Response: 11534659
Conc: 16.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AE0

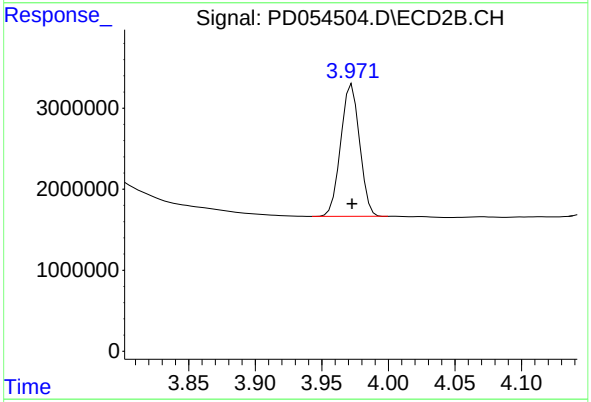

#1 Tetrachloro-m-xylene

R.T.: 3.973 min
Delta R.T.: 0.000 min
Response: 16140957
Conc: 16.35 ng/ml

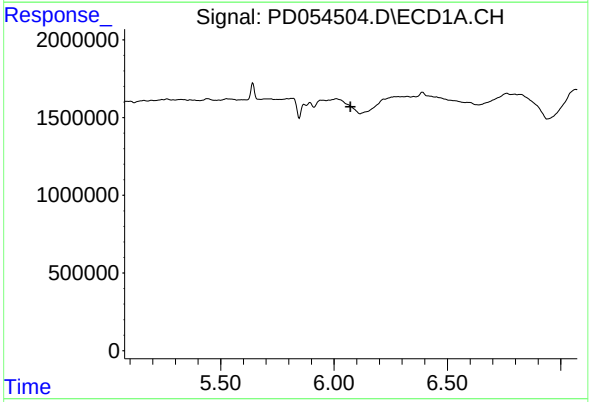

#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.073 min
Response: 0
Conc: N.D.

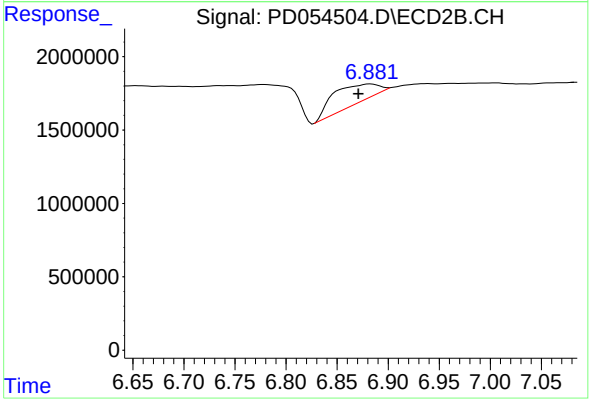

#15 Endosulfan II

R.T.: 6.883 min
Delta R.T.: 0.012 min
Response: 3875589
Conc: 3.11 ng/ml

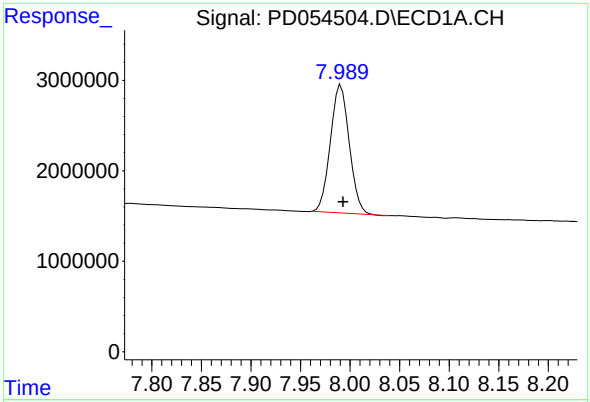

#27 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: -0.002 min
Response: 18673643
Conc: 27.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AE0

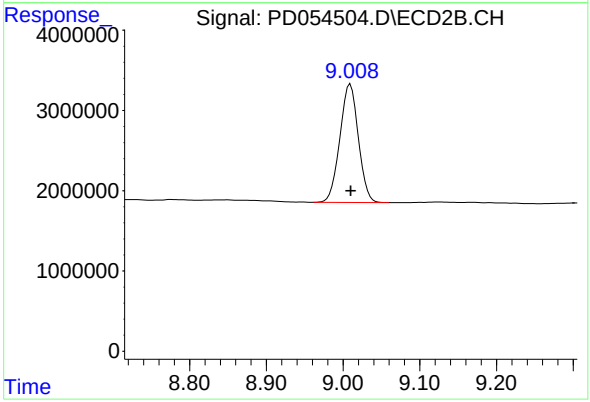

#27 Decachlorobiphenyl

R.T.: 9.009 min
Delta R.T.: 0.000 min
Response: 24742773
Conc: 26.45 ng/ml