

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091222\
 Data File : PD071821.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2022 13:00
 Operator : AR\AJ
 Sample : PB147508BS
 Misc : CH BS
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB147508BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 04:33:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091022.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 10 22:11:50 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.809	3.564	66861139	727.0E6	27.343	25.334
28)	SA Decachlor...	7.998	9.090	61094673	231.6E6	24.251	24.916
Target Compounds							
23)	Chlordane-1	3.821	4.726	23123792	243.8E6	227.375	254.092
24)	Chlordane-2	4.404	5.260	29005852	177.1E6	237.692	256.212
25)	Chlordane-3	5.041	5.971	77853963	545.5E6	228.966	248.307
26)	Chlordane-4	5.104	6.050	72299797	636.1E6	230.113	247.536
27)	Chlordane-5	6.006	6.912	27761527	121.3E6	222.515	246.635



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091222\
Data File : PD071821.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2022 13:00
Operator : AR\AJ
Sample : PB147508BS
Misc : CH BS
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB147508BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 04:33:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091022.M
Quant Title : GC Extractables
QLast Update : Sat Sep 10 22:11:50 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

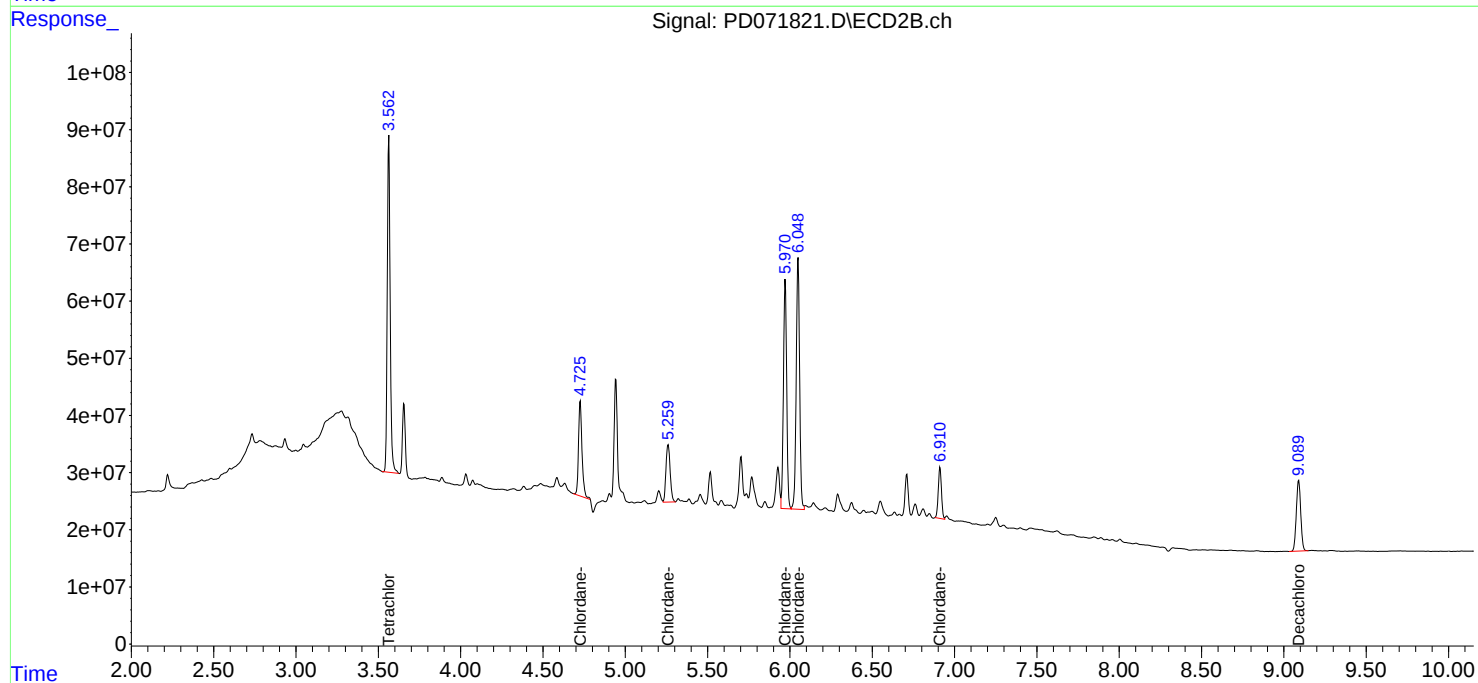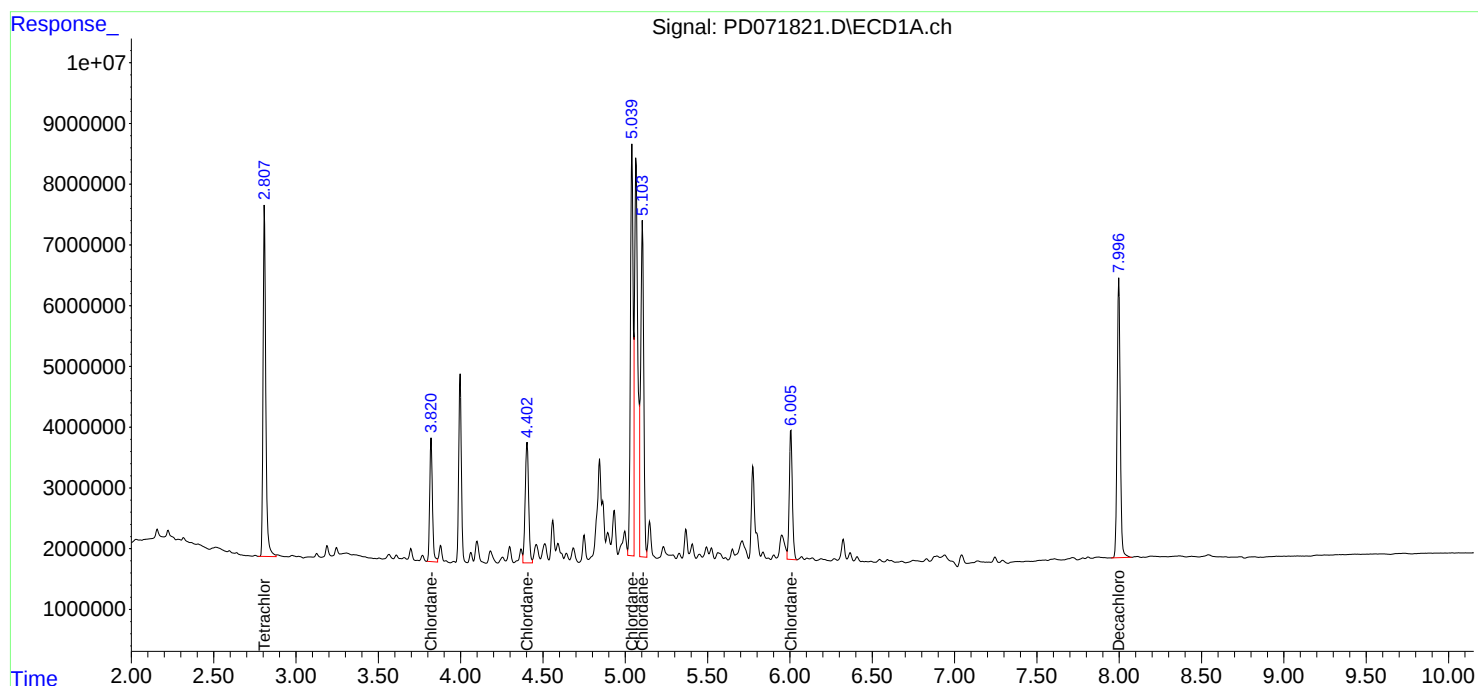


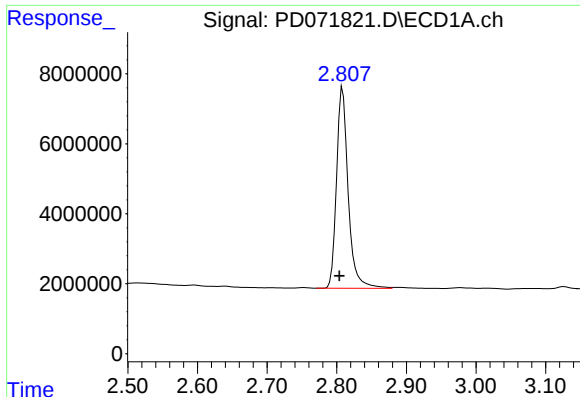

#1 Tetrachloro-m-xylene


R.T.: 2.809 min
Delta R.T.: 0.005 min
Response: 66861139
Conc: 27.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB147508BS

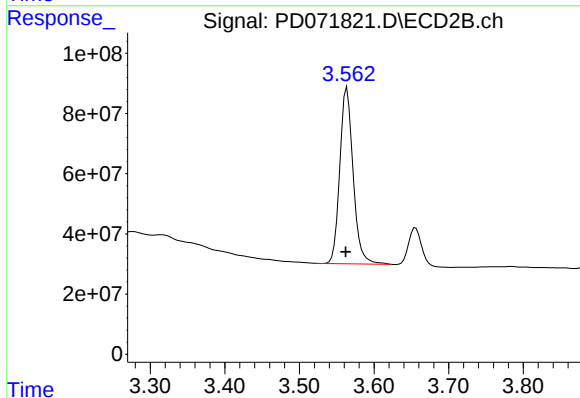


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: 0.002 min
Response: 726978126
Conc: 25.33 ng/ml

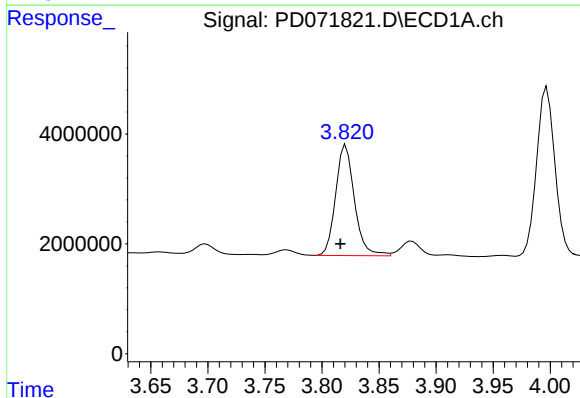


#23 Chlordane-1

R.T.: 3.821 min
Delta R.T.: 0.005 min
Response: 23123792
Conc: 227.38 ng/ml

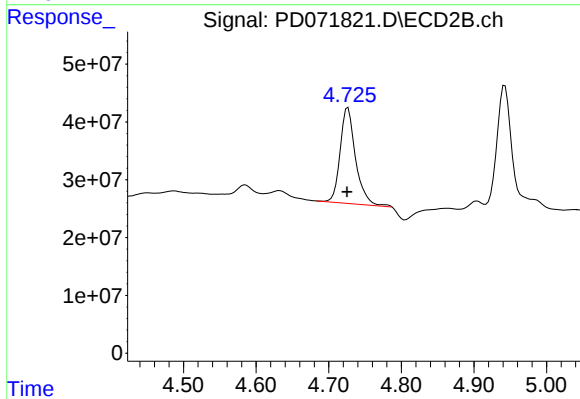

#23 Chlordane-1


R.T.: 4.726 min
Delta R.T.: 0.001 min
Response: 243830367
Conc: 254.09 ng/ml

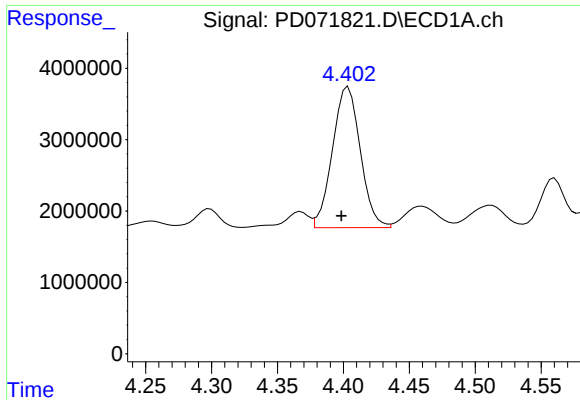

#24 Chlordane-2


R.T.: 4.404 min
Delta R.T.: 0.005 min
Response: 29005852
Conc: 237.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB147508BS

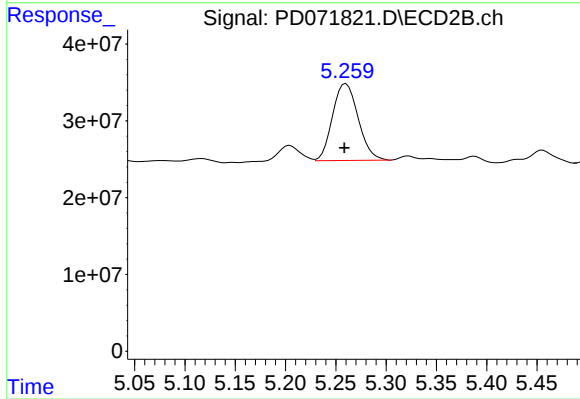


#24 Chlordane-2

R.T.: 5.260 min
Delta R.T.: 0.002 min
Response: 177134556
Conc: 256.21 ng/ml

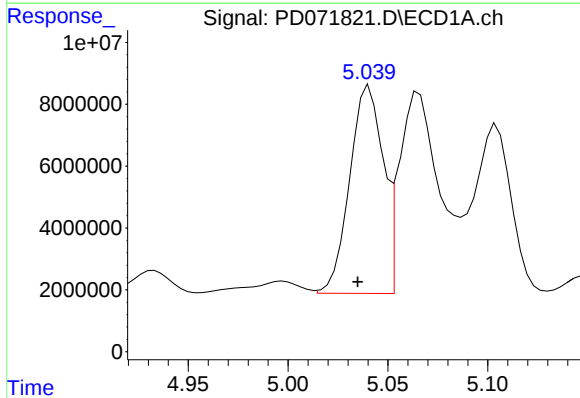


#25 Chlordane-3

R.T.: 5.041 min
Delta R.T.: 0.006 min
Response: 77853963
Conc: 228.97 ng/ml

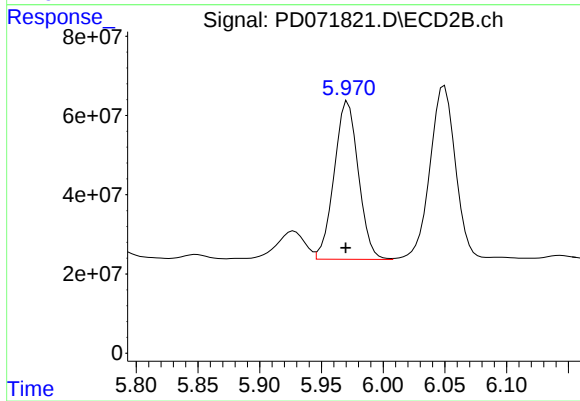

#25 Chlordane-3


R.T.: 5.971 min
Delta R.T.: 0.002 min
Response: 545483994
Conc: 248.31 ng/ml

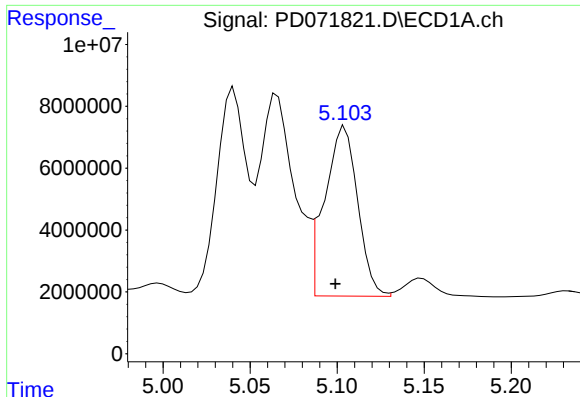

#26 Chlordane-4


R.T.: 5.104 min
Delta R.T.: 0.005 min
Response: 72299797
Conc: 230.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB147508BS

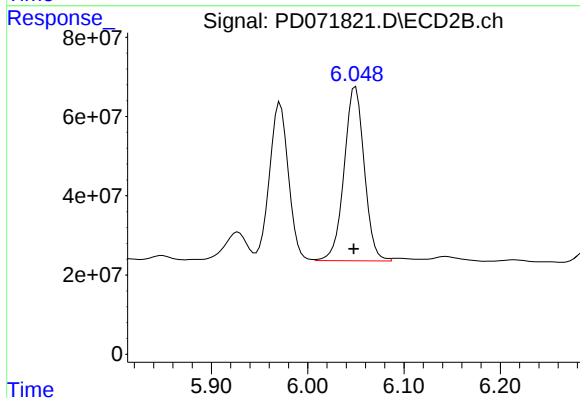


#26 Chlordane-4

R.T.: 6.050 min
Delta R.T.: 0.002 min
Response: 636090648
Conc: 247.54 ng/ml

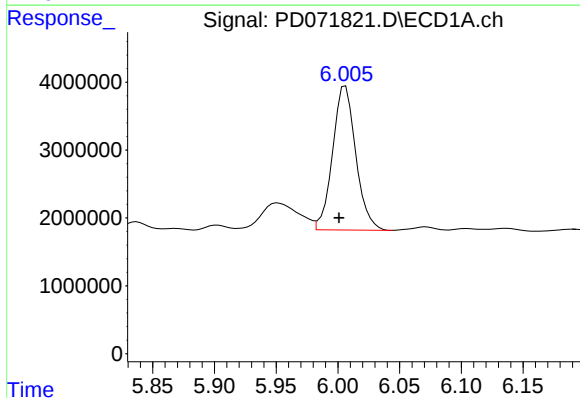


#27 Chlordane-5

R.T.: 6.006 min
Delta R.T.: 0.005 min
Response: 27761527
Conc: 222.52 ng/ml

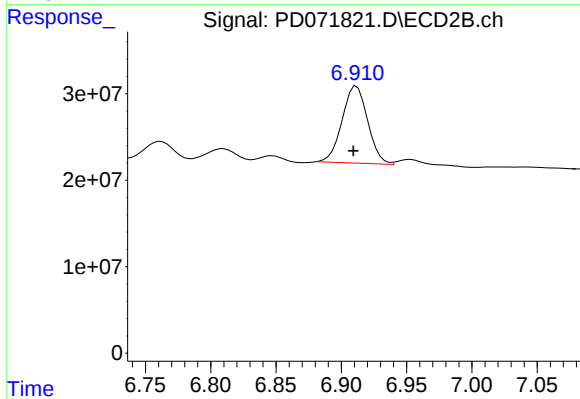

#27 Chlordane-5


R.T.: 6.912 min
Delta R.T.: 0.002 min
Response: 121312267
Conc: 246.64 ng/ml

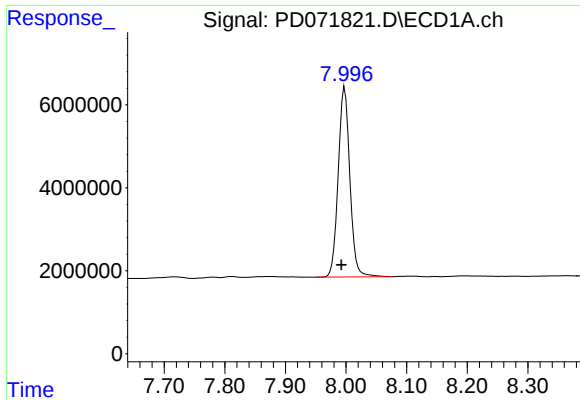

#28 Decachlorobiphenyl

R.T.: 7.998 min
Delta R.T.: 0.006 min
Response: 61094673
Conc: 24.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB147508BS

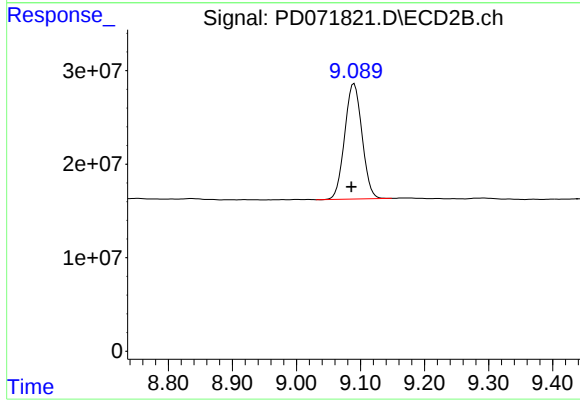

#28 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: 0.004 min
Response: 231643779
Conc: 24.92 ng/ml