

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091223\
 Data File : PD077886.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2023 02:25
 Operator : AR\AJ
 Sample : 04324-13
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 05:15:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.760	51262256	31436632	20.200	21.271
27)	SA Decachlor...	9.082	7.898	65620363	36207872	21.006	22.357
Target Compounds							
2)	A alpha-BHC	0.000	3.274	0	434449	N.D.	0.192
4)	MA Heptachlor	4.880f	3.944	1810502	2839934	0.433	1.277 #
5)	MB Aldrin	0.000	4.199	0	198270	N.D.	<MDL
6)	B beta-BHC	0.000	3.843f	0	881558	N.D.	0.892
7)	B delta-BHC	4.768	0.000	2561857	0	0.638	N.D. #
13)	MA Dieldrin	0.000	5.347	0	230914	N.D.	0.112


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091223\
Data File : PD077886.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2023 02:25
Operator : AR\AJ
Sample : 04324-13
Misc :
ALS Vial : 42 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 05:15:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

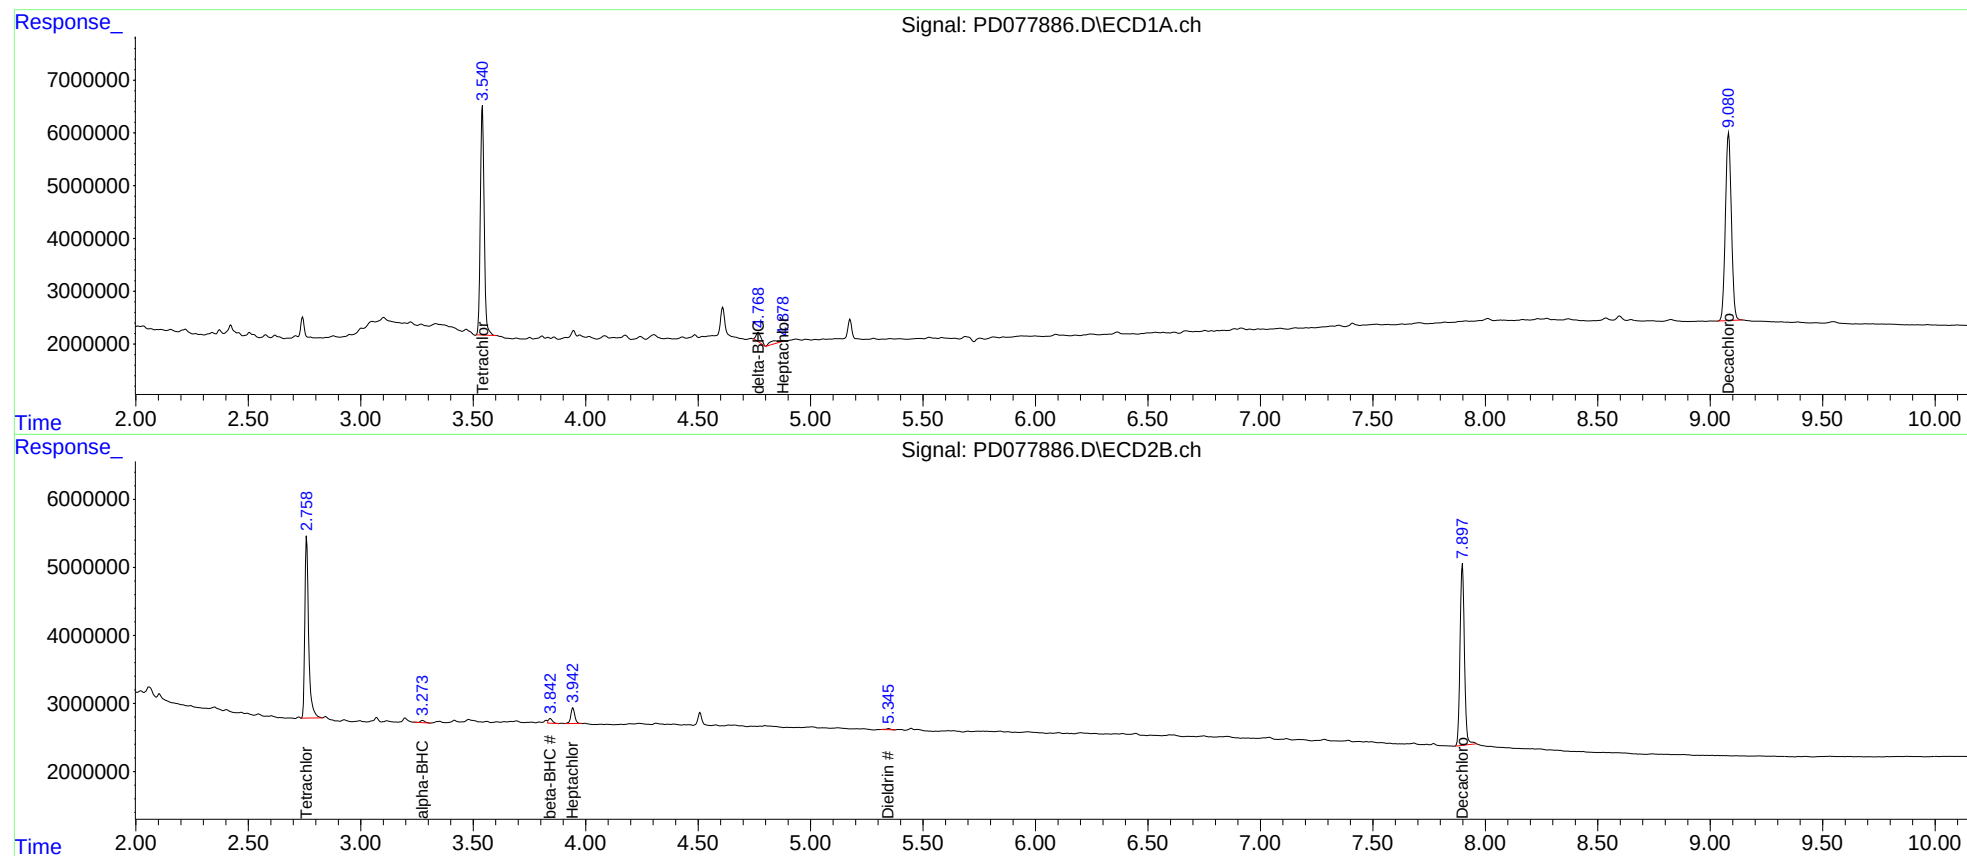

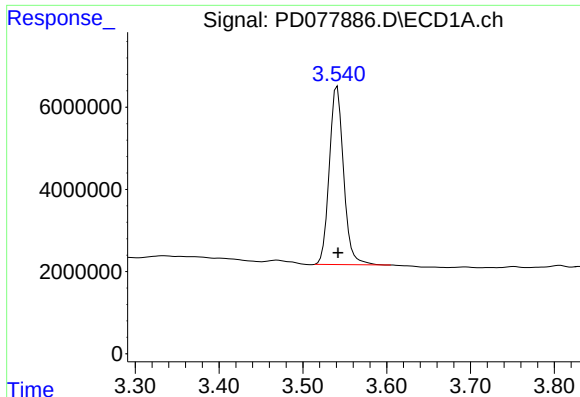


#1 Tetrachloro-m-xylene

R.T.: 3.541 min
Delta R.T.: 0.000 min
Response: 51262256
Conc: 20.20 ng/ml

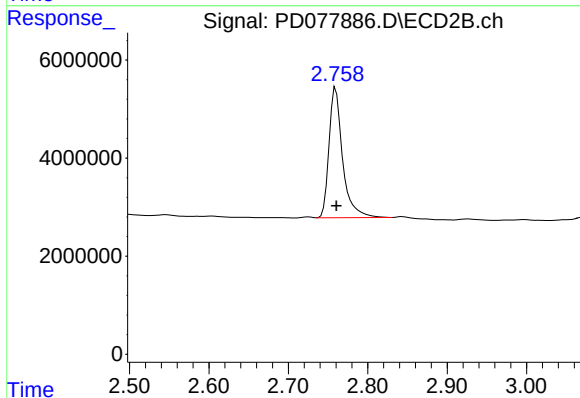


#1 Tetrachloro-m-xylene

R.T.: 2.760 min
Delta R.T.: 0.000 min
Response: 31436632
Conc: 21.27 ng/ml

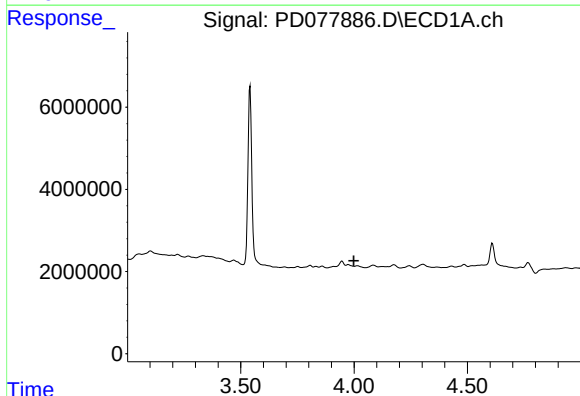


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.999 min
Response: 0
Conc: N.D.

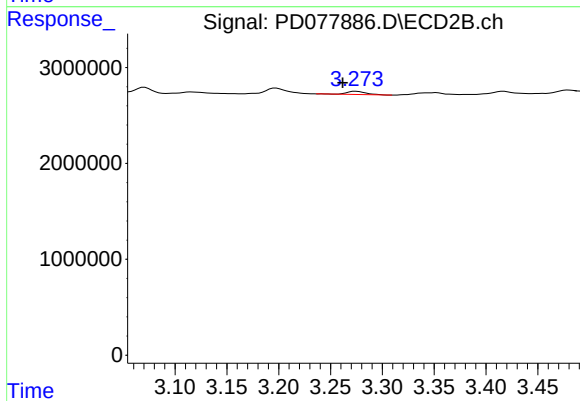


#2 alpha-BHC

R.T.: 3.274 min
Delta R.T.: 0.012 min
Response: 434449
Conc: 0.19 ng/ml

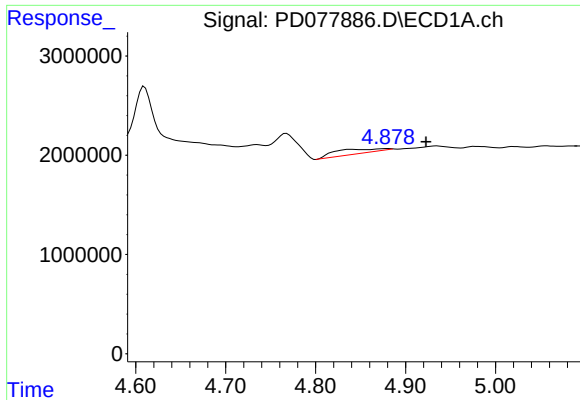


#4 Heptachlor

R.T.: 4.880 min
Delta R.T.: -0.043 min
Response: 1810502
Conc: 0.43 ng/ml

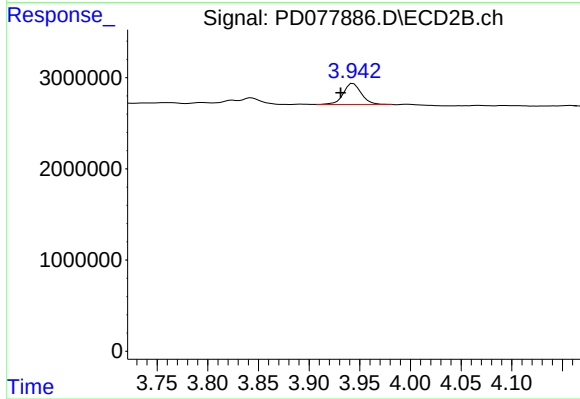


#4 Heptachlor

R.T.: 3.944 min
Delta R.T.: 0.012 min
Response: 2839934
Conc: 1.28 ng/ml

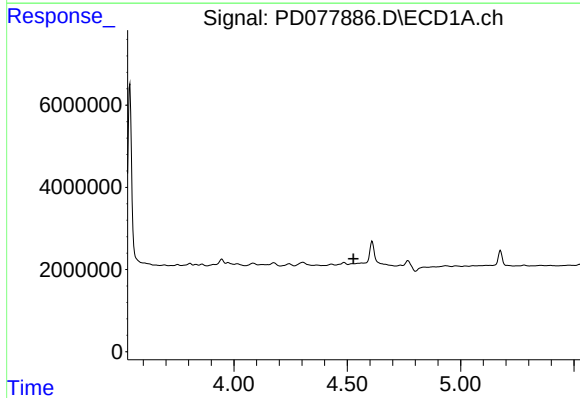


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.528 min
Response: 0
Conc: N.D.

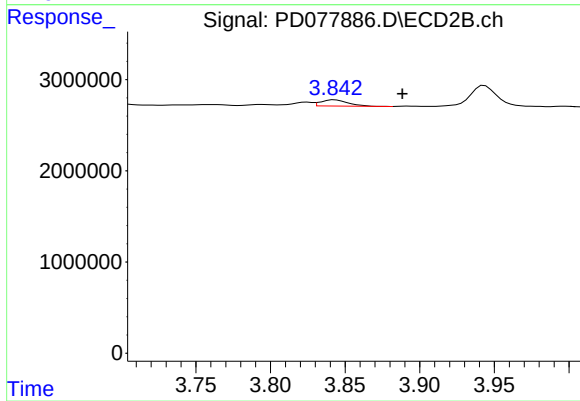


#6 beta-BHC

R.T.: 3.843 min
Delta R.T.: -0.045 min
Response: 881558
Conc: 0.89 ng/ml

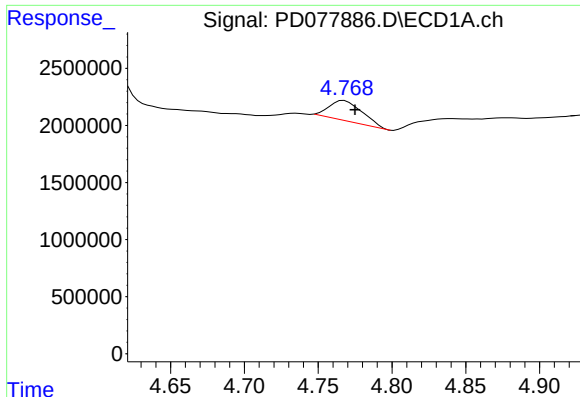


#7 delta-BHC

R.T.: 4.768 min
Delta R.T.: -0.007 min
Response: 2561857
Conc: 0.64 ng/ml

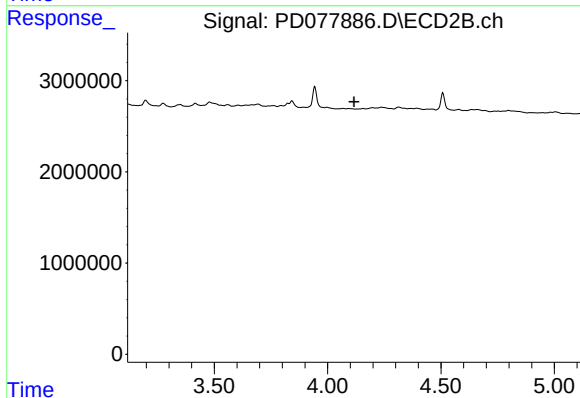


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.118 min
Response: 0
Conc: N.D.

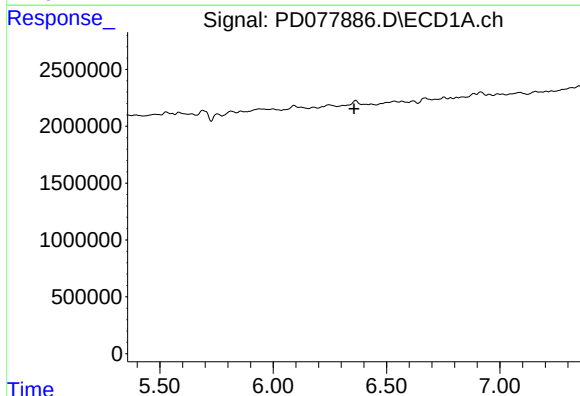


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.356 min
Response: 0
Conc: N.D.

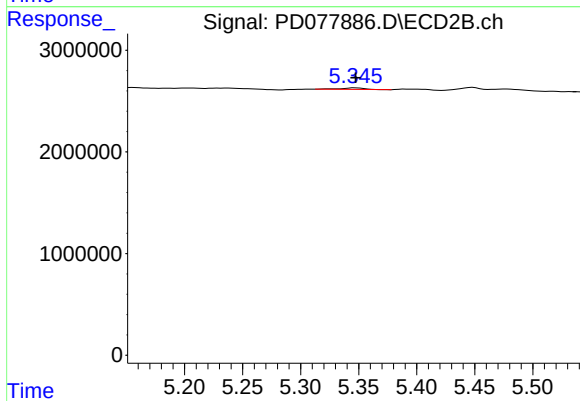


#13 Dieldrin

R.T.: 5.347 min
Delta R.T.: 0.000 min
Response: 230914
Conc: 0.11 ng/ml

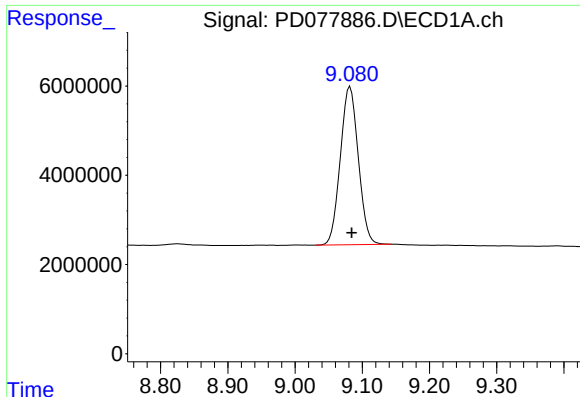

#27 Decachlorobiphenyl

R.T.: 9.082 min
Delta R.T.: -0.003 min
Response: 65620363
Conc: 21.01 ng/ml

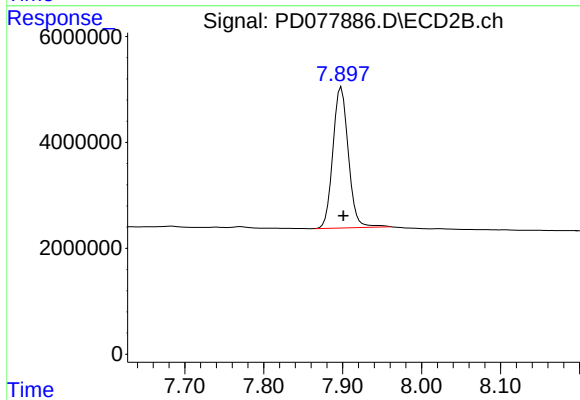

#27 Decachlorobiphenyl

R.T.: 7.898 min
Delta R.T.: -0.003 min
Response: 36207872
Conc: 22.36 ng/ml