

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091223\
 Data File : PD077891.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2023 03:32
 Operator : AR\AJ
 Sample : 04324-18
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 05:16:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.760	50655215	31203739	19.961	21.114
27)	SA Decachlor...	9.082	7.898	67285134	36877485	21.539	22.771
Target Compounds							
4)	MA Heptachlor	0.000	3.945	0	228653	N.D.	0.103
8)	B Heptachlo...	5.711	4.711	3080814	277144	0.797	0.132 #
9)	A Endosulfan I	0.000	5.055	0	1813116	N.D.	1.010
10)	B trans-Chl...	0.000	4.986	0	506940	N.D.	0.254
11)	B cis-Chlor...	0.000	5.055	0	1813116	N.D.	0.887
12)	B 4,4'-DDE	0.000	5.216	0	275937	N.D.	0.145
13)	MA Dieldrin	6.355	5.346	2796072	1331983	0.747	0.645
16)	A 4,4'-DDD	0.000	5.827f	0	276695	N.D.	0.206
20)	A Methoxychlor	0.000	6.612	0	208869	N.D.	0.268
21)	B Endrin ke...	0.000	6.826	0	109772	N.D.	<MDL
22)	Toxaphene-1	0.000	4.986	0	506940	N.D.	48.568
25)	Toxaphene-4	0.000	6.612	0	208869	N.D.	5.412


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091223\
Data File : PD077891.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2023 03:32
Operator : AR\AJ
Sample : 04324-18
Misc :
ALS Vial : 47 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 05:16:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

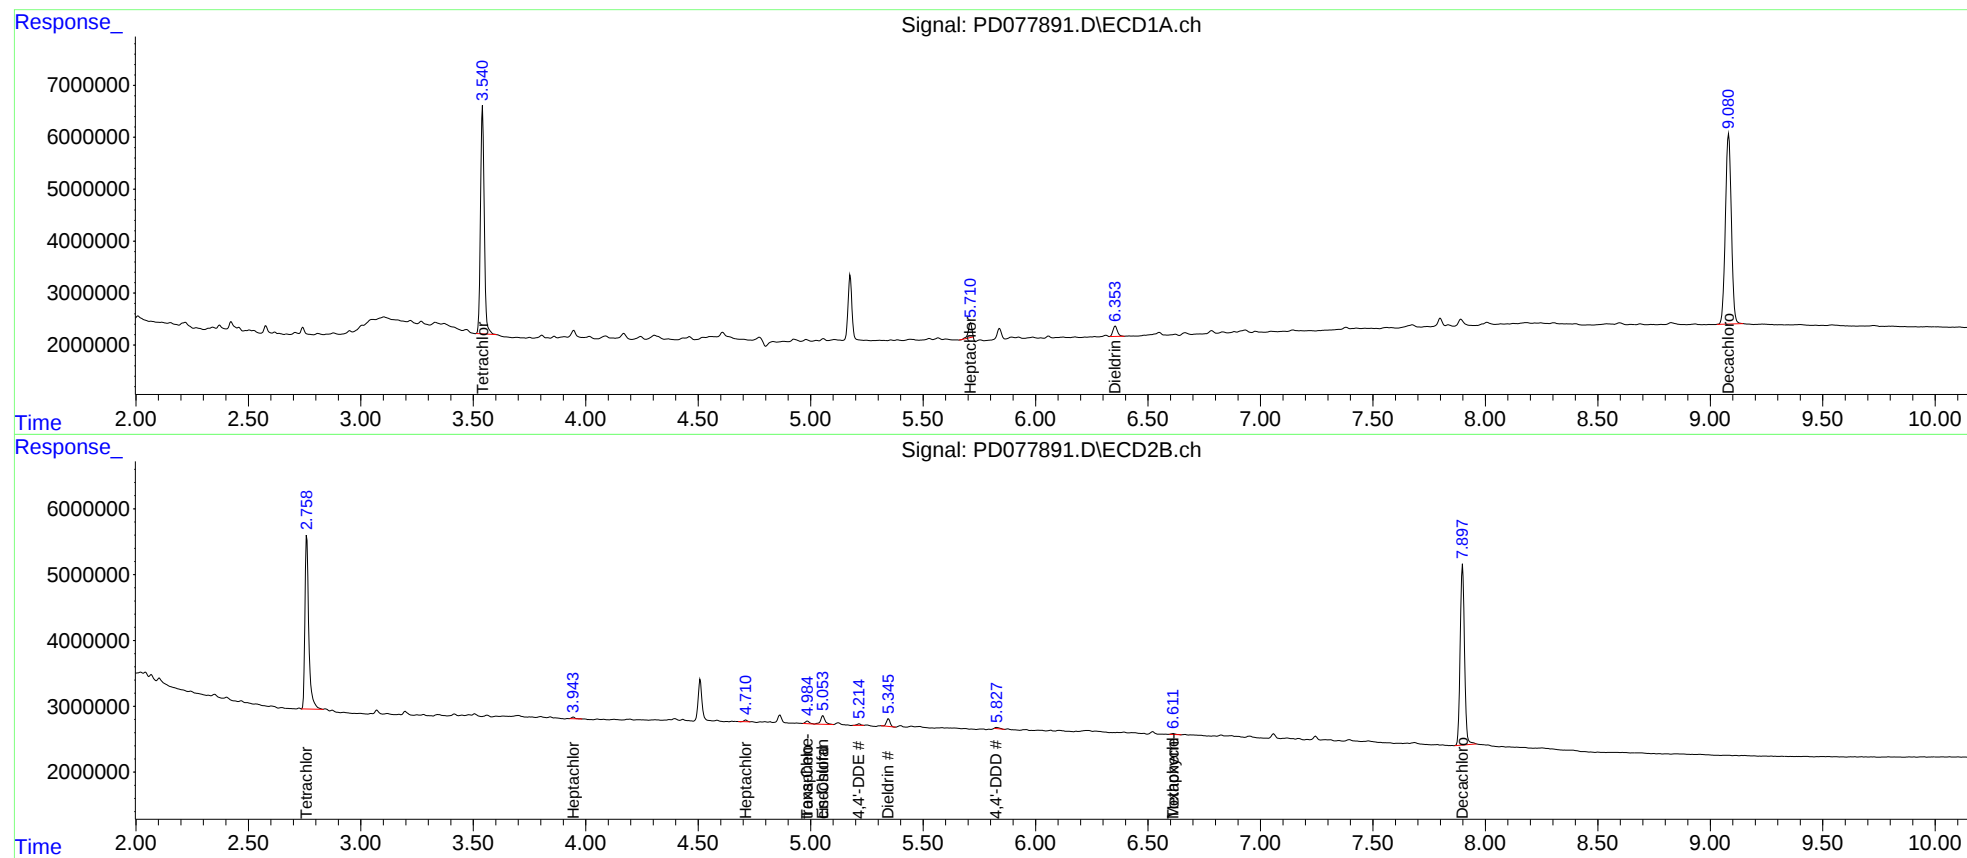

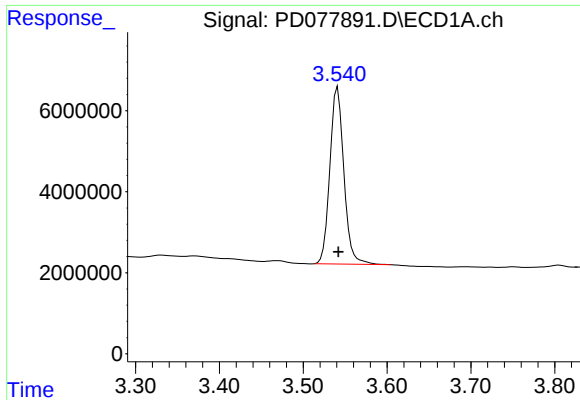


#1 Tetrachloro-m-xylene

R.T.: 3.541 min
Delta R.T.: 0.000 min
Response: 50655215
Conc: 19.96 ng/ml

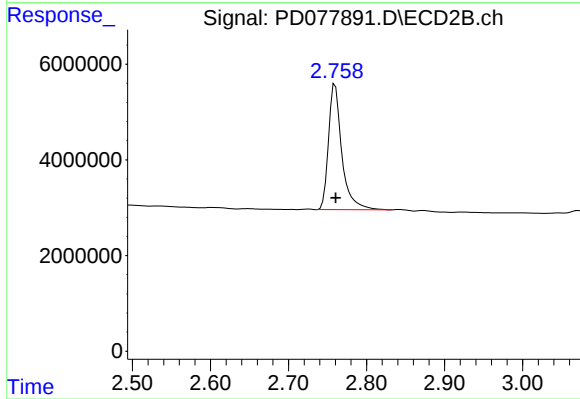


#1 Tetrachloro-m-xylene

R.T.: 2.760 min
Delta R.T.: 0.000 min
Response: 31203739
Conc: 21.11 ng/ml

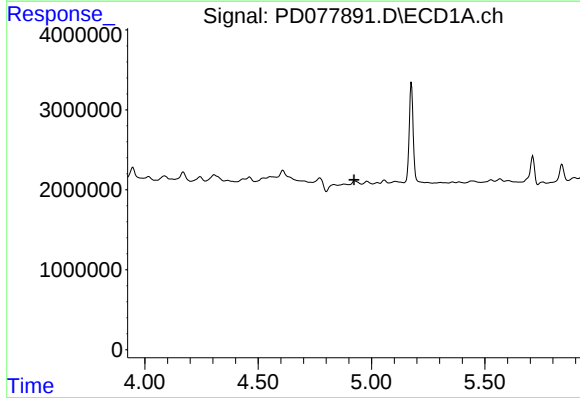


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.923 min
Response: 0
Conc: N.D.

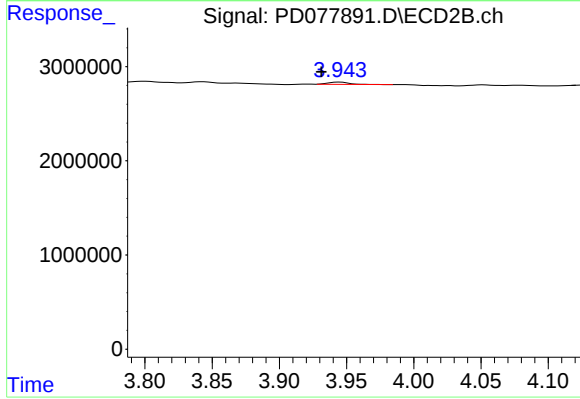


#4 Heptachlor

R.T.: 3.945 min
Delta R.T.: 0.014 min
Response: 228653
Conc: 0.10 ng/ml

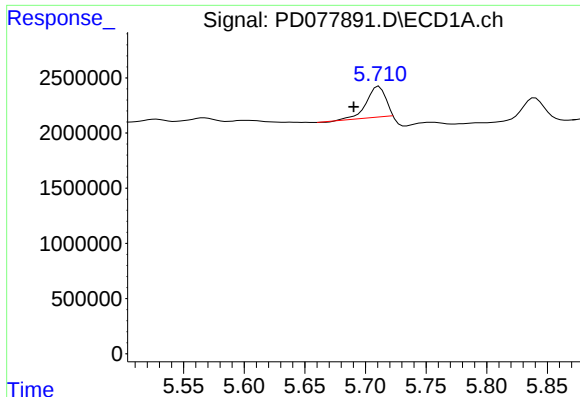


#8 Heptachlor epoxide

R.T.: 5.711 min
Delta R.T.: 0.021 min
Response: 3080814
Conc: 0.80 ng/ml

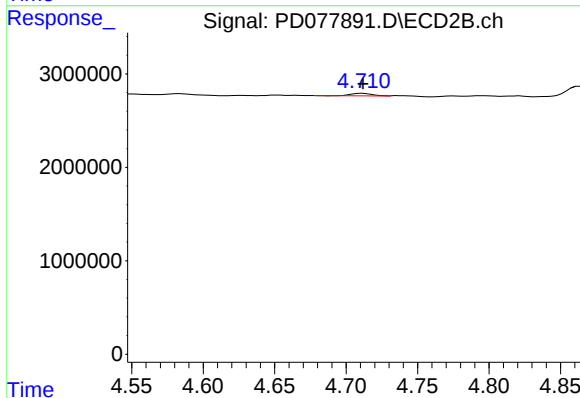


#8 Heptachlor epoxide

R.T.: 4.711 min
Delta R.T.: 0.000 min
Response: 277144
Conc: 0.13 ng/ml

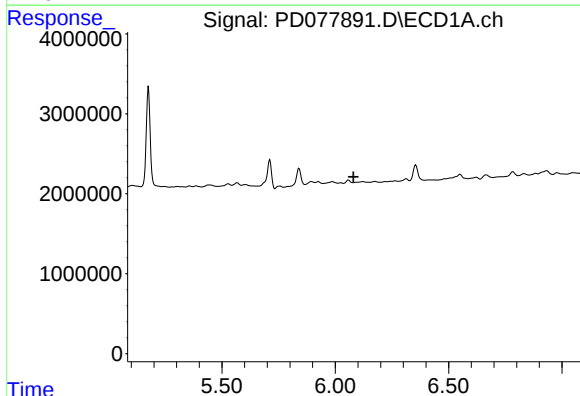


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 6.081 min
Response: 0
Conc: N.D.

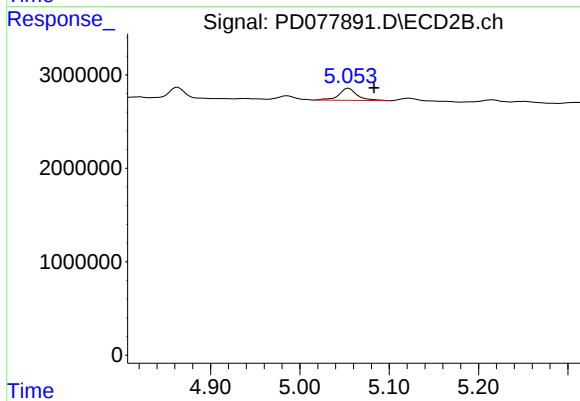


#9 Endosulfan I

R.T.: 5.055 min
Delta R.T.: -0.028 min
Response: 1813116
Conc: 1.01 ng/ml

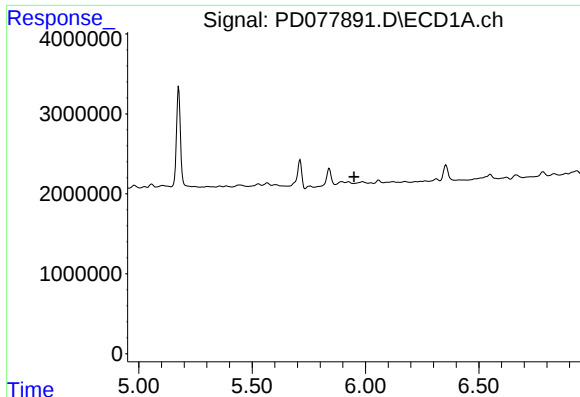


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

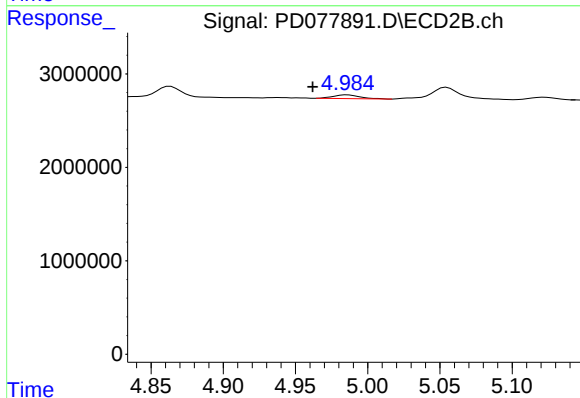


#10 trans-Chlordane

R.T.: 4.986 min
Delta R.T.: 0.024 min
Response: 506940
Conc: 0.25 ng/ml

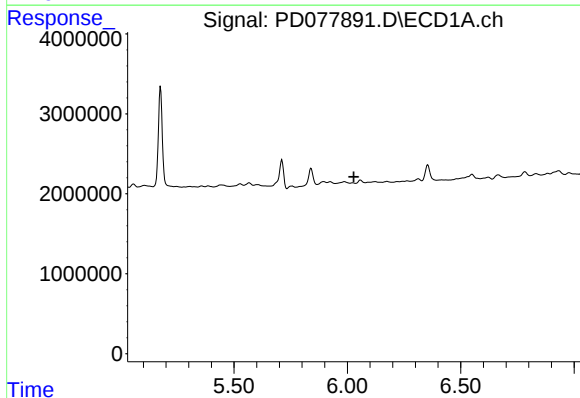


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.029 min
Response: 0
Conc: N.D.

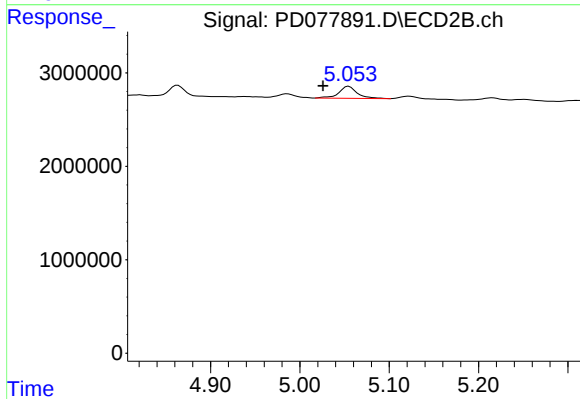


#11 cis-Chlordane

R.T.: 5.055 min
Delta R.T.: 0.029 min
Response: 1813116
Conc: 0.89 ng/ml

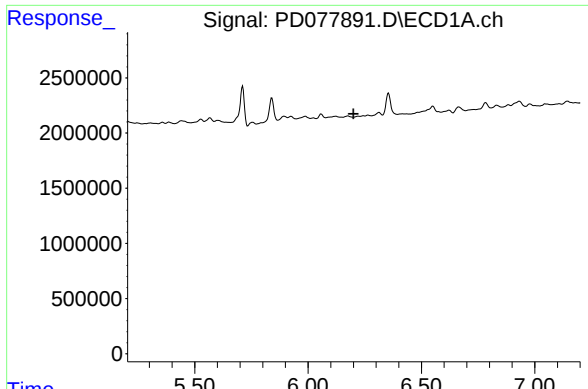


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 6.201 min
Response: 0
Conc: N.D.

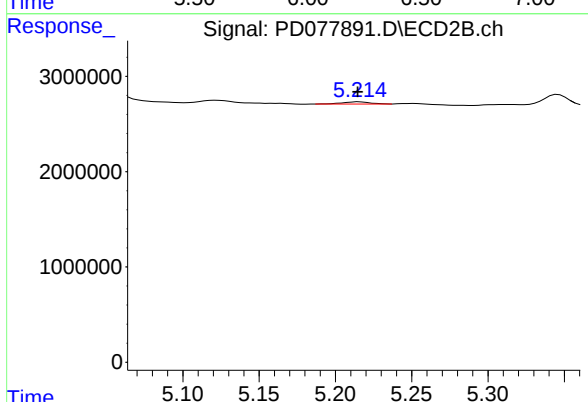


#12 4,4'-DDE

R.T.: 5.216 min
Delta R.T.: 0.000 min
Response: 275937
Conc: 0.15 ng/ml

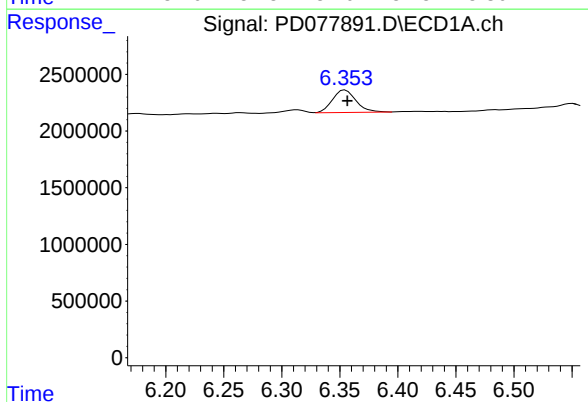


#13 Dieldrin

R.T.: 6.355 min
Delta R.T.: -0.002 min
Response: 2796072
Conc: 0.75 ng/ml

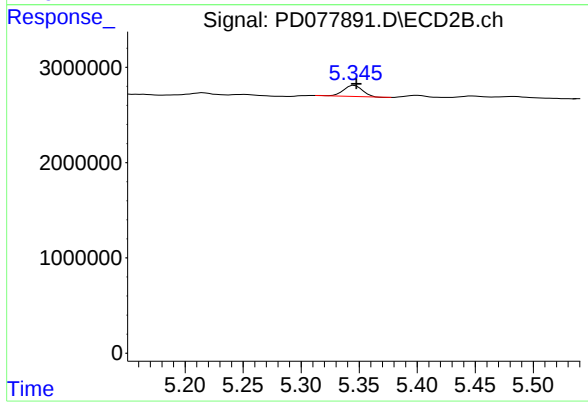


#13 Dieldrin

R.T.: 5.346 min
Delta R.T.: -0.001 min
Response: 1331983
Conc: 0.64 ng/ml

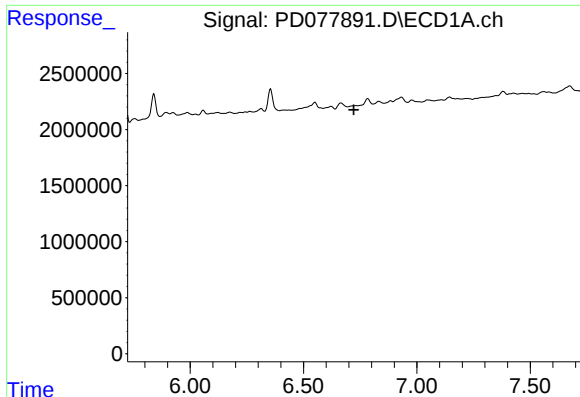


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.722 min
Response: 0
Conc: N.D.

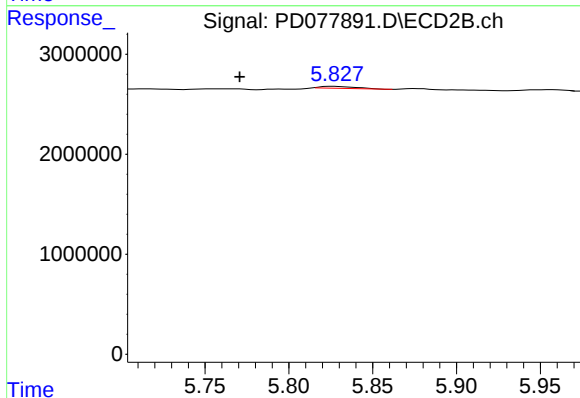


#16 4,4'-DDD

R.T.: 5.827 min
Delta R.T.: 0.056 min
Response: 276695
Conc: 0.21 ng/ml

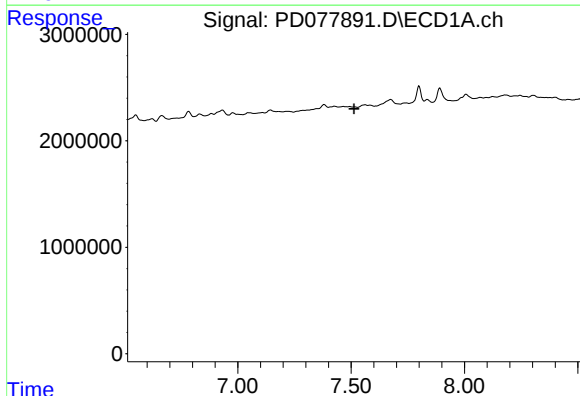


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.513 min
Response: 0
Conc: N.D.

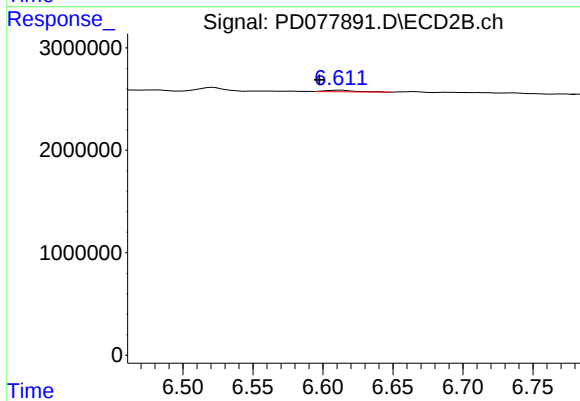


#20 Methoxychlor

R.T.: 6.612 min
Delta R.T.: 0.015 min
Response: 208869
Conc: 0.27 ng/ml

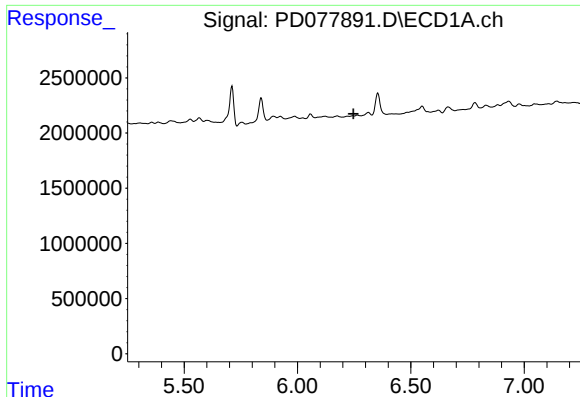


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T. : 6.247 min
Response: 0
Conc: N.D.

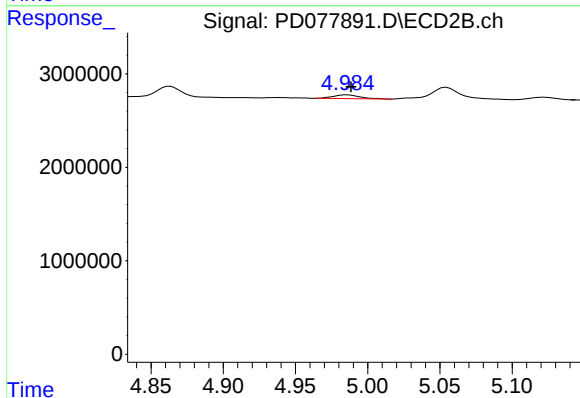


#22 Toxaphene-1

R.T.: 4.986 min
Delta R.T.: -0.003 min
Response: 506940
Conc: 48.57 ng/ml

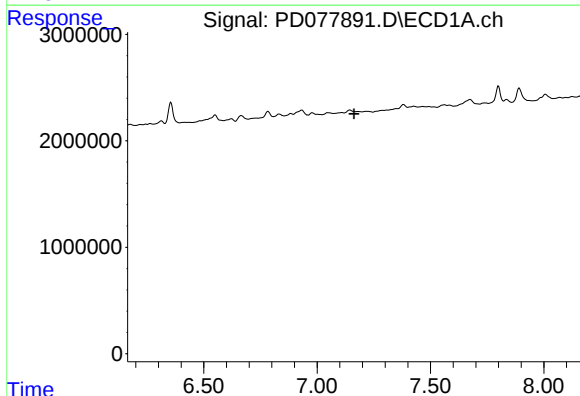


#25 Toxaphene-4

R.T.: 0.000 min
Exp R.T. : 7.163 min
Response: 0
Conc: N.D.

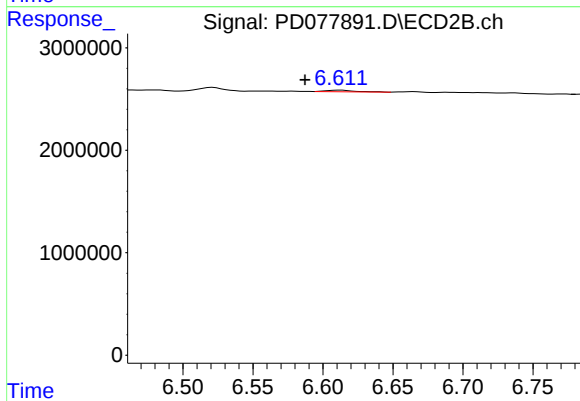


#25 Toxaphene-4

R.T.: 6.612 min
Delta R.T.: 0.025 min
Response: 208869
Conc: 5.41 ng/ml

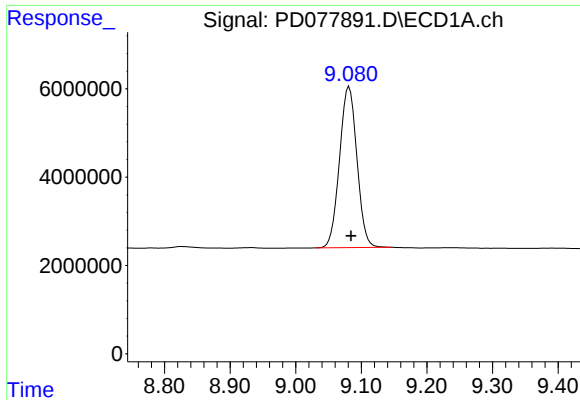

#27 Decachlorobiphenyl

R.T.: 9.082 min
Delta R.T.: -0.003 min
Response: 67285134
Conc: 21.54 ng/ml

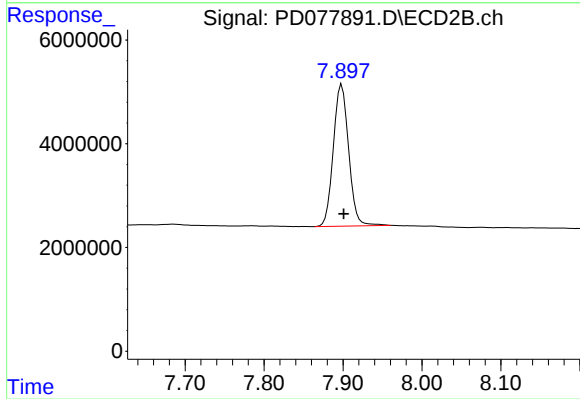

#27 Decachlorobiphenyl

R.T.: 7.898 min
Delta R.T.: -0.003 min
Response: 36877485
Conc: 22.77 ng/ml