

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091223\
 Data File : PD077893.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2023 03:58
 Operator : AR\AJ
 Sample : 04324-20
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 05:16:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.760	50428198	31620181	19.872	21.396
27)	SA Decachlor...	9.081	7.899	57831584	31442667	18.513	19.415
Target Compounds							
3)	MA gamma-BHC...	0.000	3.604	0	47817	N.D.	<MDL
8)	B Heptachlo...	5.712	4.780f	11574059	389649	2.995	0.186 #
9)	A Endosulfan I	0.000	5.055	0	9801309	N.D.	5.460
10)	B trans-Chl...	0.000	4.945	0	304462	N.D.	0.152
11)	B cis-Chlor...	0.000	5.055	0	9801309	N.D.	4.793
16)	A 4,4'-DDD	0.000	5.839f	0	123712	N.D.	<MDL
22)	Toxaphene-1	0.000	4.982	0	399575	N.D.	38.282


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091223\
Data File : PD077893.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2023 03:58
Operator : AR\AJ
Sample : 04324-20
Misc :
ALS Vial : 49 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 05:16:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

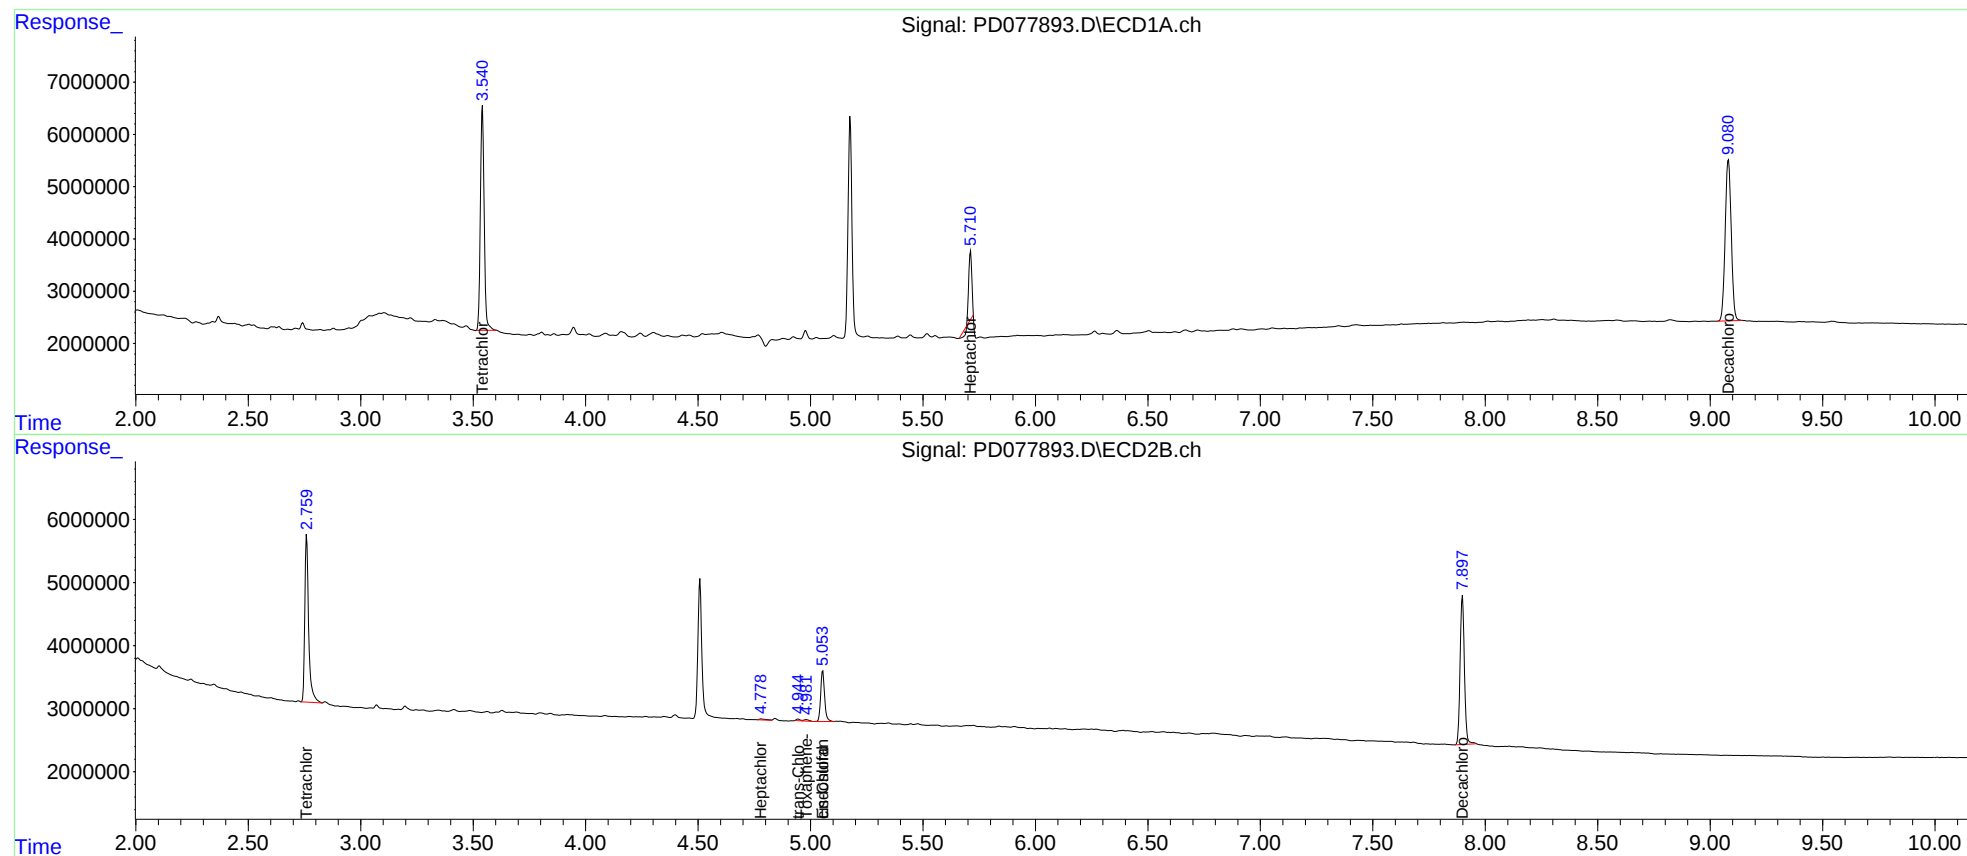

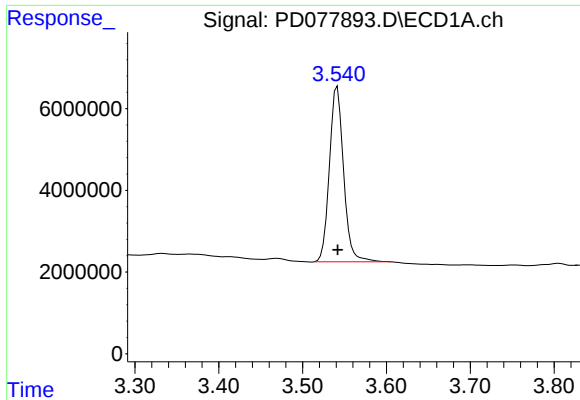


#1 Tetrachloro-m-xylene

R.T.: 3.541 min
Delta R.T.: 0.000 min
Response: 50428198
Conc: 19.87 ng/ml

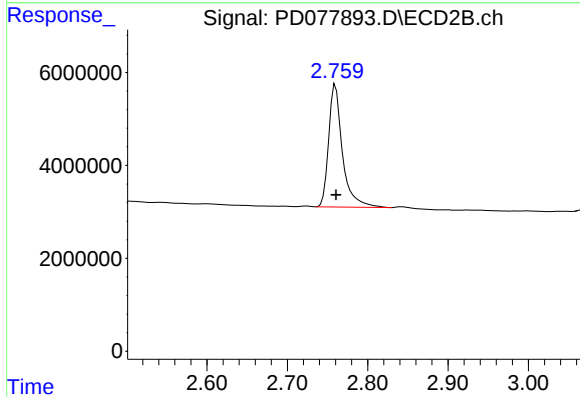


#1 Tetrachloro-m-xylene

R.T.: 2.760 min
Delta R.T.: 0.000 min
Response: 31620181
Conc: 21.40 ng/ml

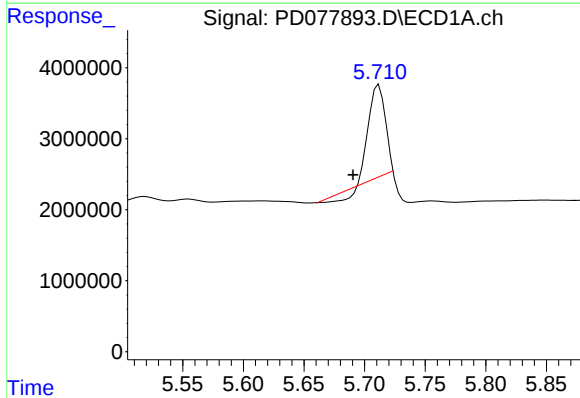


#8 Heptachlor epoxide

R.T.: 5.712 min
Delta R.T.: 0.021 min
Response: 11574059
Conc: 2.99 ng/ml

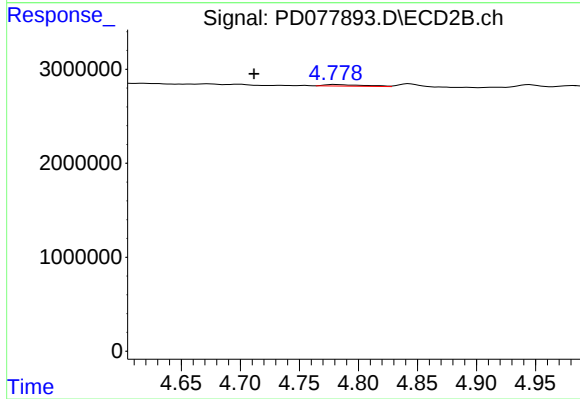


#8 Heptachlor epoxide

R.T.: 4.780 min
Delta R.T.: 0.068 min
Response: 389649
Conc: 0.19 ng/ml

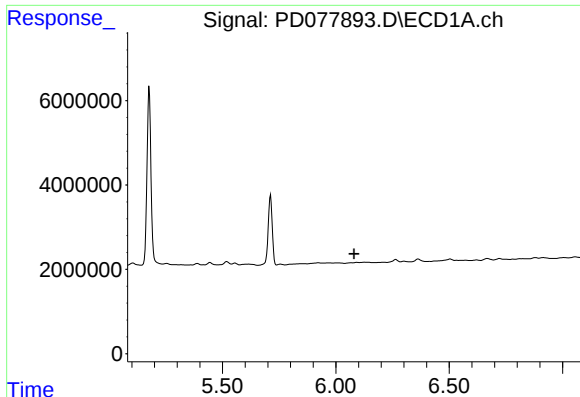


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.081 min
Response: 0
Conc: N.D.

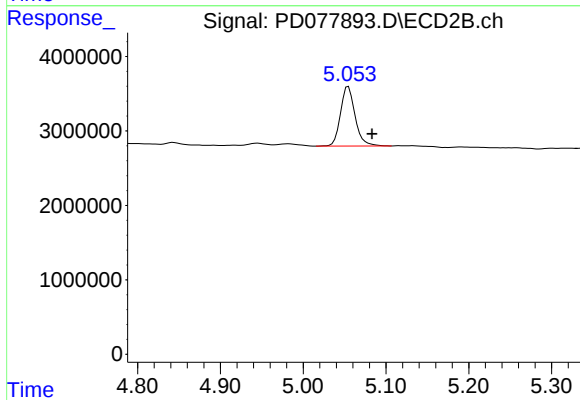


#9 Endosulfan I

R.T.: 5.055 min
Delta R.T.: -0.028 min
Response: 9801309
Conc: 5.46 ng/ml

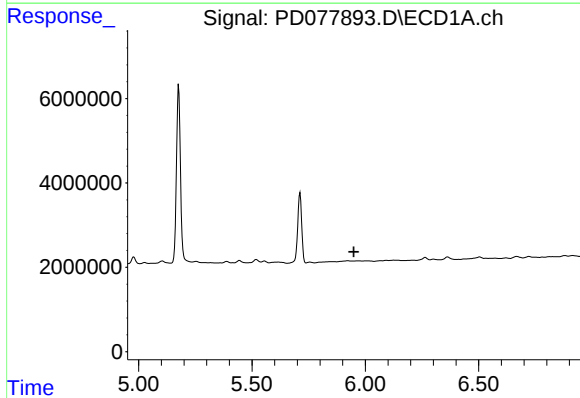


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

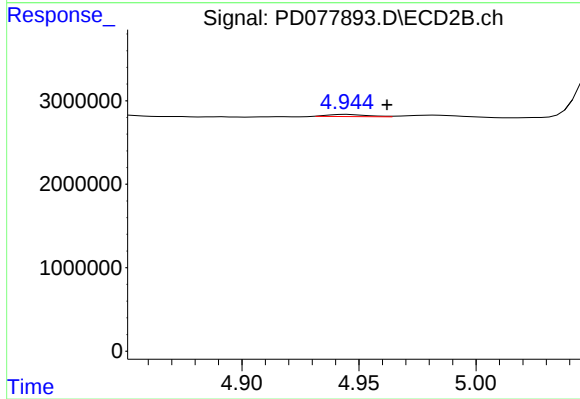


#10 trans-Chlordane

R.T.: 4.945 min
Delta R.T.: -0.017 min
Response: 304462
Conc: 0.15 ng/ml

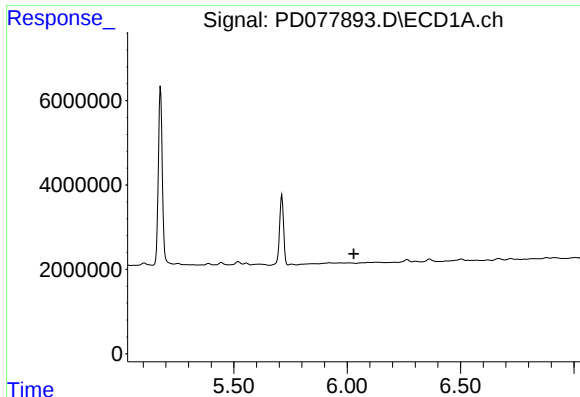


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.029 min
Response: 0
Conc: N.D.

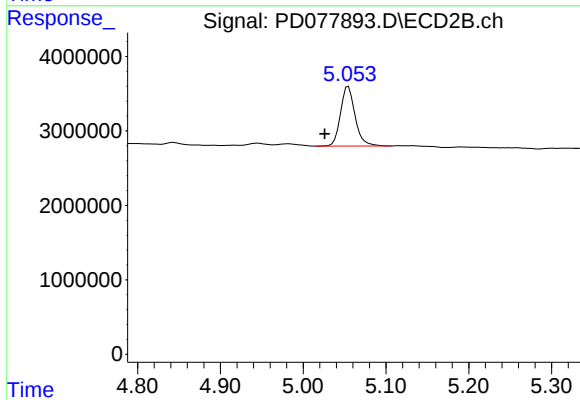


#11 cis-Chlordane

R.T.: 5.055 min
Delta R.T.: 0.029 min
Response: 9801309
Conc: 4.79 ng/ml

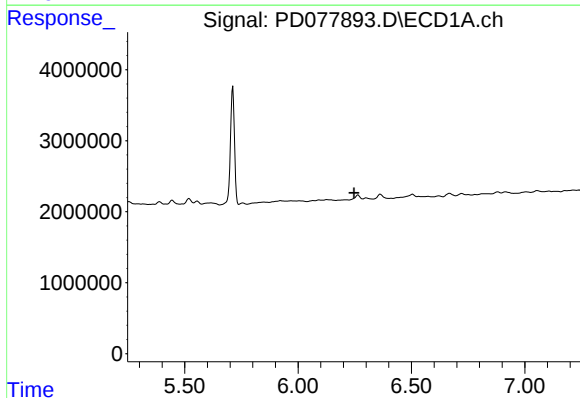


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T. : 6.247 min
Response: 0
Conc: N.D.

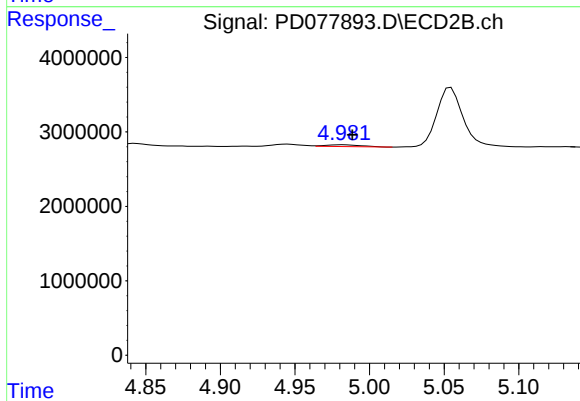


#22 Toxaphene-1

R.T.: 4.982 min
Delta R.T.: -0.006 min
Response: 399575
Conc: 38.28 ng/ml

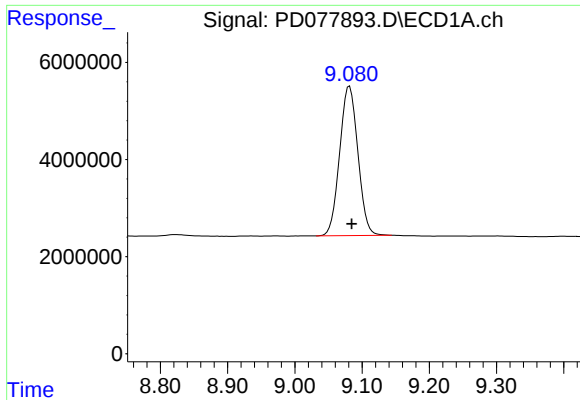

#27 Decachlorobiphenyl

R.T.: 9.081 min
Delta R.T.: -0.003 min
Response: 57831584
Conc: 18.51 ng/ml

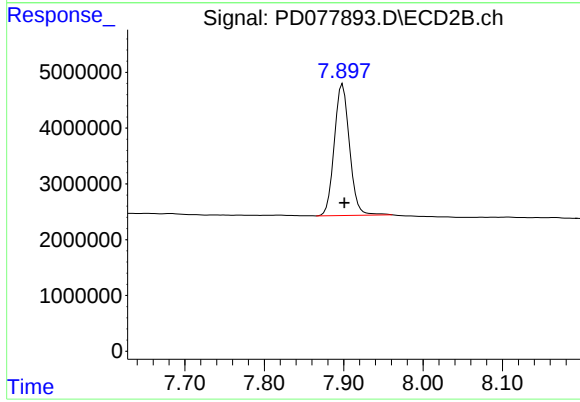

#27 Decachlorobiphenyl

R.T.: 7.899 min
Delta R.T.: -0.002 min
Response: 31442667
Conc: 19.41 ng/ml