

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD091224\  
Data File : PIBLK114.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 12 Sep 2024 19:08  
Operator : AR\AJ  
Sample : PIBLK114  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 13 01:59:05 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm


| Compound                    | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml    |
|-----------------------------|--------|-------|----------|----------|--------|----------|
| -----                       |        |       |          |          |        |          |
| System Monitoring Compounds |        |       |          |          |        |          |
| 1) SA Tetrachlo...          | 3.537  | 2.904 | 15965353 | 80068441 | 15.785 | 22.626 # |
| 2) SA Decachlor...          | 9.033  | 8.105 | 30431116 | 75997281 | 23.300 | 21.856   |
| Target Compounds            |        |       |          |          |        |          |
| 12) B 4,4'-DDE              | 6.218f | 0.000 | 1185557  | 0        | 0.950  | N.D. #   |
| -----                       |        |       |          |          |        |          |


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD091224\  
Data File : PIBLK114.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 12 Sep 2024 19:08  
Operator : AR\AJ  
Sample : PIBLK114  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 13 01:59:05 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

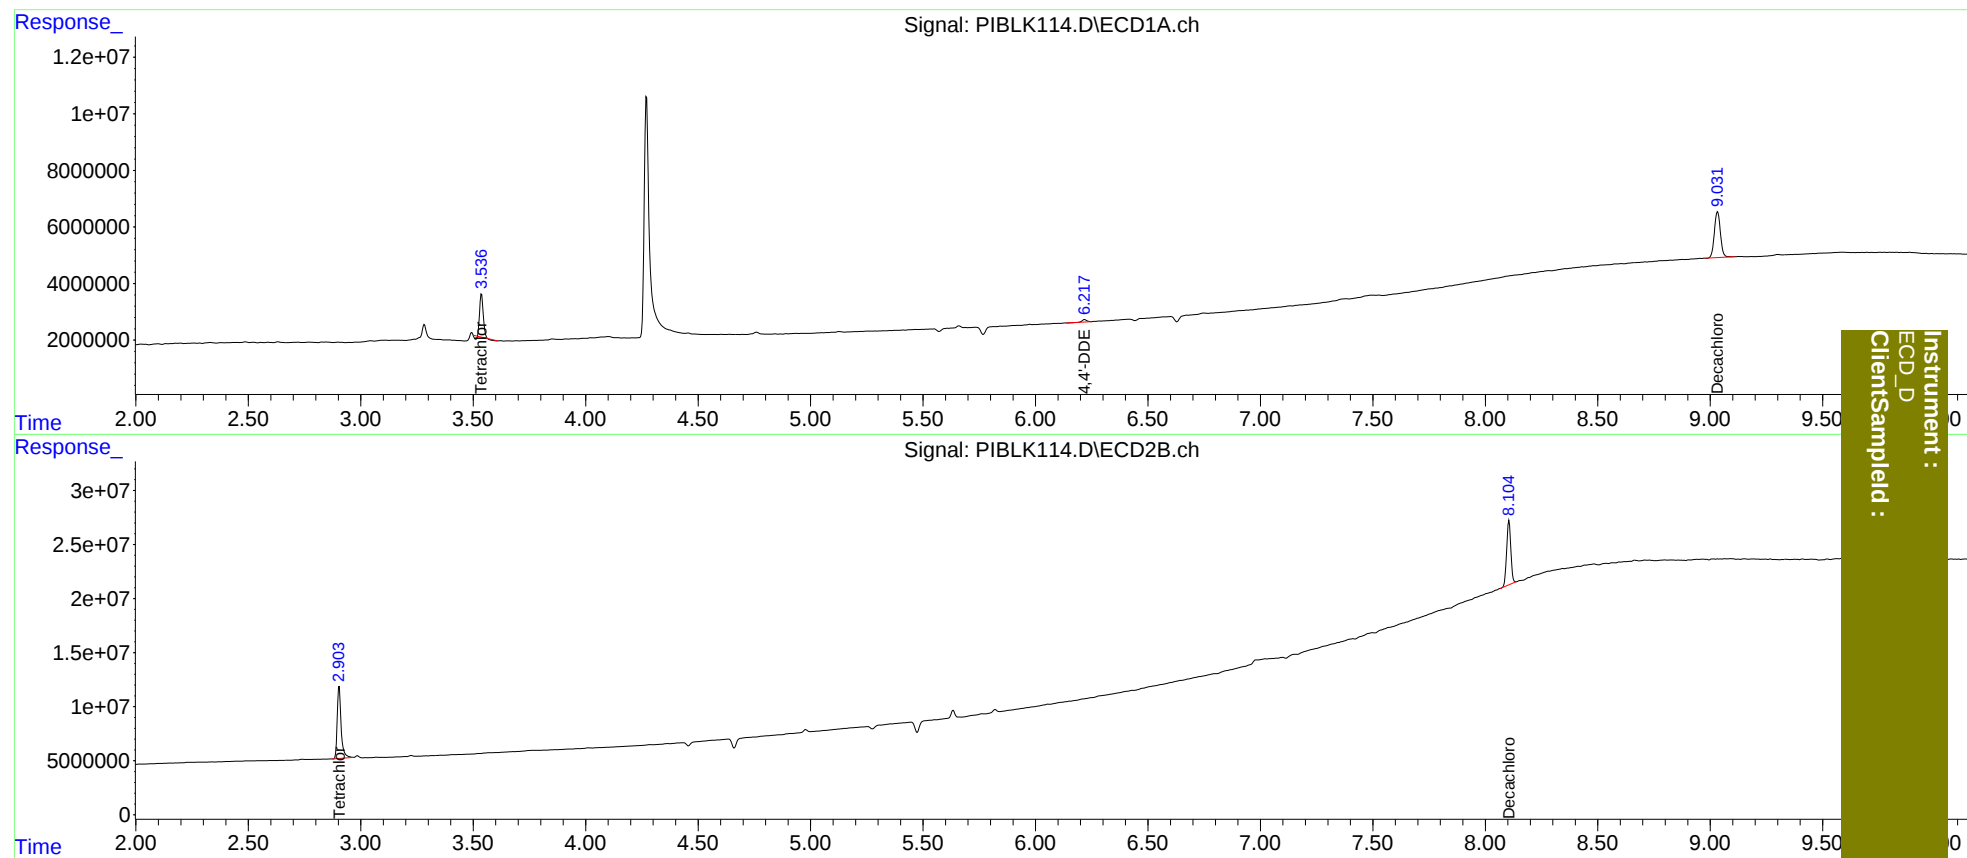


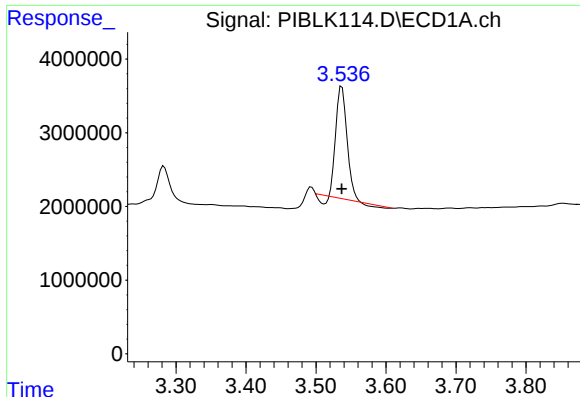

#1 Tetrachloro-m-xylene


R.T.: 3.537 min  
Delta R.T.: 0.000 min  
Response: 15965353  
Conc: 15.79 ng/ml

Instrument :  
ECD\_D  
ClientSampleId :

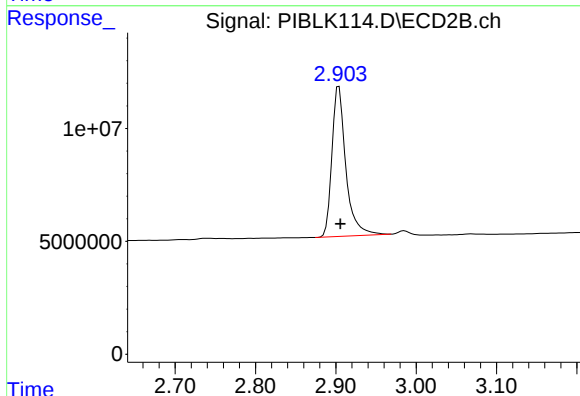


#1 Tetrachloro-m-xylene

R.T.: 2.904 min  
Delta R.T.: -0.002 min  
Response: 80068441  
Conc: 22.63 ng/ml

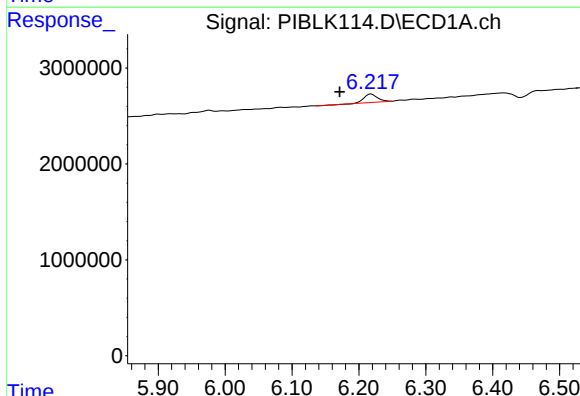


#12 4,4'-DDE

R.T.: 6.218 min  
Delta R.T.: 0.047 min  
Response: 1185557  
Conc: 0.95 ng/ml

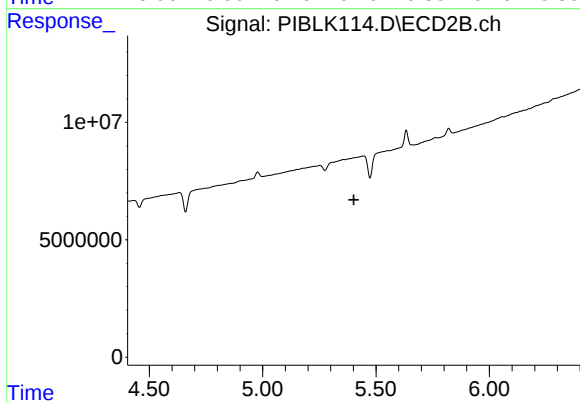

#12 4,4'-DDE


R.T.: 0.000 min  
Exp R.T.: 5.402 min  
Response: 0  
Conc: N.D.

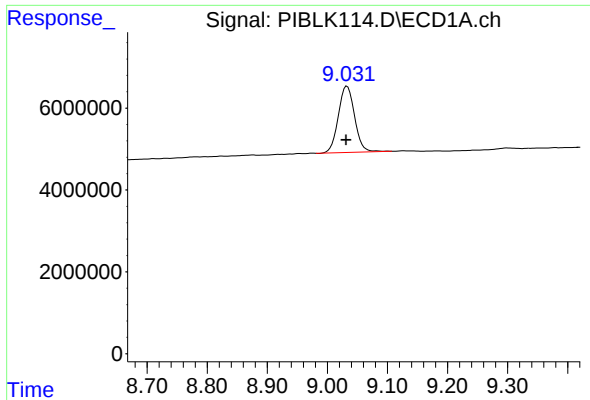

#27 Decachlorobiphenyl

R.T.: 9.033 min  
Delta R.T.: 0.001 min  
Response: 30431116  
Conc: 23.30 ng/ml

Instrument :  
ECD\_D  
ClientSampleId :

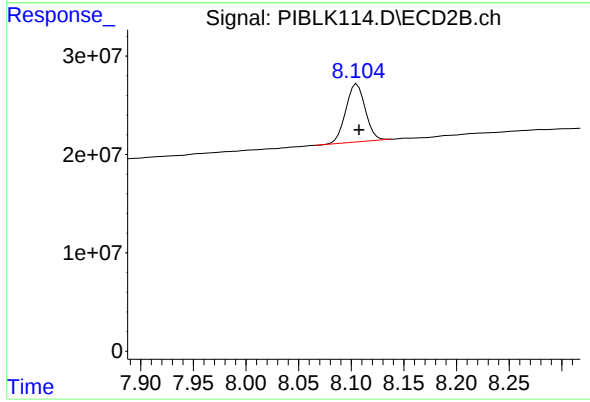

#27 Decachlorobiphenyl

R.T.: 8.105 min  
Delta R.T.: -0.002 min  
Response: 75997281  
Conc: 21.86 ng/ml