

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091224\
 Data File : PD085046.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2024 14:05
 Operator : AR\AJ
 Sample : P3878-21MS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDCC3MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/15/2024
 Supervised By :Ankita Jodhani 09/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 01:50:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.527	2.916	19360546	2754.3E6	19.142m	778.307m#
2) SA Decachlor...	9.033	8.105	12105937	24866714	9.269	7.151
Target Compounds						
2) A alpha-BHC	3.983	3.415	182.1E6	412.6E6	107.137	81.379
3) MA gamma-BHC...	4.258f	3.750	47949.0E6	418.9E6	29637.379m	86.443 #
4) MA Heptachlor	4.909	4.099	80375485	253.0E6	52.239	59.432m
5) MB Aldrin	5.251	4.388	85009309	148.9E6	53.152	33.523 #
6) B beta-BHC	4.492	4.043	49340747	106.4E6	67.928m	49.088 #
7) B delta-BHC	4.741	4.281	227.8E6	527.9E6	138.879m	106.345
8) B Heptachlo...	5.670	4.894	78350618	217.0E6	52.533	51.224
9) A Endosulfan I	6.051	5.270	83560787	190.7E6	60.736m	49.735m
10) B trans-Chl...	5.923	5.147	80514918	216.5E6	57.088	52.636m
11) B cis-Chlor...	6.003	5.214	81590435	205.8E6	55.182m	49.042
12) B 4,4'-DDE	6.173	5.398	149.5E6	384.4E6	119.818	97.993
13) MA Dieldrin	6.324	5.538	159.6E6	416.6E6	108.211	96.970
14) MA Endrin	6.550	5.814	152.5E6	415.0E6	135.170m	112.087m
15) B Endosulfa...	6.760	6.107	125.2E6	326.8E6	94.844m	88.132
16) A 4,4'-DDD	6.680	5.956	134.9E6	389.2E6	136.582m	114.691
17) MA 4,4'-DDT	6.996	6.211	112.7E6	354.7E6	125.946m	110.867
18) B Endrin al...	6.890	6.287	130.1E6	265.6E6	144.047m	93.012 #
19) B Endosulfa...	7.124	6.511	155.4E6	326.5E6	134.872	91.414 #
20) A Methoxychlor	7.467	6.782	456.5E6	781.4E6	876.286m	472.327m#
21) B Endrin ke...	7.604	7.022	143.9E6	397.2E6	117.733	90.199

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091224\
Data File : PD085046.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2024 14:05
Operator : AR\AJ
Sample : P3878-21MS
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 01:50:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

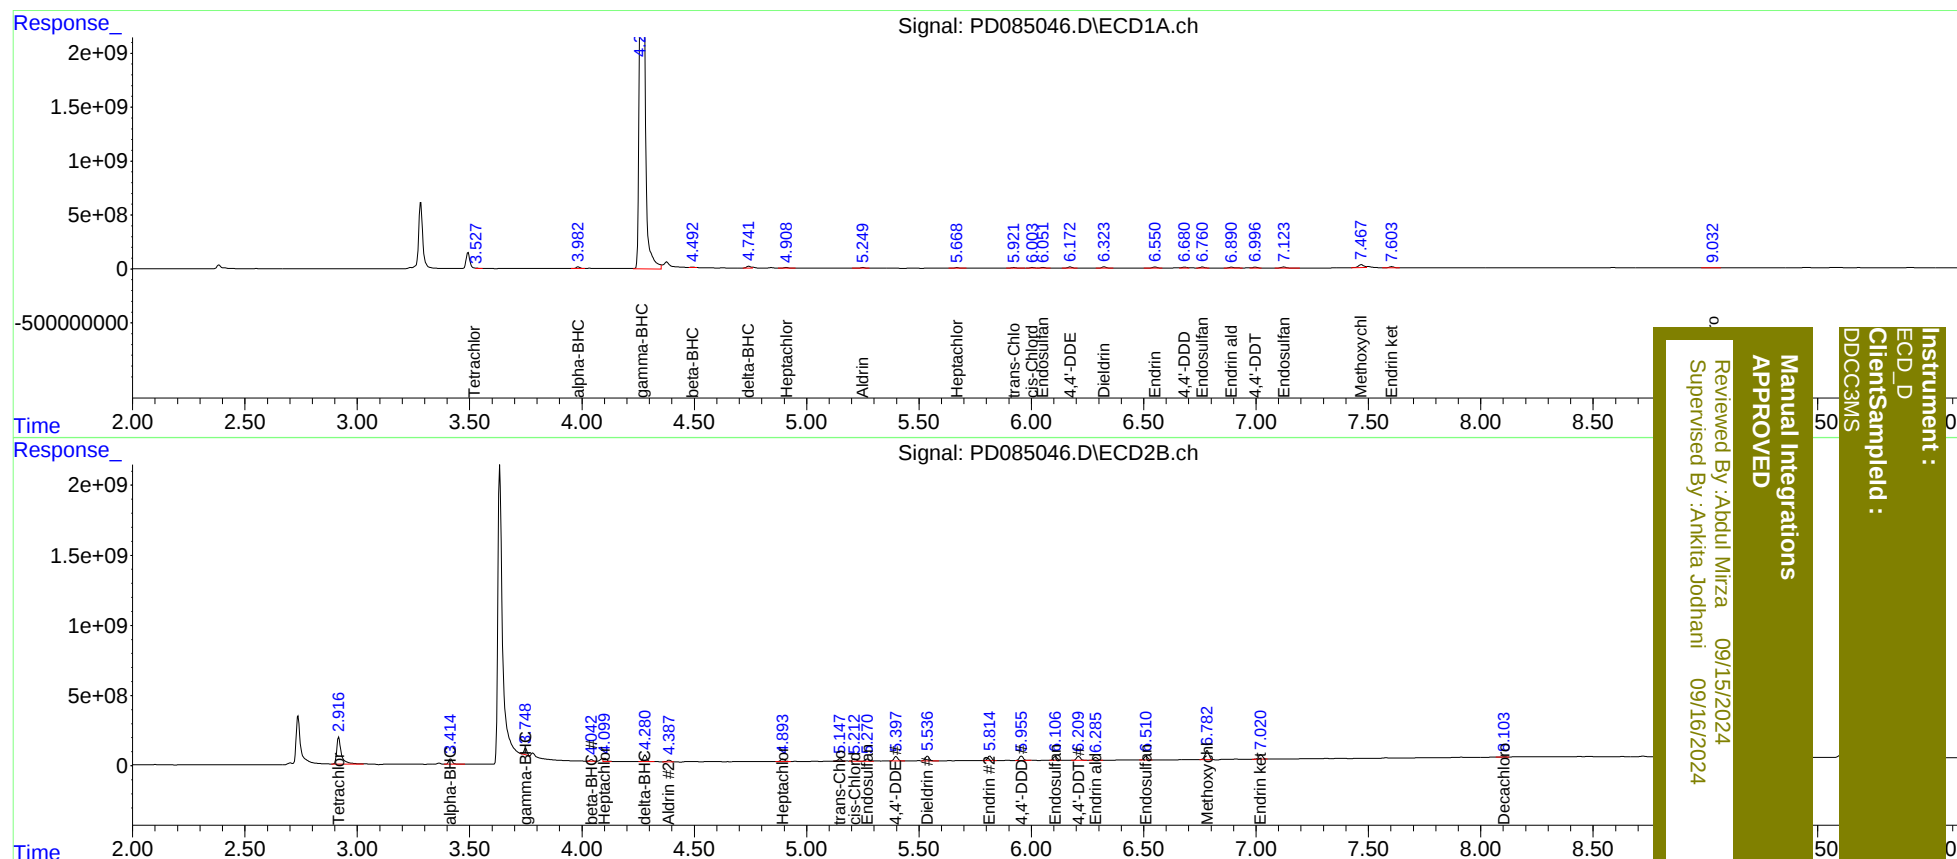

Reviewed By: Abdul Mirza 09/15/2024
Supervised By: Ankita Jodhani 09/16/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
DDCCMS