

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091224\
 Data File : PD085047.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2024 14:18
 Operator : AR\AJ
 Sample : P3878-22MSD
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :

ECD_D

ClientSampleId :

DDCC3MSD

Manual Integrations**APPROVED**

Reviewed By :Abdul Mirza 09/15/2024

Supervised By :Ankita Jodhani 09/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 01:50:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.527	2.916	28234802	2683.4E6	27.916m	758.277m#
27)	SA Decachlor...	9.035	8.105	12268150	25881959	9.393	7.443
Target Compounds							
2)	A alpha-BHC	3.983	3.415	179.8E6	413.4E6	105.783	81.543
3)	MA gamma-BHC...	4.259f	3.749	47781.5E6	404.5E6	29533.838m	83.471 #
4)	MA Heptachlor	4.909	4.097	79108985	245.7E6	51.416	57.708m
5)	MB Aldrin	5.250	4.388	83921389	131.1E6	52.472	29.525 #
6)	B beta-BHC	4.492	4.043	63136919	103.1E6	86.921m	47.553 #
7)	B delta-BHC	4.741	4.281	212.4E6	539.8E6	129.504m	108.742
8)	B Heptachlo...	5.669	4.895	77394886	218.4E6	51.892	51.564
9)	A Endosulfan I	6.051	5.270	78493508	175.2E6	57.053m	45.698m
10)	B trans-Chl...	5.923	5.147	80395252	216.8E6	57.003	52.709m
11)	B cis-Chlor...	6.003	5.214	79515350	205.6E6	53.779m	49.005
12)	B 4,4'-DDE	6.173	5.399	146.2E6	384.4E6	117.190	98.008
13)	MA Dieldrin	6.325	5.538	158.3E6	413.5E6	107.283	96.256
14)	MA Endrin	6.550	5.814	148.6E6	415.2E6	131.676m	112.138m
15)	B Endosulfa...	6.761	6.107	124.8E6	327.6E6	94.509m	88.363
16)	A 4,4'-DDD	6.680	5.956	145.9E6	380.7E6	147.798m	112.172
17)	MA 4,4'-DDT	6.996	6.209	112.3E6	360.3E6	125.414m	112.623m
18)	B Endrin al...	6.890	6.286	128.5E6	263.3E6	142.326m	92.229 #
19)	B Endosulfa...	7.125	6.511	151.2E6	329.4E6	131.208	92.228 #
20)	A Methoxychlor	7.467	6.782	499.9E6	772.6E6	959.581m	467.030m#
21)	B Endrin ke...	7.604	7.022	144.0E6	390.7E6	117.809	88.721

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091224\
Data File : PD085047.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2024 14:18
Operator : AR\AJ
Sample : P3878-22MSD
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 01:50:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

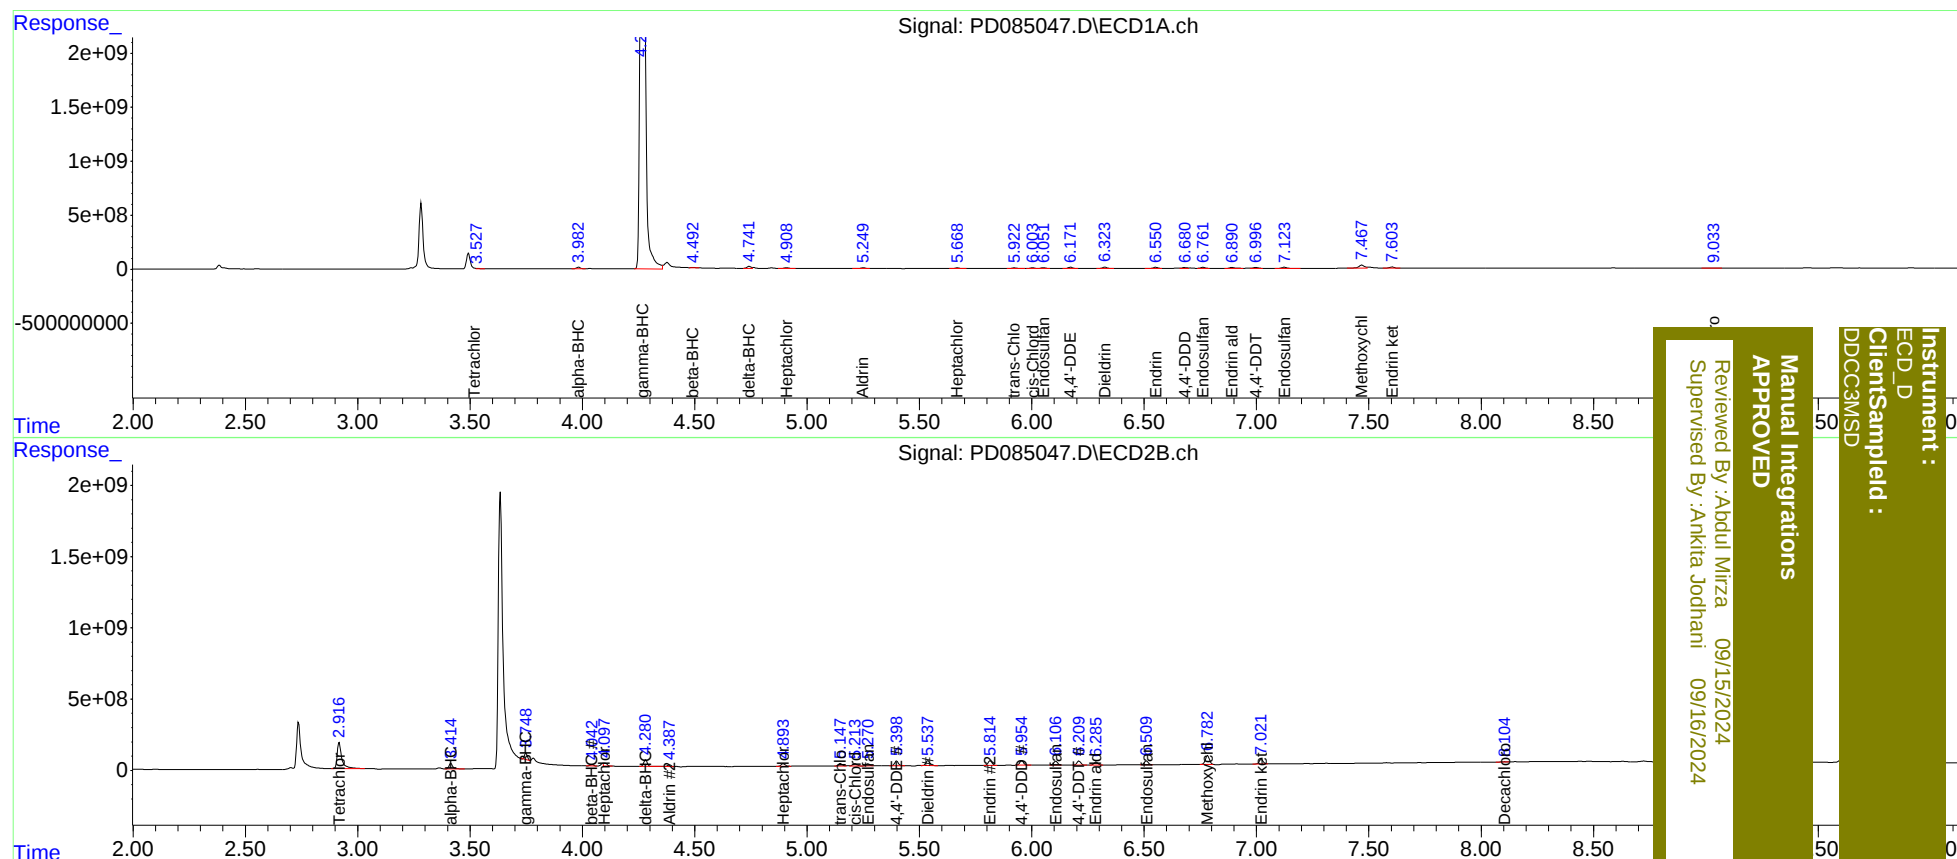

Reviewed By: Abdul Mirza 09/15/2024
Supervised By: Ankita Jodhani 09/16/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
DDCCMSD