

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091224\
 Data File : PD085039.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2024 12:31
 Operator : AR\AJ
 Sample : P3878-14RE
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDC03RE

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/15/2024
 Supervised By : Ankita Jodhani 09/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 01:47:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.535	2.915	11267322	83069222	11.140m	23.474m#
2) SA Decachlor...	9.033	8.104	15423351	29528409	11.809	8.492 #
Target Compounds						
2) A alpha-BHC	3.983	3.414	12197095	31758823	7.174	6.264
7) B delta-BHC	4.742	4.279	16199621	56479164	9.878m	11.377m
13) MA Dieldrin	6.323	5.538	6510944	9943539	4.414m	2.315m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091224\
Data File : PD085039.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2024 12:31
Operator : AR\AJ
Sample : P3878-14RE
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 01:47:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

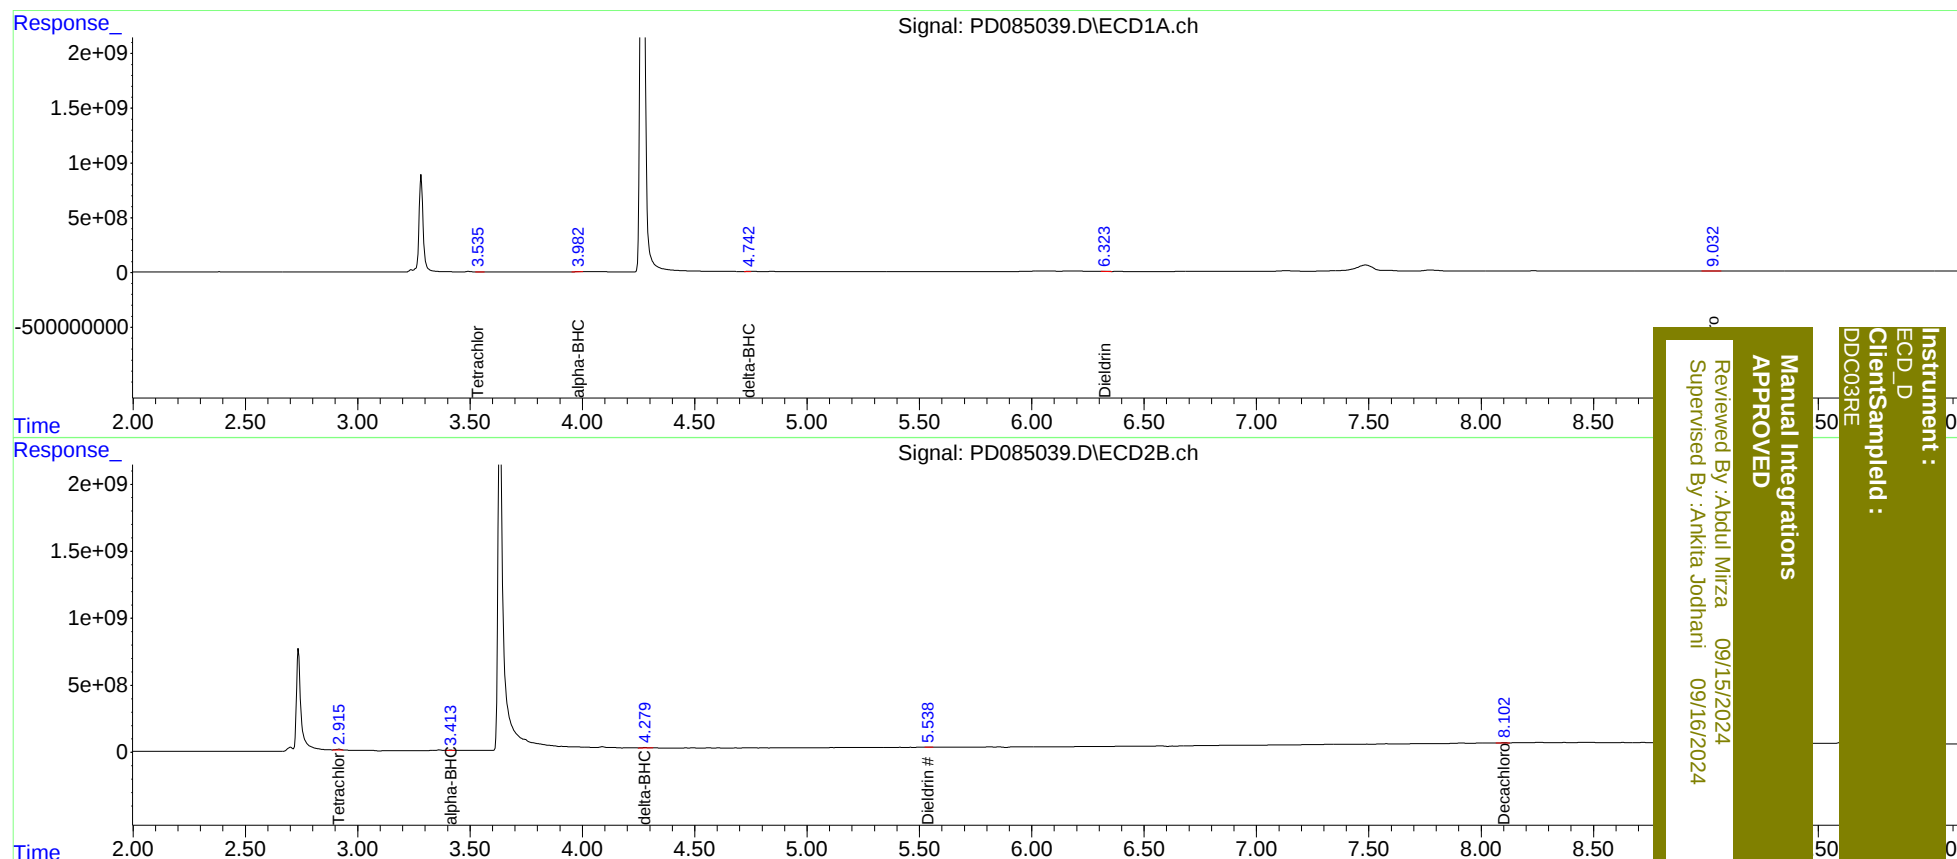

Reviewed By: Abdul Mirza 09/15/2024
Supervised By: Ankita Jodhani 09/16/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
DDC03RE