

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091319\
Data File : PD054570.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Sep 2019 16:46
Operator : SG\AJ
Sample : K4731-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0AF6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 23:12:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090419CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 05 08:40:10 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.301	3.972	9234604	12784992	13.066	12.954
27)	SA Decachlor...	7.988	9.007	12629509	15522542	18.662	16.593

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091319\
Data File : PD054570.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Sep 2019 16:46
Operator : SG\AJ
Sample : K4731-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0AF6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 23:12:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090419CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 05 08:40:10 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

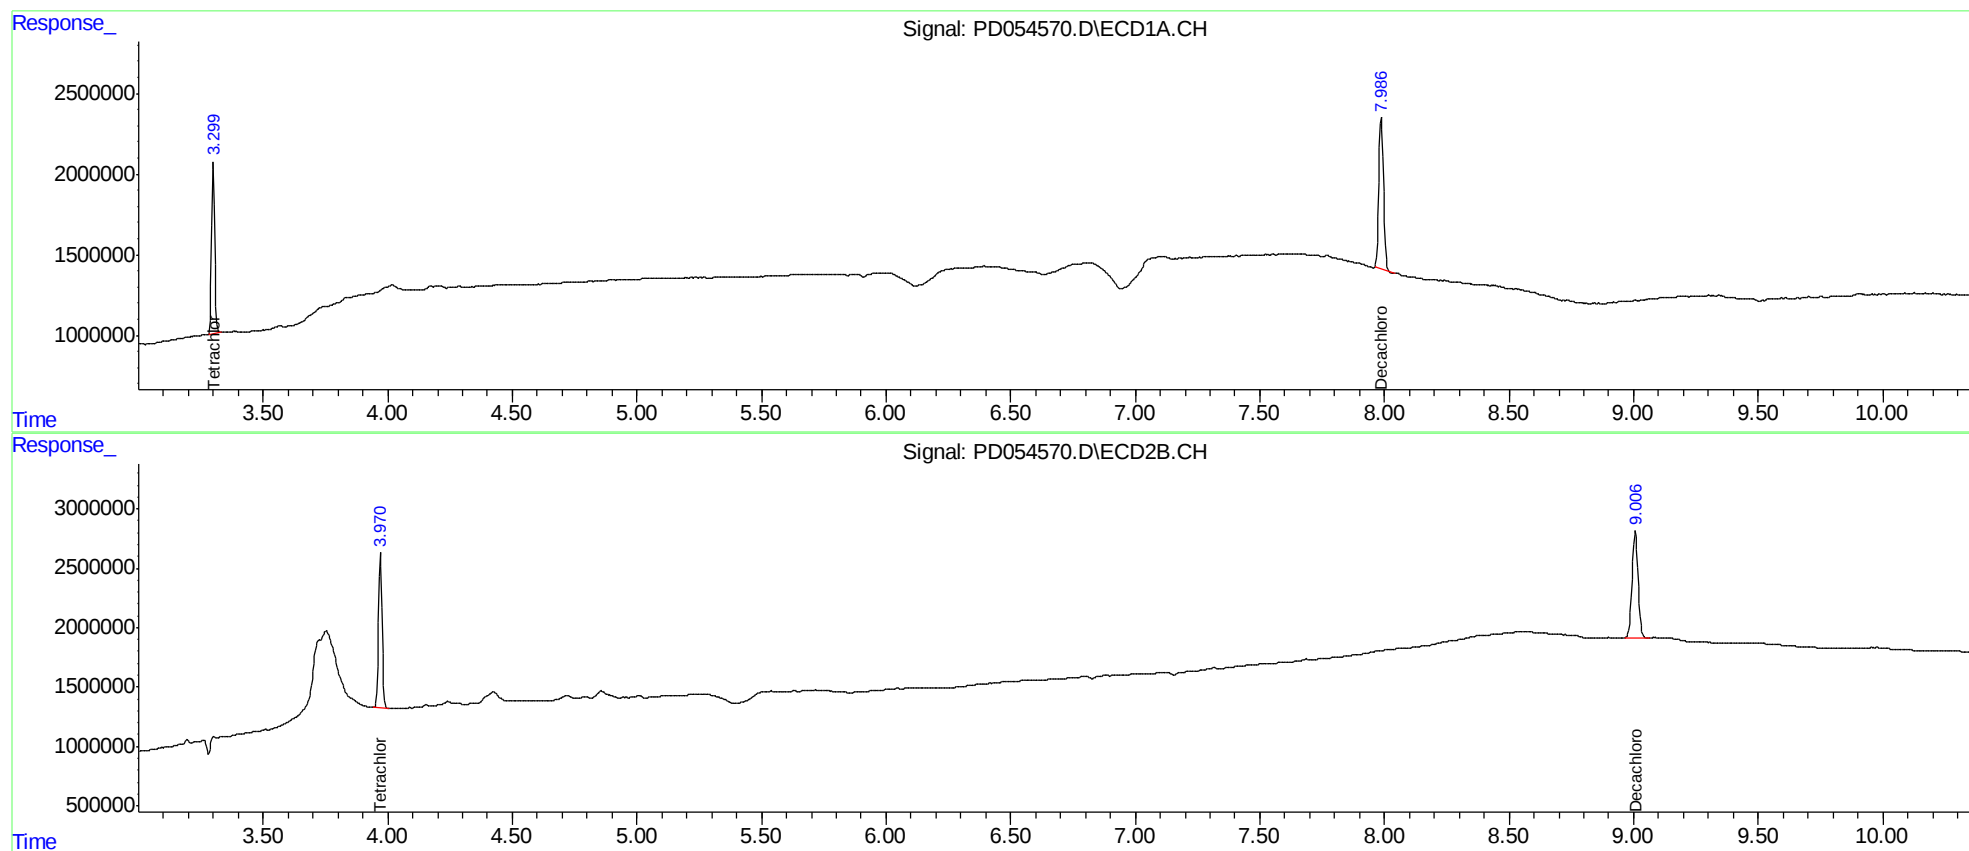


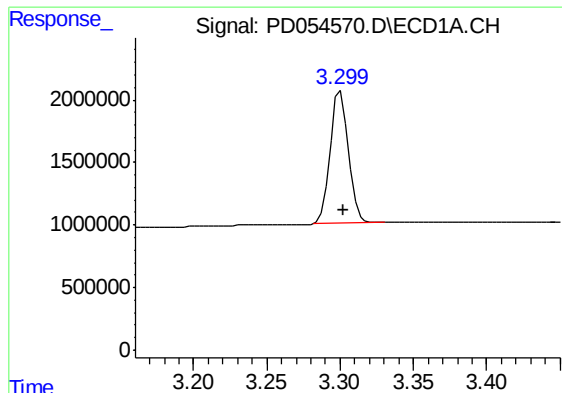

#1 Tetrachloro-m-xylene


R.T.: 3.301 min
Delta R.T.: -0.001 min
Response: 9234604
Conc: 13.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AF6

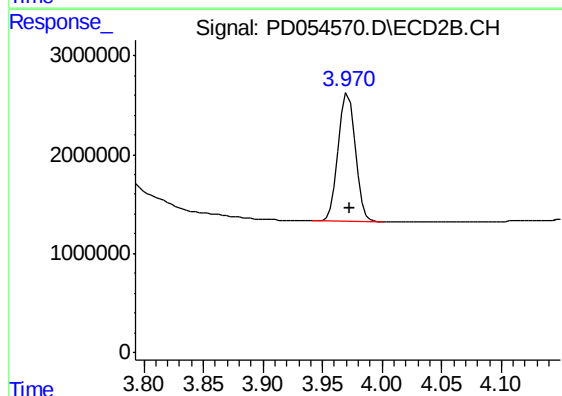


#1 Tetrachloro-m-xylene

R.T.: 3.972 min
Delta R.T.: -0.001 min
Response: 12784992
Conc: 12.95 ng/ml

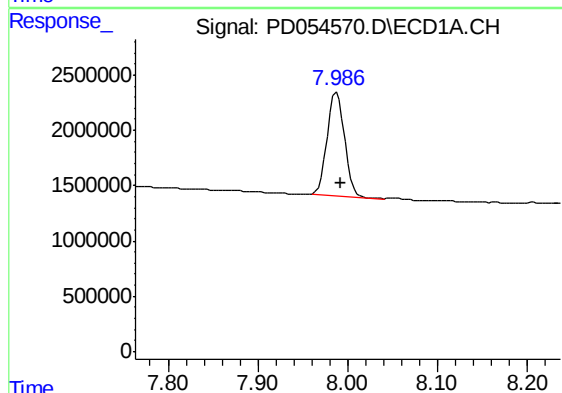

#27 Decachlorobiphenyl

R.T.: 7.988 min
Delta R.T.: -0.005 min
Response: 12629509
Conc: 18.66 ng/ml

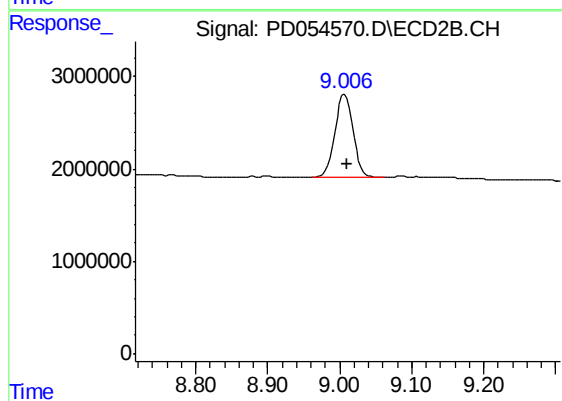

#27 Decachlorobiphenyl

R.T.: 9.007 min
Delta R.T.: -0.003 min
Response: 15522542
Conc: 16.59 ng/ml