

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091319\
 Data File : PD054577.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Sep 2019 19:47
 Operator : SG\AJ
 Sample : K4731-22
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AH8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 23:13:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090419CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 05 08:40:10 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.302	3.972	10753319	14516465	15.215	14.709
27)	SA Decachlor...	7.988	9.008	18665960	23192989	27.582	24.792
Target Compounds							
10)	B trans-Chl...	0.000	6.051	0	2839058	N.D.	2.056
13)	MA Dieldrin	0.000	6.472	0	1315036	N.D.	0.976
16)	A 4,4'-DDD	0.000	6.778	0	2366512	N.D.	2.221


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091319\
Data File : PD054577.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Sep 2019 19:47
Operator : SG\AJ
Sample : K4731-22
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0AH8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 23:13:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090419CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 05 08:40:10 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

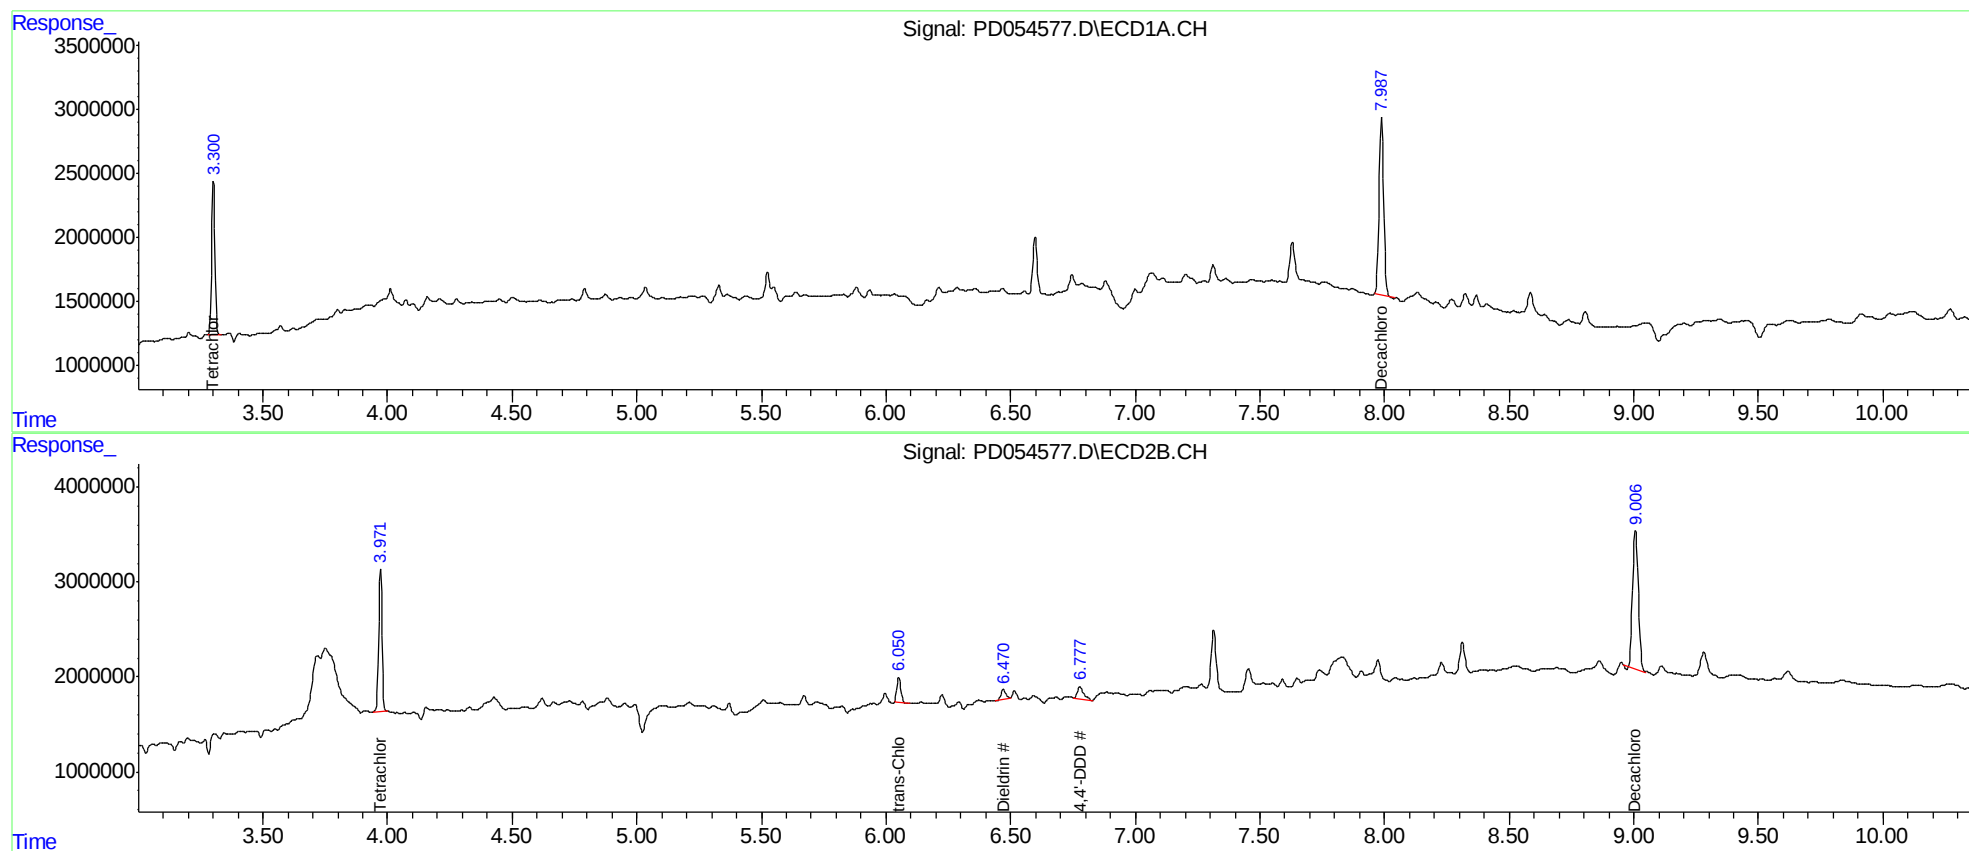


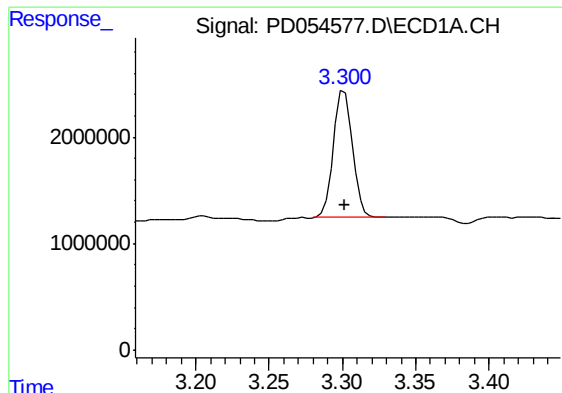

#1 Tetrachloro-m-xylene


R.T.: 3.302 min
Delta R.T.: 0.000 min
Response: 10753319
Conc: 15.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AH8

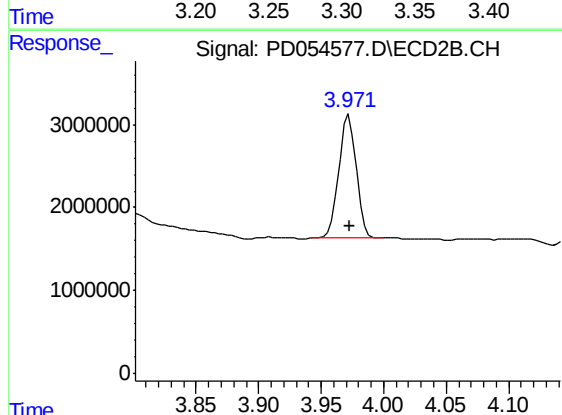


#1 Tetrachloro-m-xylene

R.T.: 3.972 min
Delta R.T.: 0.000 min
Response: 14516465
Conc: 14.71 ng/ml

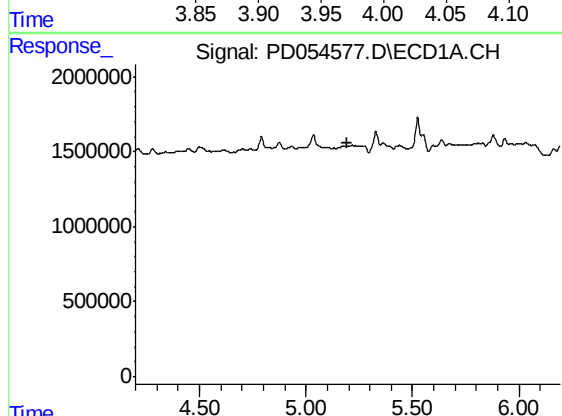


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.197 min
Response: 0
Conc: N.D.

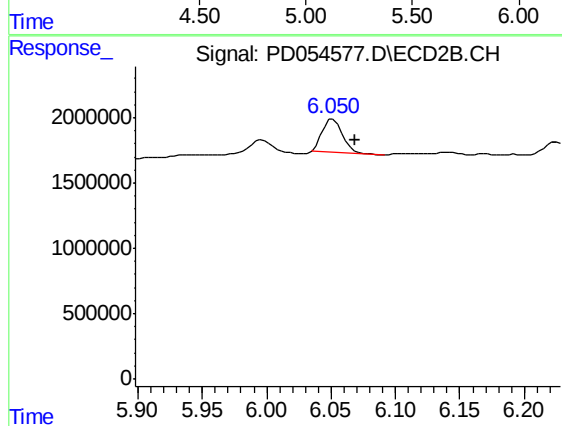

#10 trans-Chlordane


R.T.: 6.051 min
Delta R.T.: -0.017 min
Response: 2839058
Conc: 2.06 ng/ml

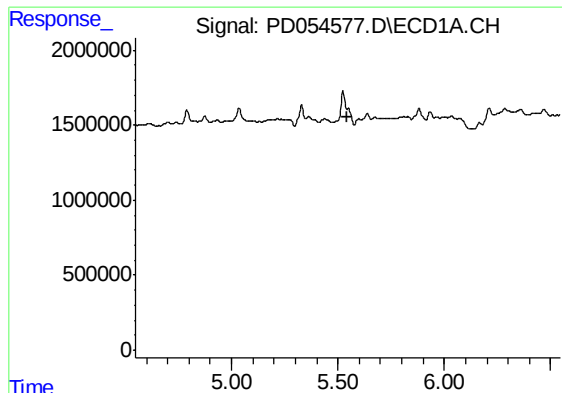

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.547 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0AH8

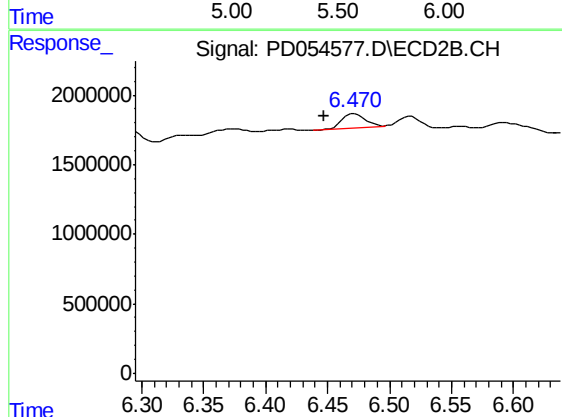


#13 Dieldrin

R.T.: 6.472 min
Delta R.T.: 0.024 min
Response: 1315036
Conc: 0.98 ng/ml

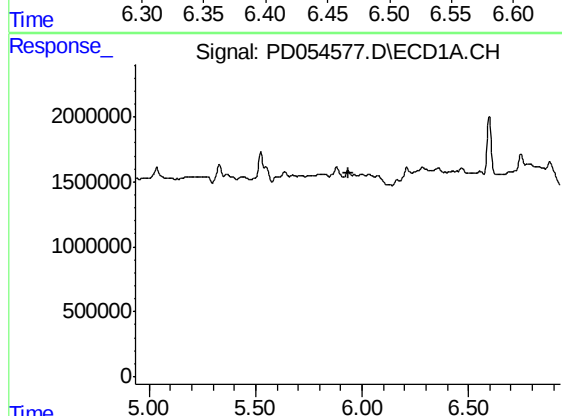


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.935 min
Response: 0
Conc: N.D.

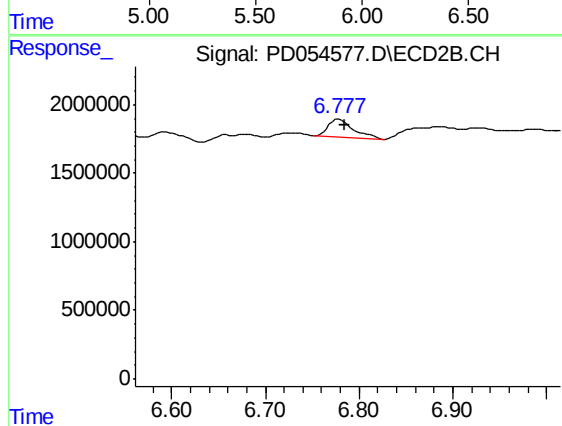

#16 4,4'-DDD


R.T.: 6.778 min
Delta R.T.: -0.007 min
Response: 2366512
Conc: 2.22 ng/ml

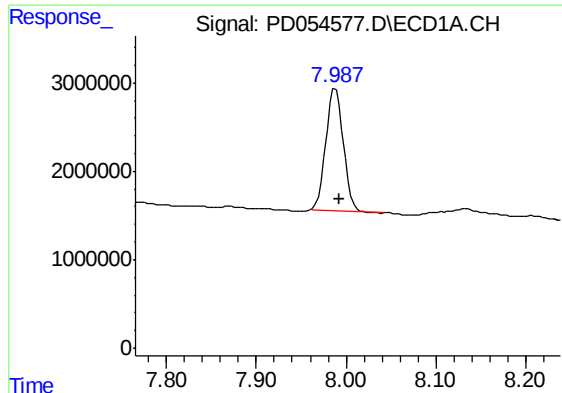

#27 Decachlorobiphenyl

R.T.: 7.988 min
Delta R.T.: -0.005 min
Response: 18665960
Conc: 27.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AH8

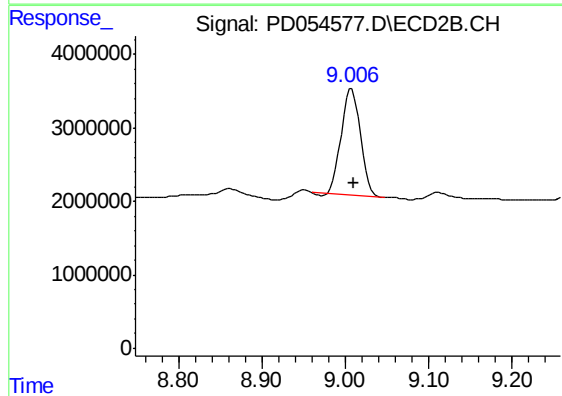

#27 Decachlorobiphenyl

R.T.: 9.008 min
Delta R.T.: -0.002 min
Response: 23192989
Conc: 24.79 ng/ml